

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101818\
Data File : FF002426.D
Signal(s) : FID2B.ch
Acq On : 18 Oct 2018 09:47
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 18 23:53:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.652	2486520	17.890 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.717	99761	0.643 ug/ml
14) N-DOTRIACONTANE	18.571	313035	2.019 ug/ml
16) N-HEXATRIACONTANE	20.080	339050	2.472 ug/ml
18) N-TETRACONTANE	21.780	308663	2.591 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101818\
Data File : FF002426.D
Signal(s) : FID2B.ch
Acq On : 18 Oct 2018 09:47
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 18 23:53:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

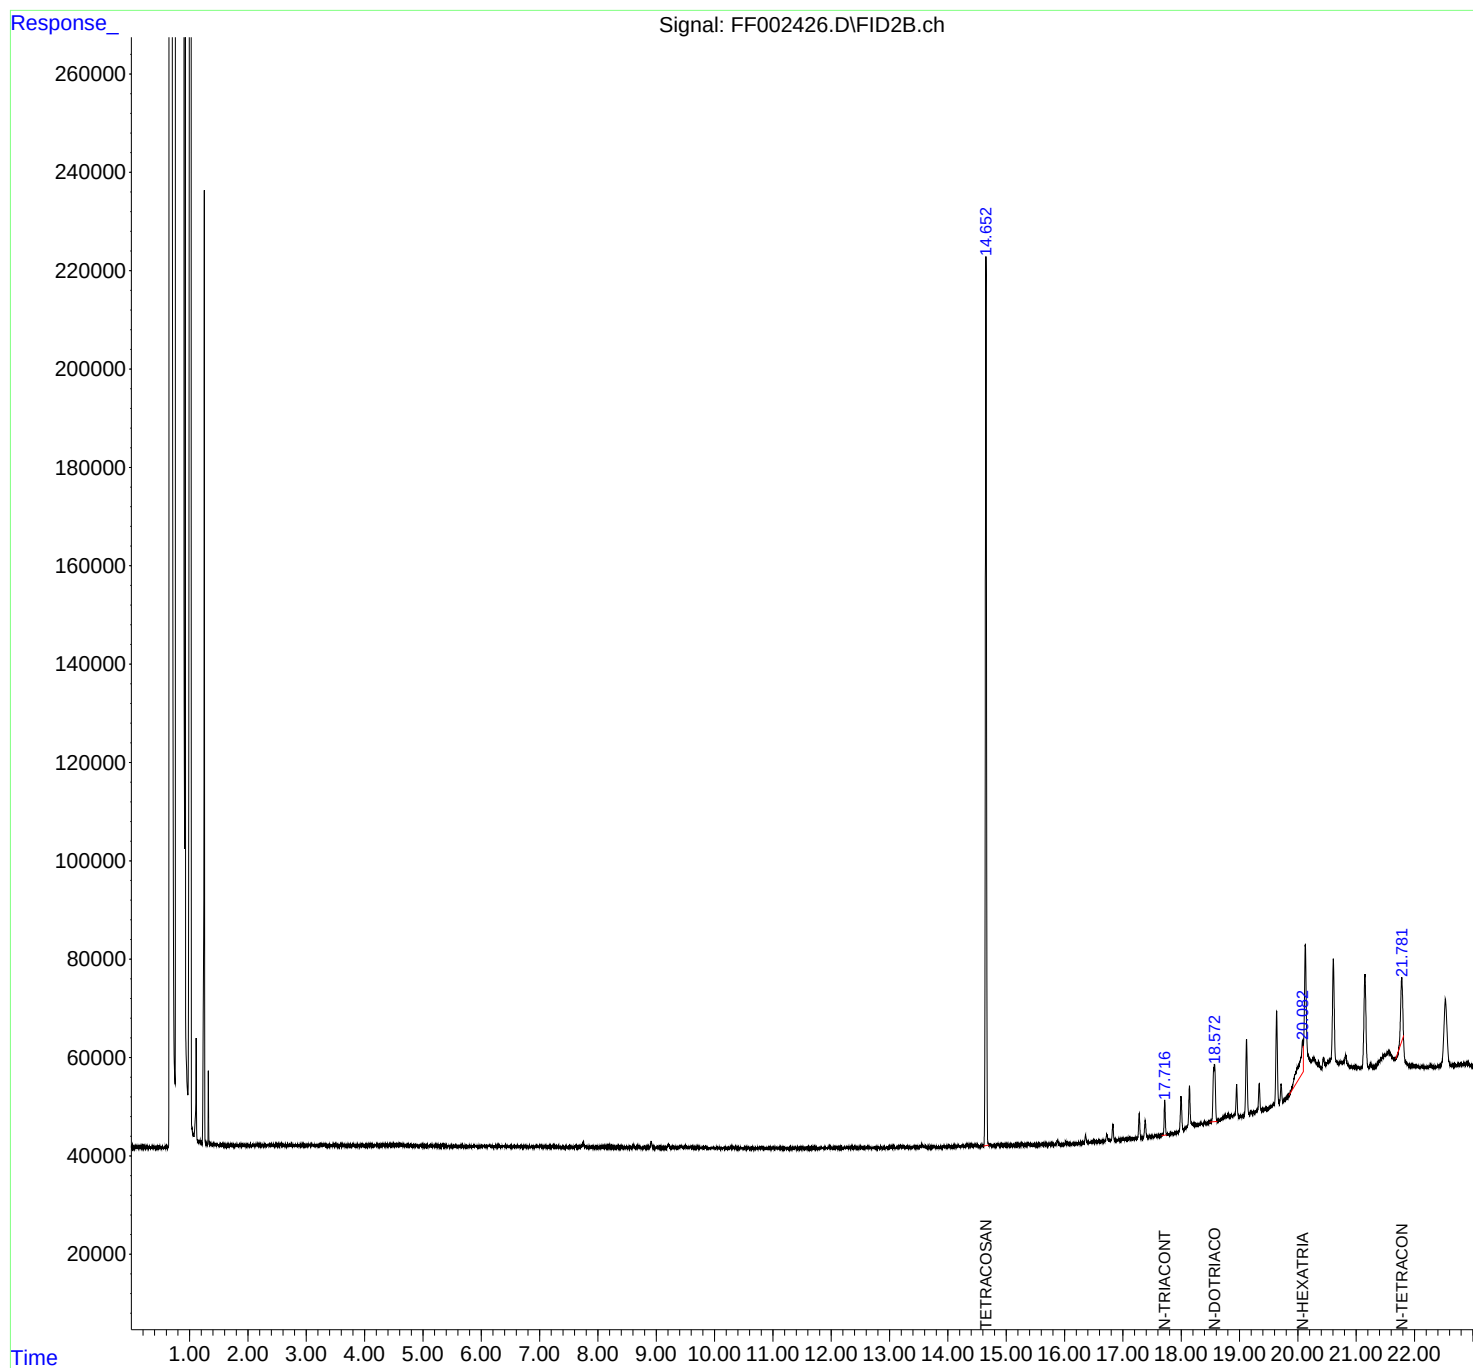

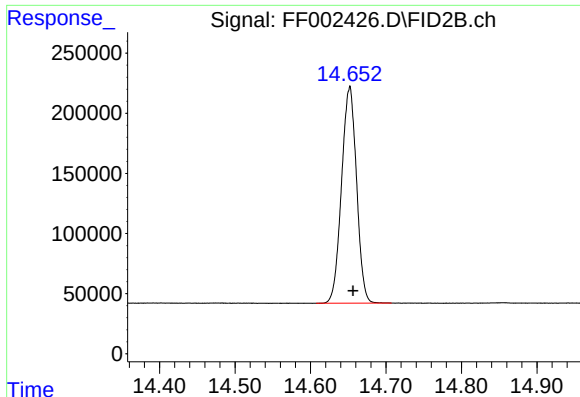


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.652 min
Delta R.T.: -0.004 min
Response: 2486520
Conc: 17.89 ug/ml

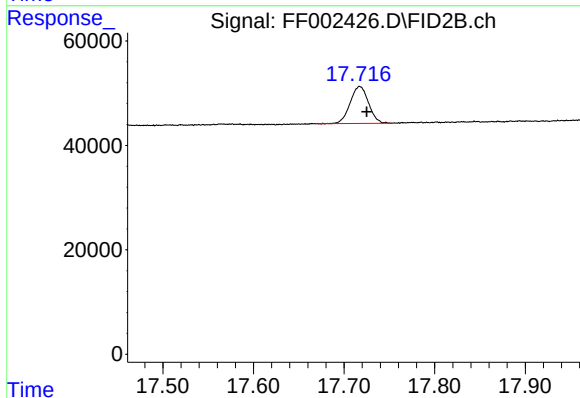


#13 N-TRIACONTANE

R.T.: 17.717 min
Delta R.T.: -0.008 min
Response: 99761
Conc: 0.64 ug/ml

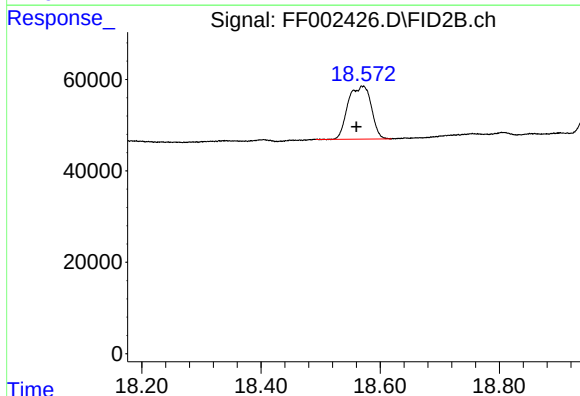


#14 N-DOTRIACONTANE

R.T.: 18.571 min
Delta R.T.: 0.011 min
Response: 313035
Conc: 2.02 ug/ml

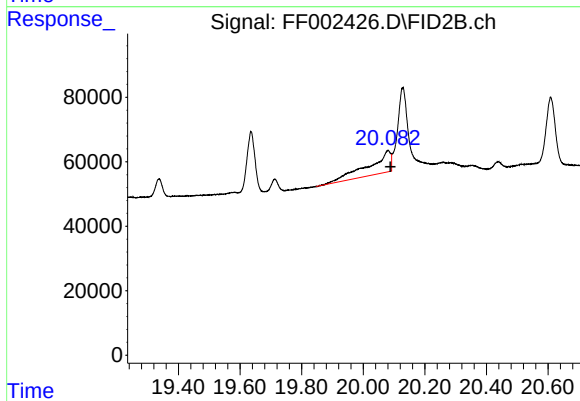

#16 N-HEXATRIACONTANE

R.T.: 20.080 min
Delta R.T.: -0.008 min
Response: 339050
Conc: 2.47 ug/ml

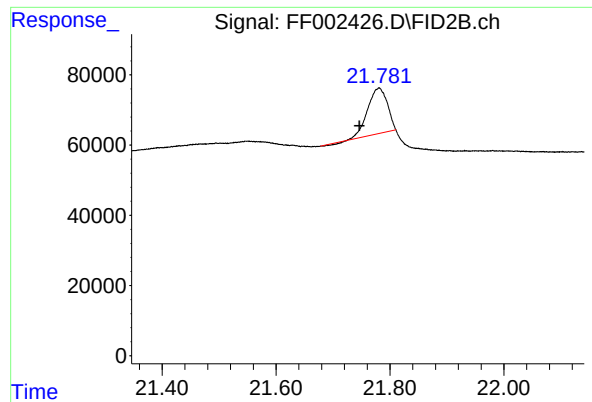

#18 N-TETRACONTANE

R.T.: 21.780 min
Delta R.T.: 0.034 min
Response: 308663
Conc: 2.59 ug/ml