

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101818\
 Data File : FF002433.D
 Signal(s) : FID2B.ch
 Acq On : 18 Oct 2018 16:42
 Operator : AJ\SJ
 Sample : J5204-07 10X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 18 23:54:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
 Quant Title :
 QLast Update : Fri Oct 12 13:21:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.652	340526	2.450 ug/ml
Target Compounds			
4) N-TETRADECANE	8.147	238372	1.523 ug/ml
5) N-HEXADECANE	9.802	208875	1.329 ug/ml
6) N-OCTADECANE	11.307f	190234	1.197 ug/ml
7) N-EICOSANE	12.551	152176	0.961 ug/ml
8) N-DOCOSANE	13.768	308801	1.957 ug/ml
10) N-TETRACOSANE	14.823	1103215	7.051 ug/ml
12) N-OCTACOSANE	16.822	337311	2.175 ug/ml
13) N-TRIACONTANE	17.718	148239	0.955 ug/ml
14) N-DOTRIACONTANE	18.554	134716	0.869 ug/ml
16) N-HEXATRIACONTANE	20.023f	106772	0.778 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101818\
Data File : FF002433.D
Signal(s) : FID2B.ch
Acq On : 18 Oct 2018 16:42
Operator : AJ\SJ
Sample : J5204-07 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 18 23:54:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

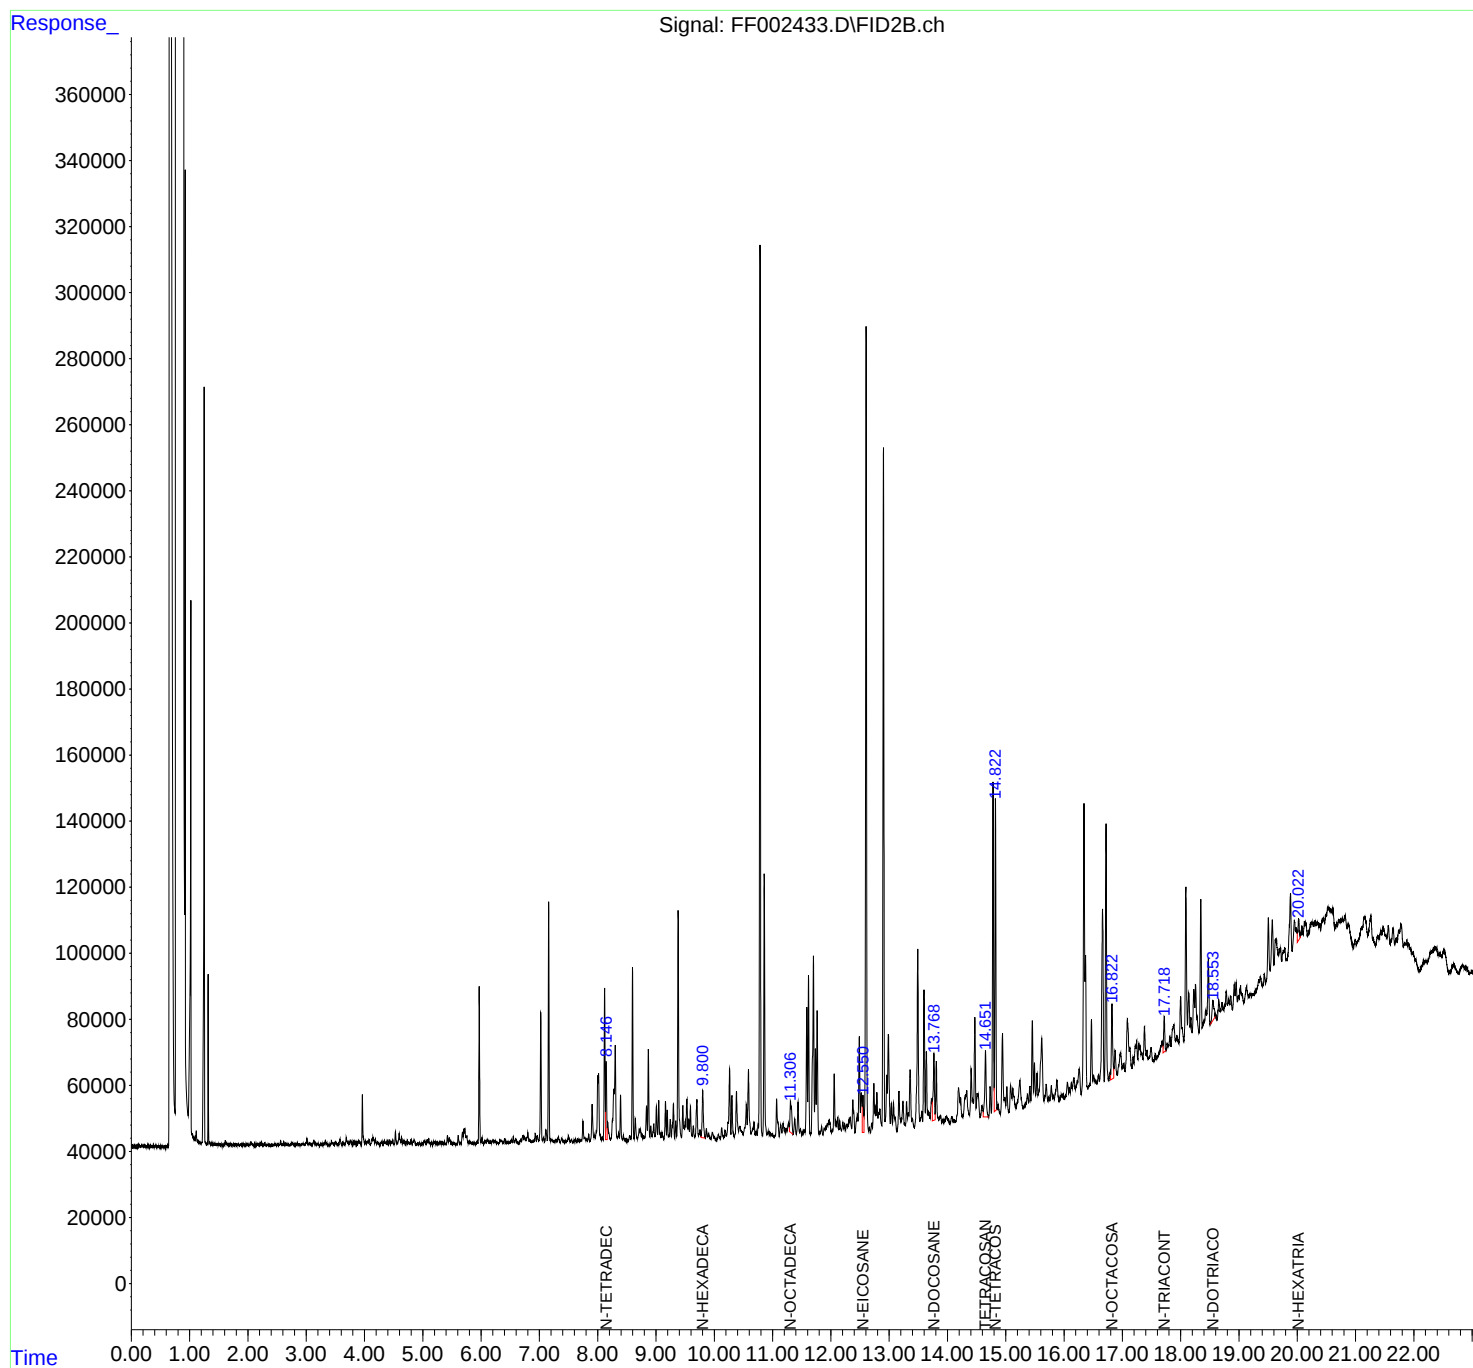

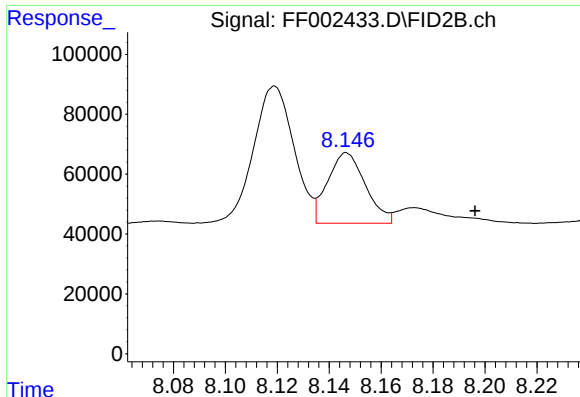


#4 N-TETRADECANE

R.T.: 8.147 min
Delta R.T.: -0.049 min
Response: 238372
Conc: 1.52 ug/ml

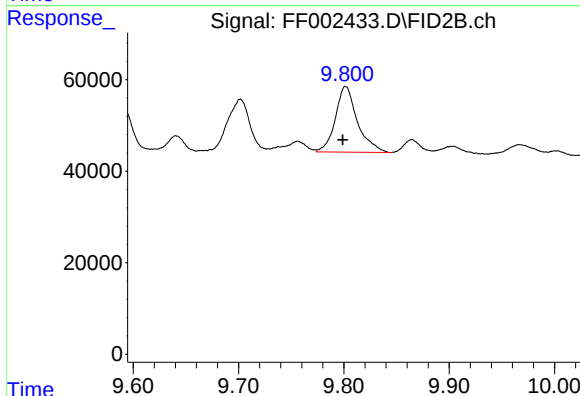


#5 N-HEXADECANE

R.T.: 9.802 min
Delta R.T.: 0.003 min
Response: 208875
Conc: 1.33 ug/ml

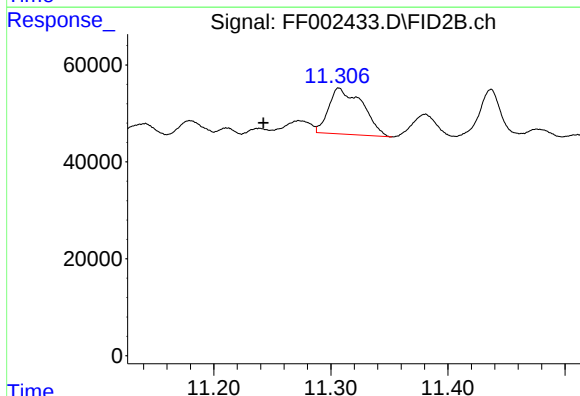


#6 N-OCTADECANE

R.T.: 11.307 min
Delta R.T.: 0.065 min
Response: 190234
Conc: 1.20 ug/ml

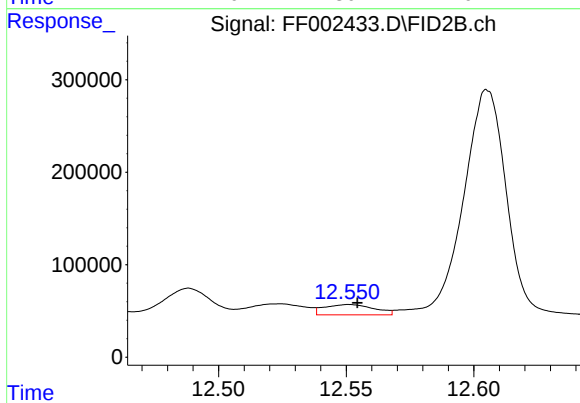


#7 N-EICOSANE

R.T.: 12.551 min
Delta R.T.: -0.003 min
Response: 152176
Conc: 0.96 ug/ml

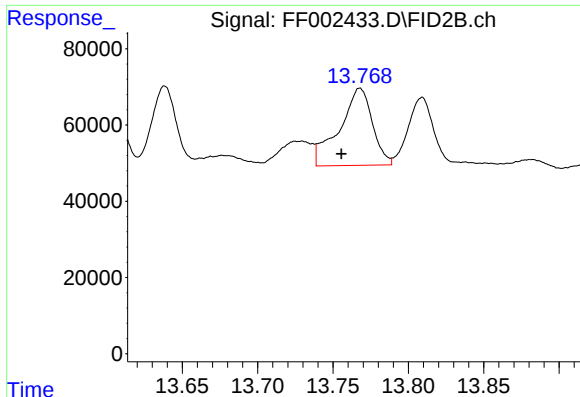


#8 N-DOCOSANE

R.T.: 13.768 min
Delta R.T.: 0.012 min
Response: 308801
Conc: 1.96 ug/ml

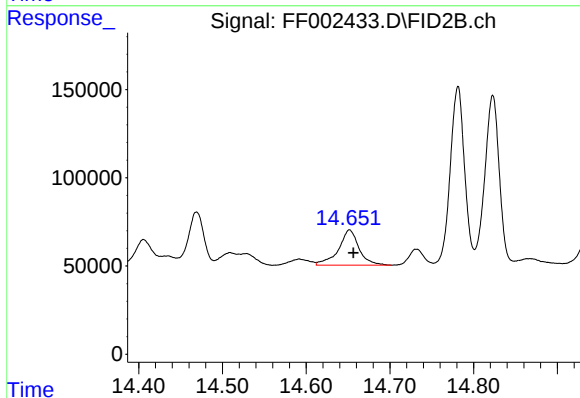


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.652 min
Delta R.T.: -0.005 min
Response: 340526
Conc: 2.45 ug/ml

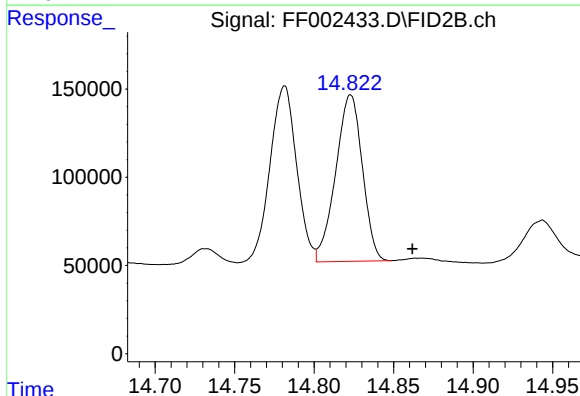


#10 N-TETRACOSANE

R.T.: 14.823 min
Delta R.T.: -0.039 min
Response: 1103215
Conc: 7.05 ug/ml

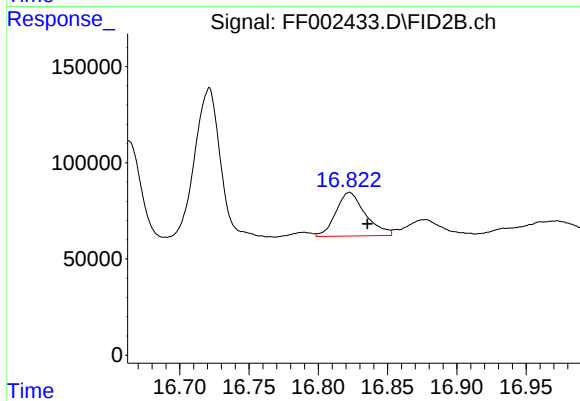


#12 N-OCTACOSANE

R.T.: 16.822 min
Delta R.T.: -0.013 min
Response: 337311
Conc: 2.17 ug/ml

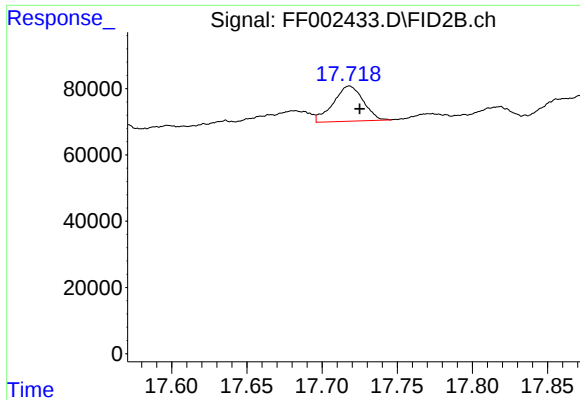


#13 N-TRIACONTANE

R.T.: 17.718 min
Delta R.T.: -0.007 min
Response: 148239
Conc: 0.96 ug/ml

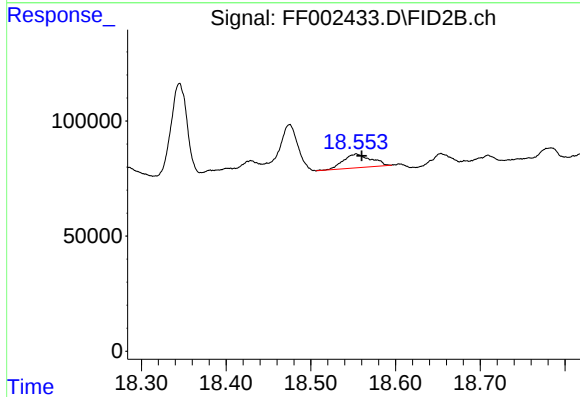

#14 N-DOTRIACONTANE

R.T.: 18.554 min
Delta R.T.: -0.006 min
Response: 134716
Conc: 0.87 ug/ml

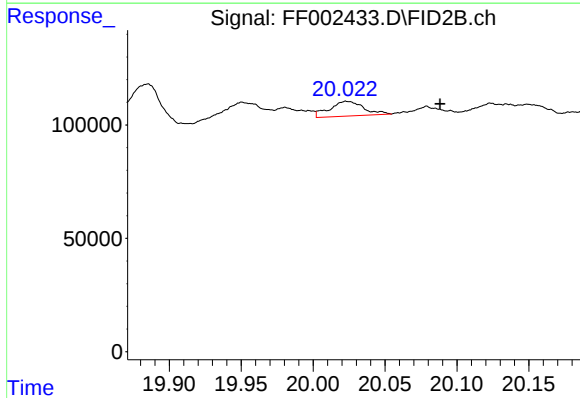

#16 N-HEXATRIACONTANE

R.T.: 20.023 min
Delta R.T.: -0.065 min
Response: 106772
Conc: 0.78 ug/ml