

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101818\
 Data File : FF002430.D
 Signal(s) : FID2B.ch
 Acq On : 18 Oct 2018 15:13
 Operator : AJ\SJ
 Sample : J5204-05MSD 10X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Oct 18 23:54:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
 Quant Title :
 QLast Update : Fri Oct 12 13:21:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.649	383112	2.756 ug/ml
Target Compounds			
2) N-DECANE	4.382	258239	1.691 ug/ml
3) N-DODECANE	6.401	305987	1.976 ug/ml
4) N-TETRADECANE	8.194	360688	2.305 ug/ml
5) N-HEXADECANE	9.796	507408	3.228 ug/ml
6) N-OCTADECANE	11.238	454740	2.861 ug/ml
7) N-EICOSANE	12.549	454648	2.870 ug/ml
8) N-DOCOSANE	13.749	538319	3.412 ug/ml
10) N-TETRACOSANE	14.852	346191	2.213 ug/ml
11) N-HEXACOSANE	15.876	404605	2.598 ug/ml
12) N-OCTACOSANE	16.825	450718	2.906 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101818\
Data File : FF002430.D
Signal(s) : FID2B.ch
Acq On : 18 Oct 2018 15:13
Operator : AJ\SJ
Sample : J5204-05MSD 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Oct 18 23:54:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

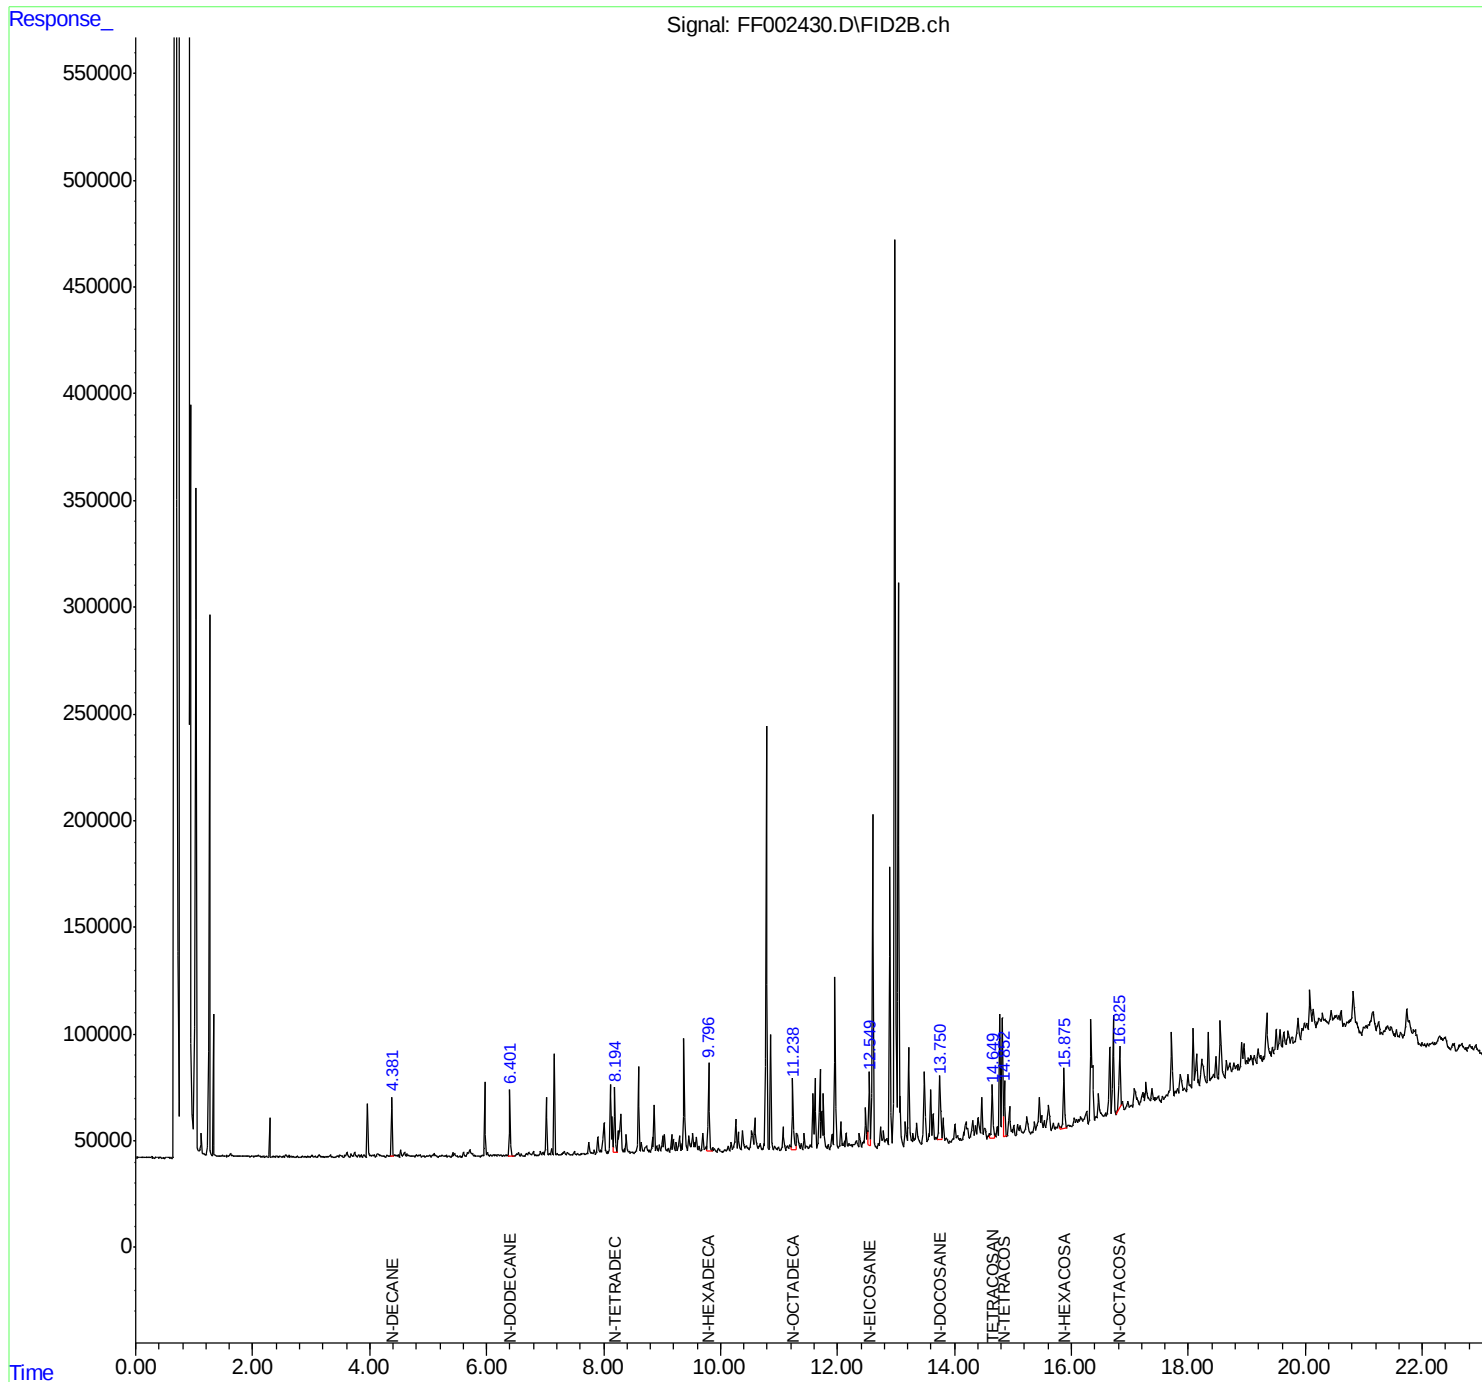

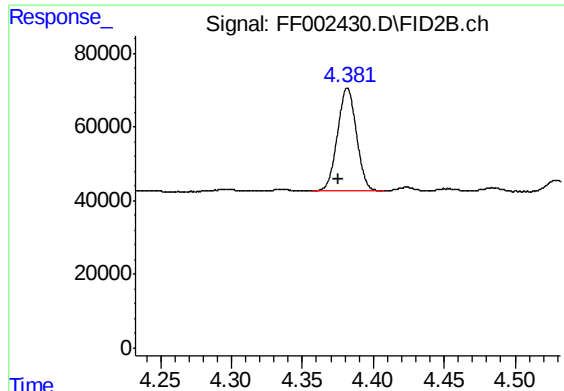


#2 N-DECANE

R.T.: 4.382 min
Delta R.T.: 0.006 min
Response: 258239
Conc: 1.69 ug/ml

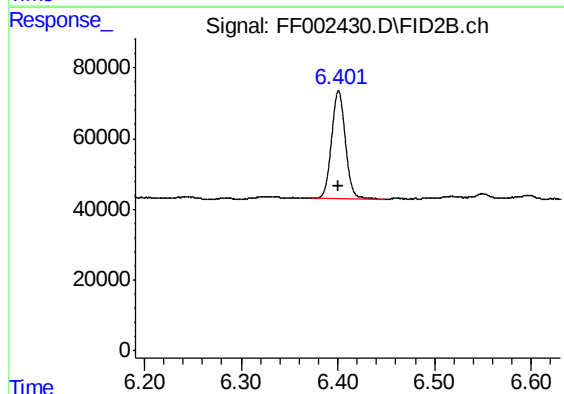


#3 N-DODECANE

R.T.: 6.401 min
Delta R.T.: 0.000 min
Response: 305987
Conc: 1.98 ug/ml

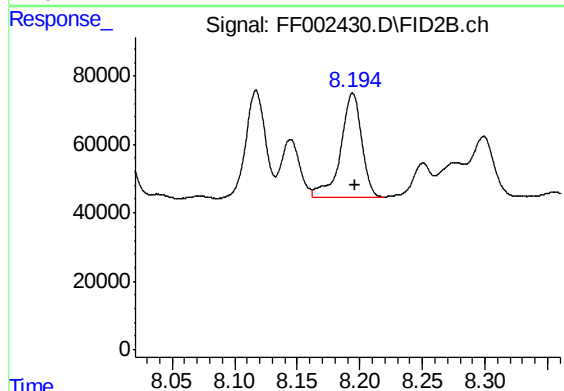


#4 N-TETRADECANE

R.T.: 8.194 min
Delta R.T.: -0.002 min
Response: 360688
Conc: 2.30 ug/ml

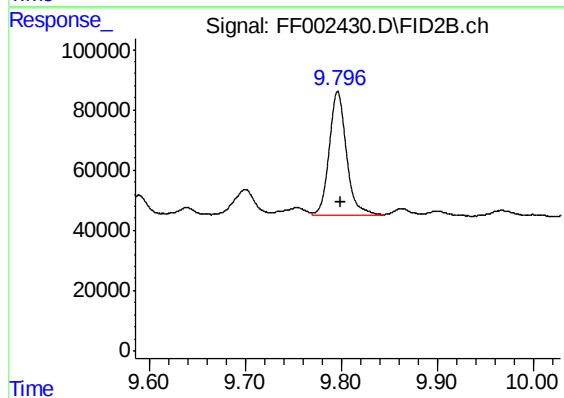


#5 N-HEXADECANE

R.T.: 9.796 min
Delta R.T.: -0.003 min
Response: 507408
Conc: 3.23 ug/ml

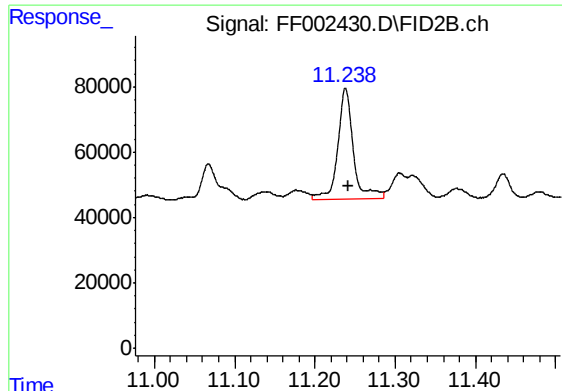


#6 N-OCTADECANE

R.T.: 11.238 min
Delta R.T.: -0.004 min
Response: 454740
Conc: 2.86 ug/ml

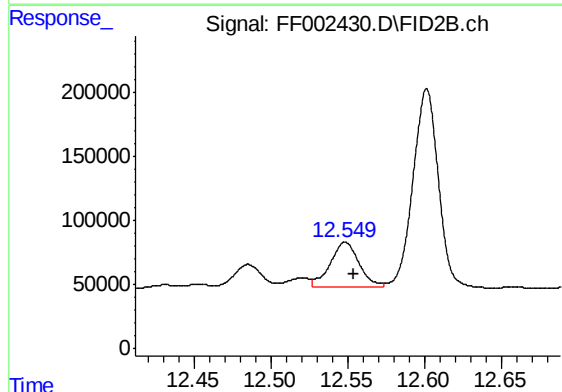


#7 N-EICOSANE

R.T.: 12.549 min
Delta R.T.: -0.006 min
Response: 454648
Conc: 2.87 ug/ml

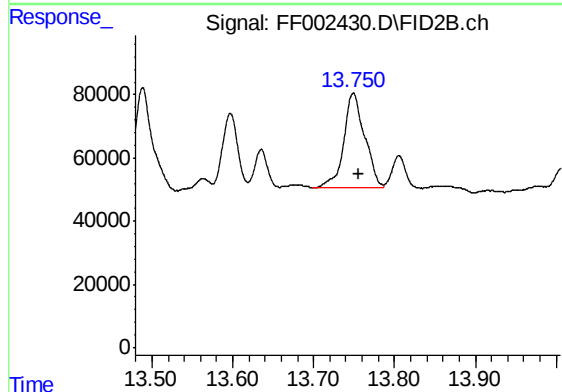


#8 N-DOCOSANE

R.T.: 13.749 min
Delta R.T.: -0.006 min
Response: 538319
Conc: 3.41 ug/ml

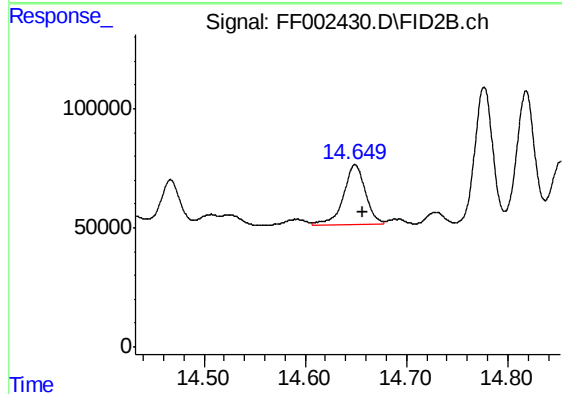


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.649 min
Delta R.T.: -0.007 min
Response: 383112
Conc: 2.76 ug/ml

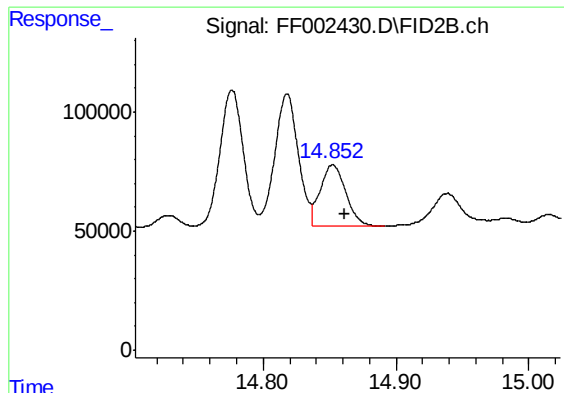


#10 N-TETRACOSANE

R.T.: 14.852 min
Delta R.T.: -0.009 min
Response: 346191
Conc: 2.21 ug/ml

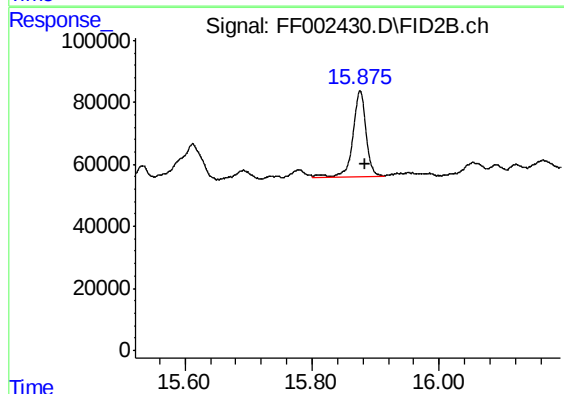

#11 N-HEXACOSANE

R.T.: 15.876 min
Delta R.T.: -0.009 min
Response: 404605
Conc: 2.60 ug/ml

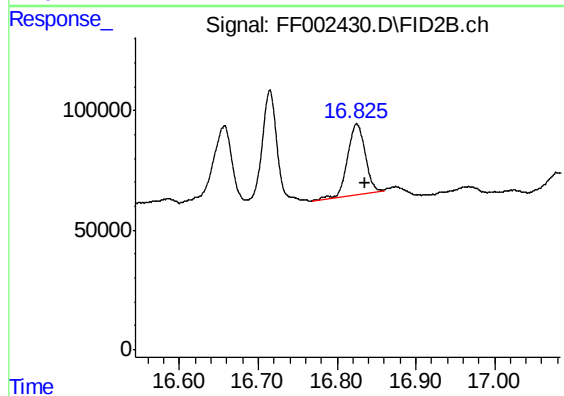

#12 N-OCTACOSANE

R.T.: 16.825 min
Delta R.T.: -0.010 min
Response: 450718
Conc: 2.91 ug/ml