

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101818\
 Data File : FF002436.D
 Signal(s) : FID2B.ch
 Acq On : 18 Oct 2018 18:12
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Oct 18 23:55:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
 Quant Title :
 QLast Update : Fri Oct 12 13:21:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.655	6067890	43.657 ug/ml
Target Compounds			
2) N-DECANE	4.385	7665394	50.181 ug/ml
3) N-DODECANE	6.406	7661469	49.478 ug/ml
4) N-TETRADECANE	8.200	7593832	48.528 ug/ml
5) N-HEXADECANE	9.801	7506809	47.763 ug/ml
6) N-OCTADECANE	11.244	7419825	46.688 ug/ml
7) N-EICOSANE	12.555	7211994	45.534 ug/ml
8) N-DOCOSANE	13.755	6998614	44.361 ug/ml
10) N-TETRACOSANE	14.860	6750762	43.149 ug/ml
11) N-HEXACOSANE	15.883	6554736	42.095 ug/ml
12) N-OCTACOSANE	16.834	6427265	41.435 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF101818\
Data File : FF002436.D
Signal(s) : FID2B.ch
Acq On : 18 Oct 2018 18:12
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Oct 18 23:55:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

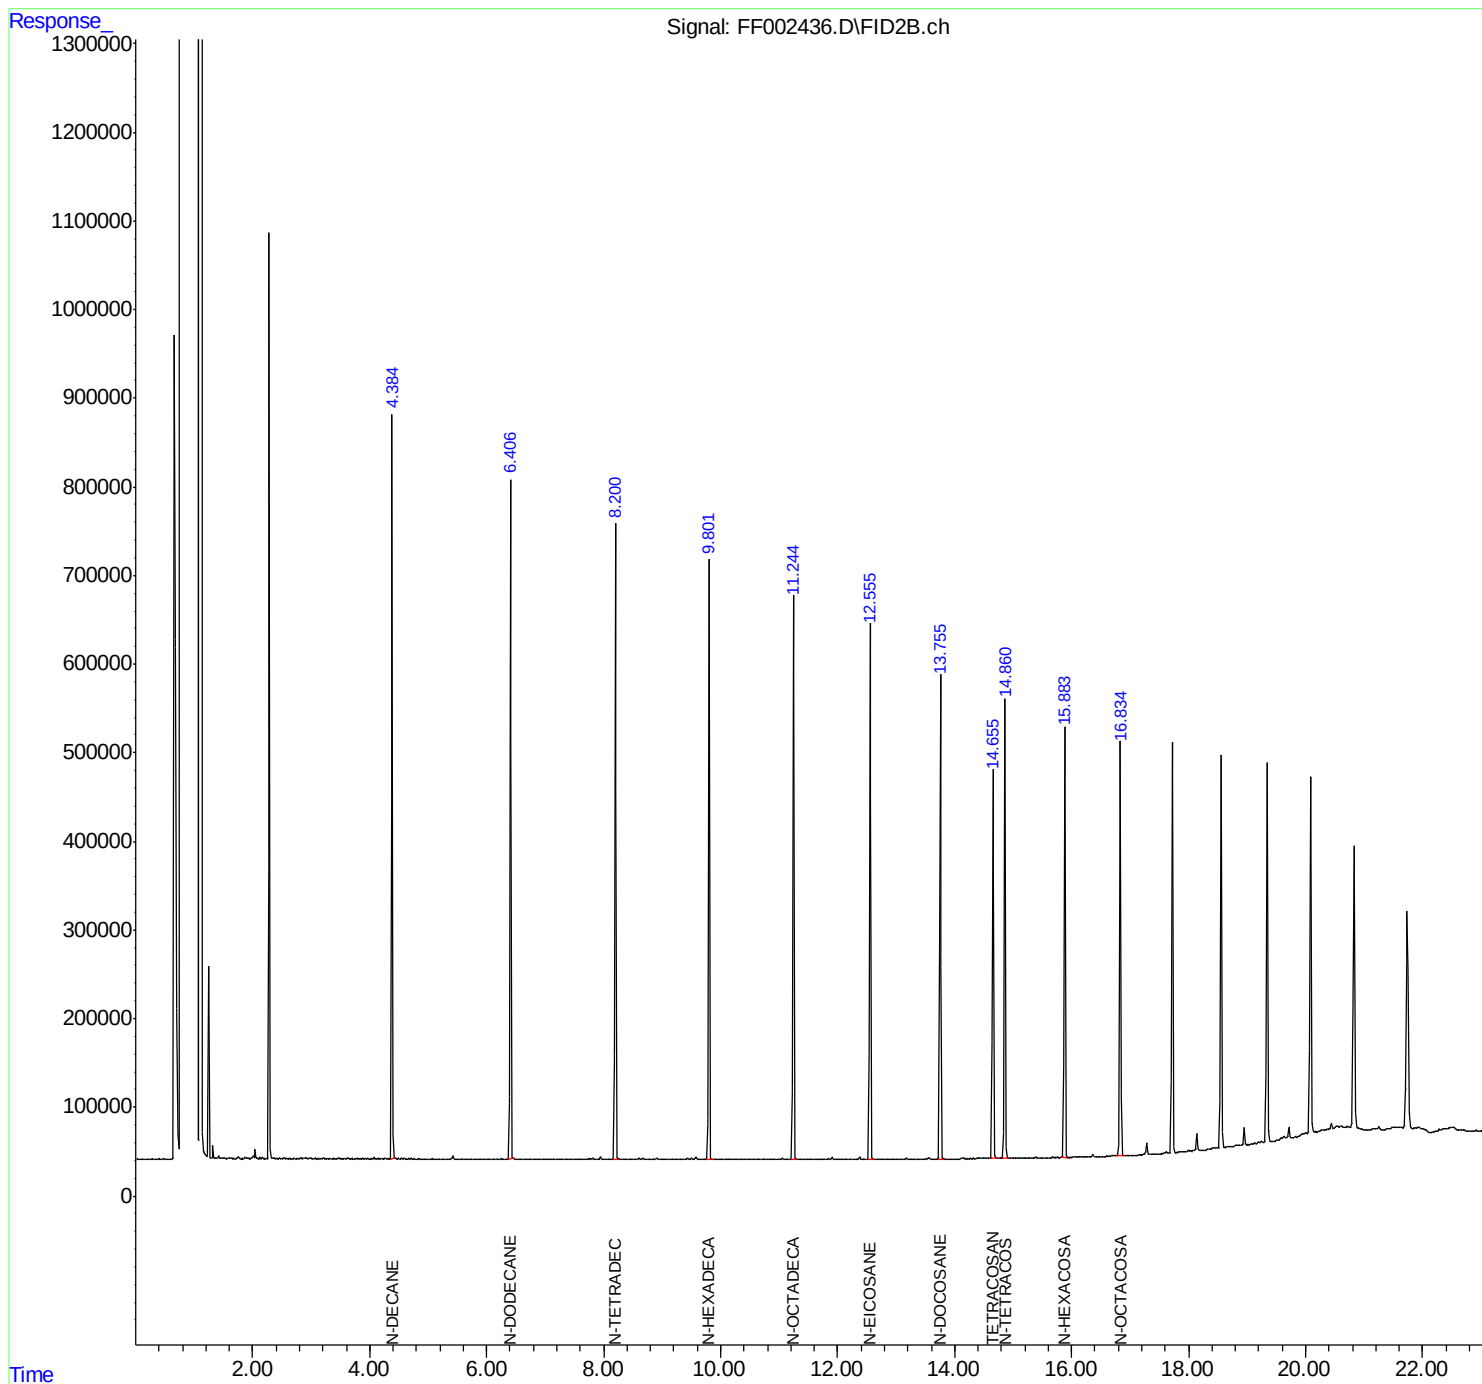

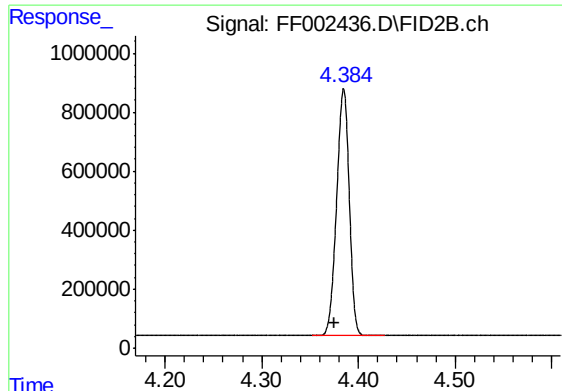


#2 N-DECANE

R.T.: 4.385 min
Delta R.T.: 0.009 min
Response: 7665394
Conc: 50.18 ug/ml

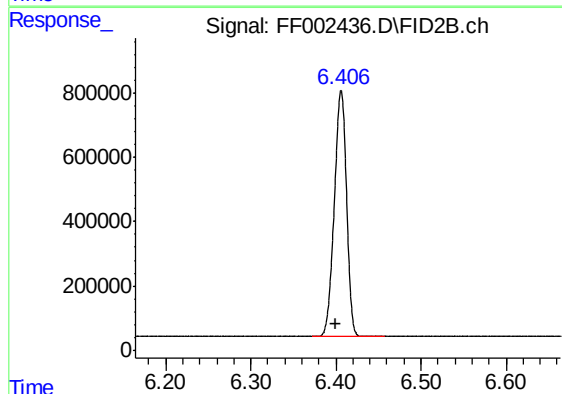


#3 N-DODECANE

R.T.: 6.406 min
Delta R.T.: 0.006 min
Response: 7661469
Conc: 49.48 ug/ml

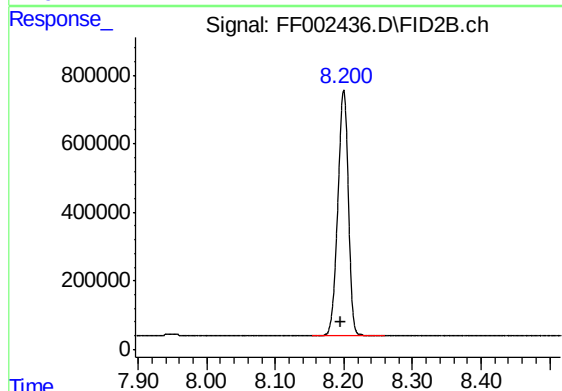


#4 N-TETRADECANE

R.T.: 8.200 min
Delta R.T.: 0.004 min
Response: 7593832
Conc: 48.53 ug/ml

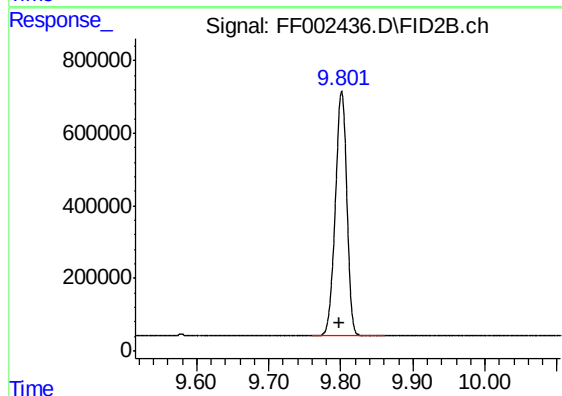


#5 N-HEXADECANE

R.T.: 9.801 min
Delta R.T.: 0.002 min
Response: 7506809
Conc: 47.76 ug/ml

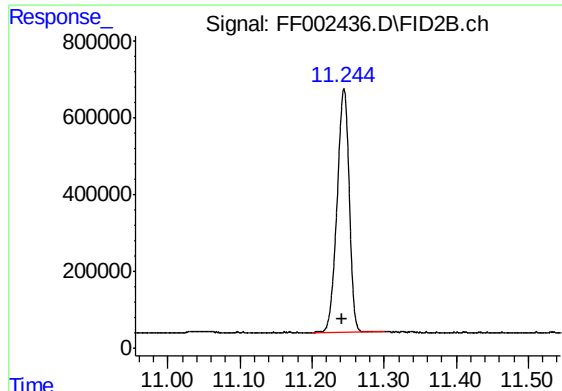


#6 N-OCTADECANE

R.T.: 11.244 min
Delta R.T.: 0.002 min
Response: 7419825
Conc: 46.69 ug/ml

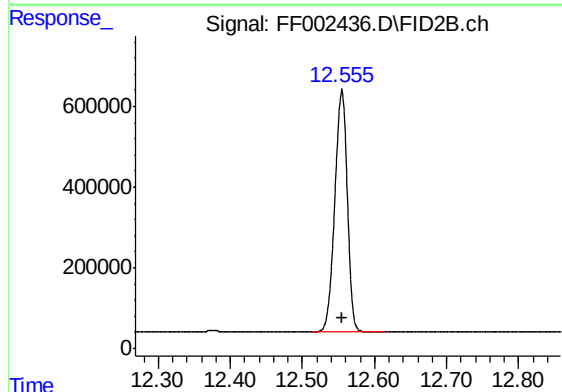


#7 N-EICOSANE

R.T.: 12.555 min
Delta R.T.: 0.000 min
Response: 7211994
Conc: 45.53 ug/ml

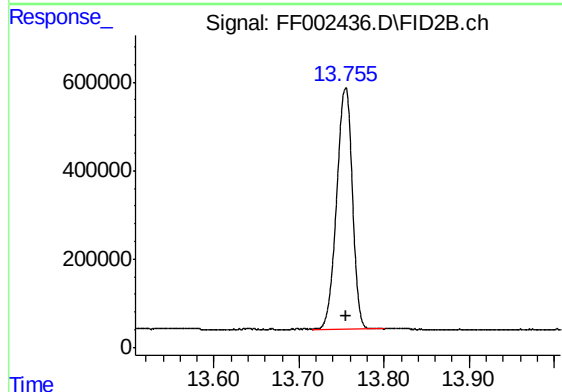


#8 N-DOCOSANE

R.T.: 13.755 min
Delta R.T.: 0.000 min
Response: 6998614
Conc: 44.36 ug/ml

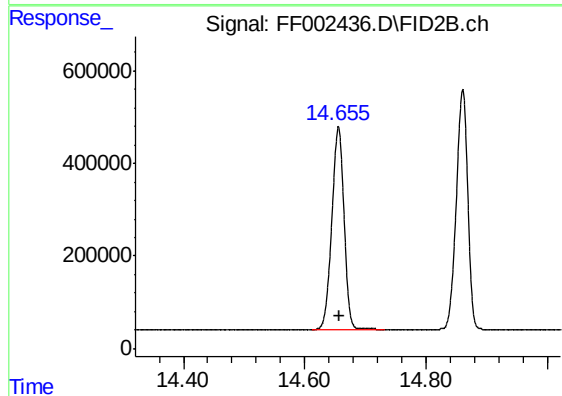


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.655 min
Delta R.T.: 0.000 min
Response: 6067890
Conc: 43.66 ug/ml

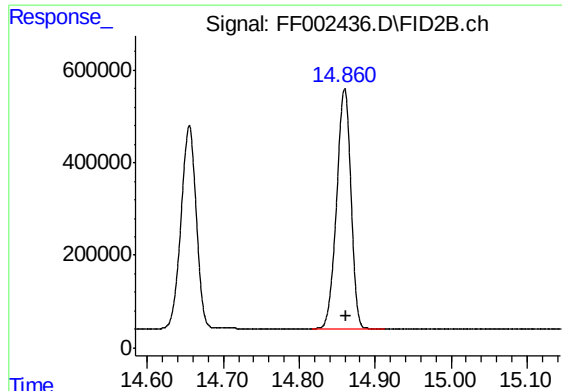


#10 N-TETRACOSANE

R.T.: 14.860 min
Delta R.T.: -0.002 min
Response: 6750762
Conc: 43.15 ug/ml

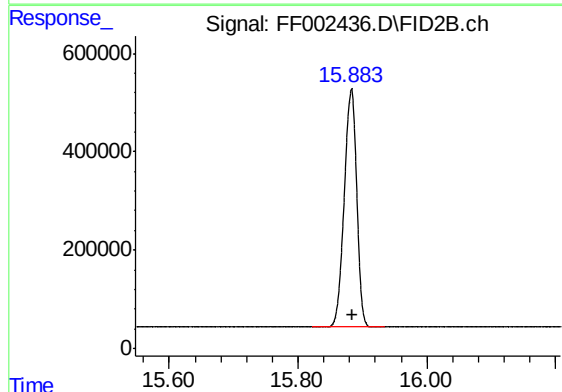

#11 N-HEXACOSANE

R.T.: 15.883 min
Delta R.T.: -0.001 min
Response: 6554736
Conc: 42.09 ug/ml

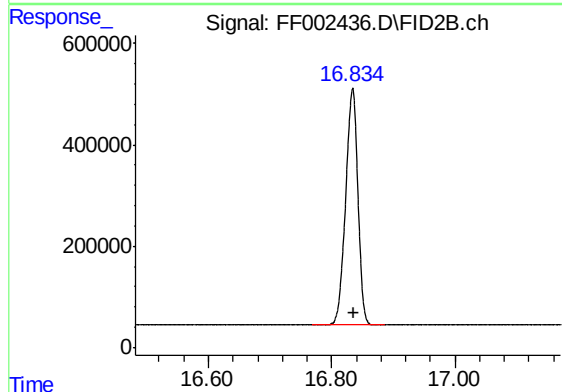

#12 N-OCTACOSANE

R.T.: 16.834 min
Delta R.T.: -0.001 min
Response: 6427265
Conc: 41.44 ug/ml