

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF101921\  
Data File : FF009176.D  
Signal(s) : FID2B.ch  
Acq On : 19 Oct 2021 10:33  
Operator : AJ\MA  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Oct 20 00:39:19 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF100721.M  
Quant Title :  
QLast Update : Fri Oct 08 02:25:33 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

|                             | Compound                 | R.T.   | Response | Conc Units   |
|-----------------------------|--------------------------|--------|----------|--------------|
| -----                       |                          |        |          |              |
| System Monitoring Compounds |                          |        |          |              |
| 9) S                        | TETRACOSANE-d50 (SURR... | 14.710 | 2033608  | 18.545 ug/ml |
|                             |                          |        |          |              |
| Target Compounds            |                          |        |          |              |
| 14)                         | N-DOTRIACONTANE          | 18.596 | 103640   | 0.981 ug/ml  |
| -----                       |                          |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF101921\  
Data File : FF009176.D  
Signal(s) : FID2B.ch  
Acq On : 19 Oct 2021 10:33  
Operator : AJ\MA  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Oct 20 00:39:19 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF100721.M  
Quant Title :  
QLast Update : Fri Oct 08 02:25:33 2021  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

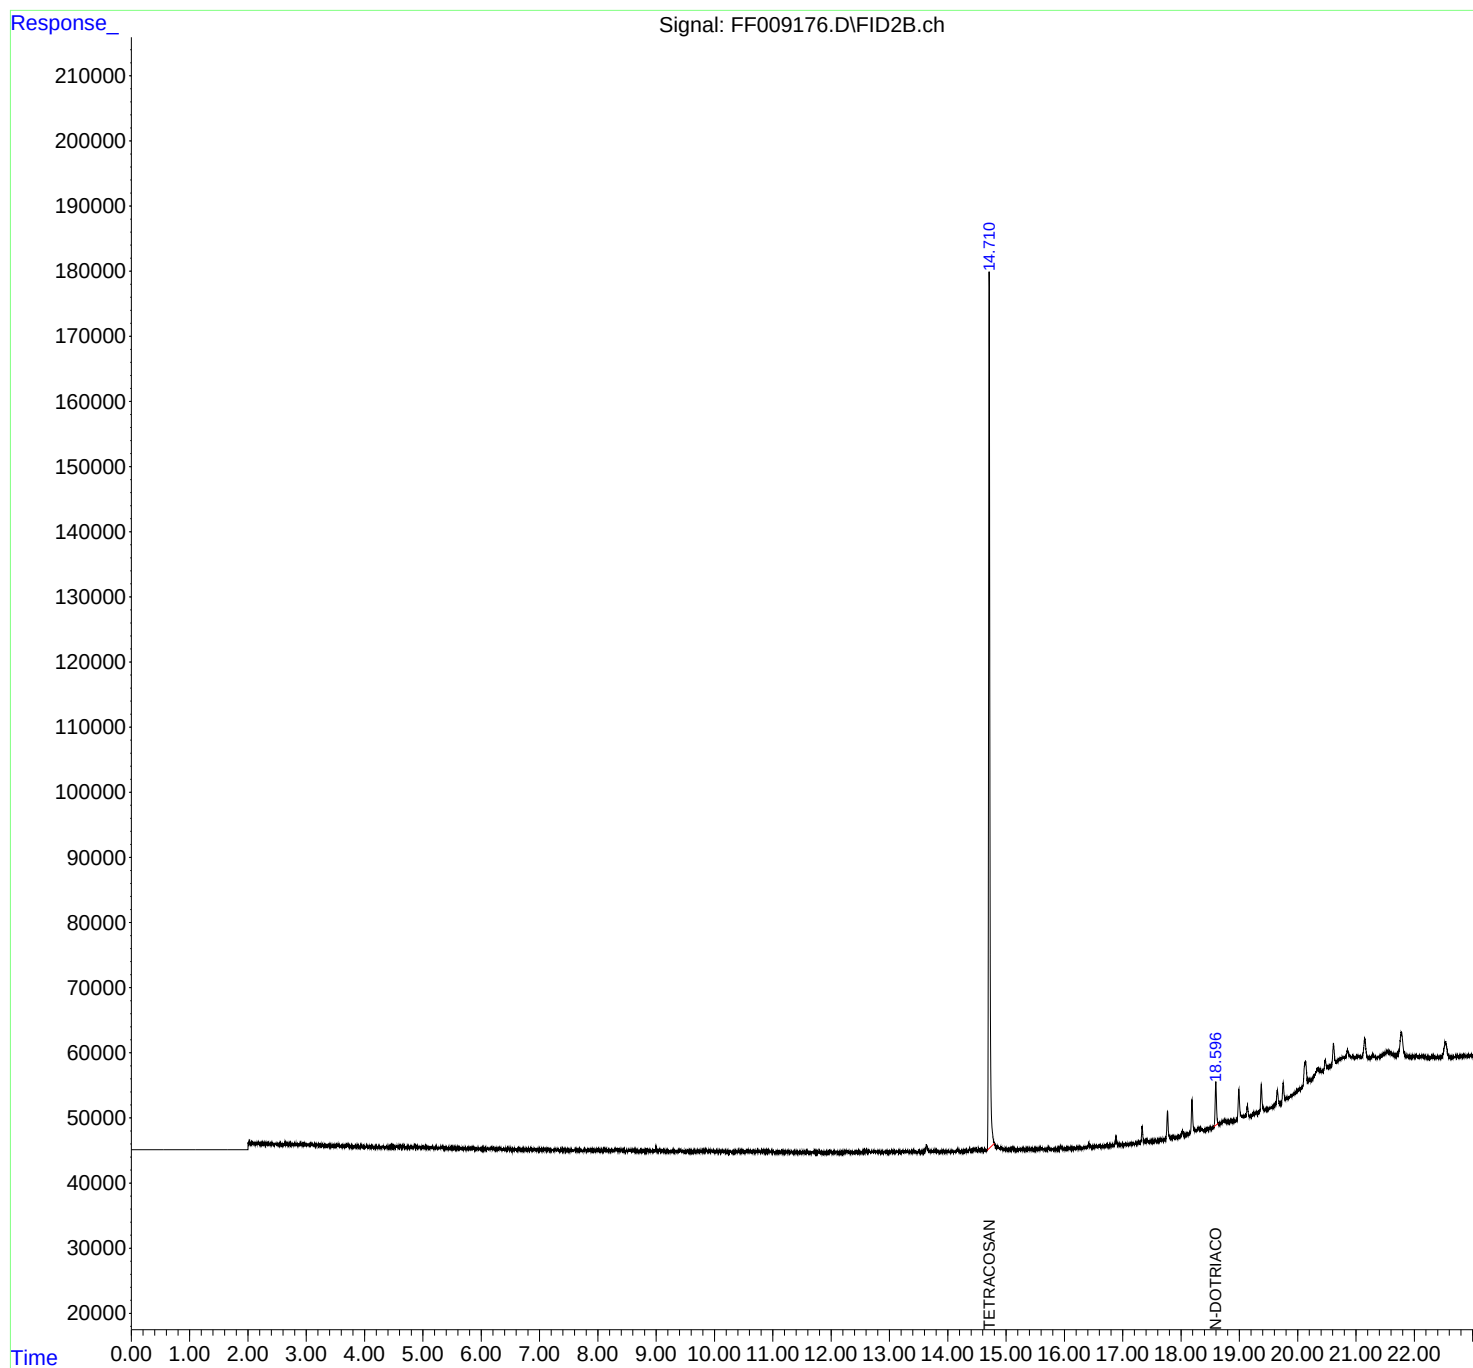

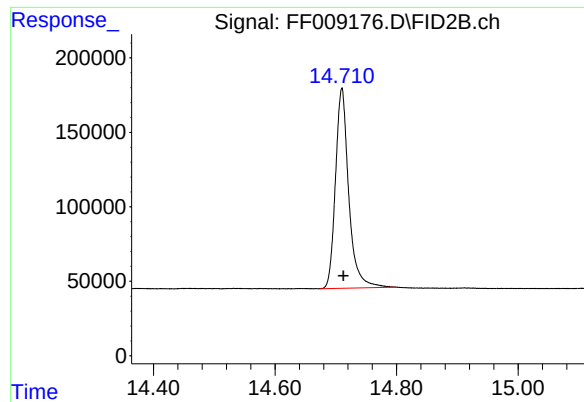

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.710 min  
Delta R.T.: -0.002 min  
Response: 2033608  
Conc: 18.55 ug/ml

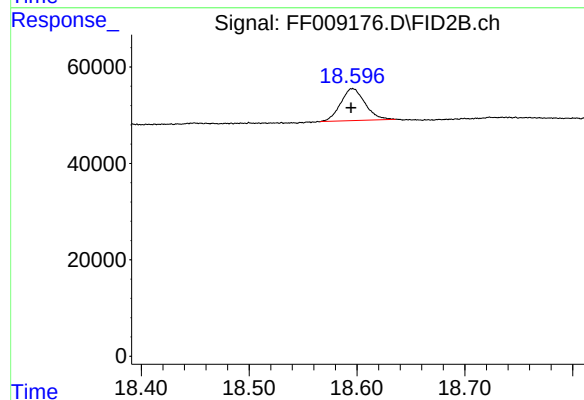

#14 N-DOTRIACONTANE

R.T.: 18.596 min  
Delta R.T.: 0.002 min  
Response: 103640  
Conc: 0.98 ug/ml