

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102025AL\
Data File : FF016567.D
Signal(s) : FID2B.ch
Acq On : 20 Oct 2025 13:17
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Oct 20 23:18:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 100225.M
Quant Title : GC Extractables
QLast Update : Fri Oct 03 05:49:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

17) T	n-Tricontane (C30)	18.145	30760	0.247 ug/ml
18) T	n-Dotriacontane (C32)	18.981	71919	0.597 ug/ml
19) T	n-Tetratriacontane (C34)	19.768	46450	0.426 ug/ml
20) T	n-Hexatriacontane (C36)	20.512	71806	0.769 ug/ml
21) T	n-Octatriacontane (C38)	21.271	135645	1.613 ug/ml
22) T	n-Tetracontane (C40)	22.223	137969	1.757 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102025AL\
Data File : FF016567.D
Signal(s) : FID2B.ch
Acq On : 20 Oct 2025 13:17
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Oct 20 23:18:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aliphatic EPH 100225.M
Quant Title : GC Extractables
QLast Update : Fri Oct 03 05:49:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

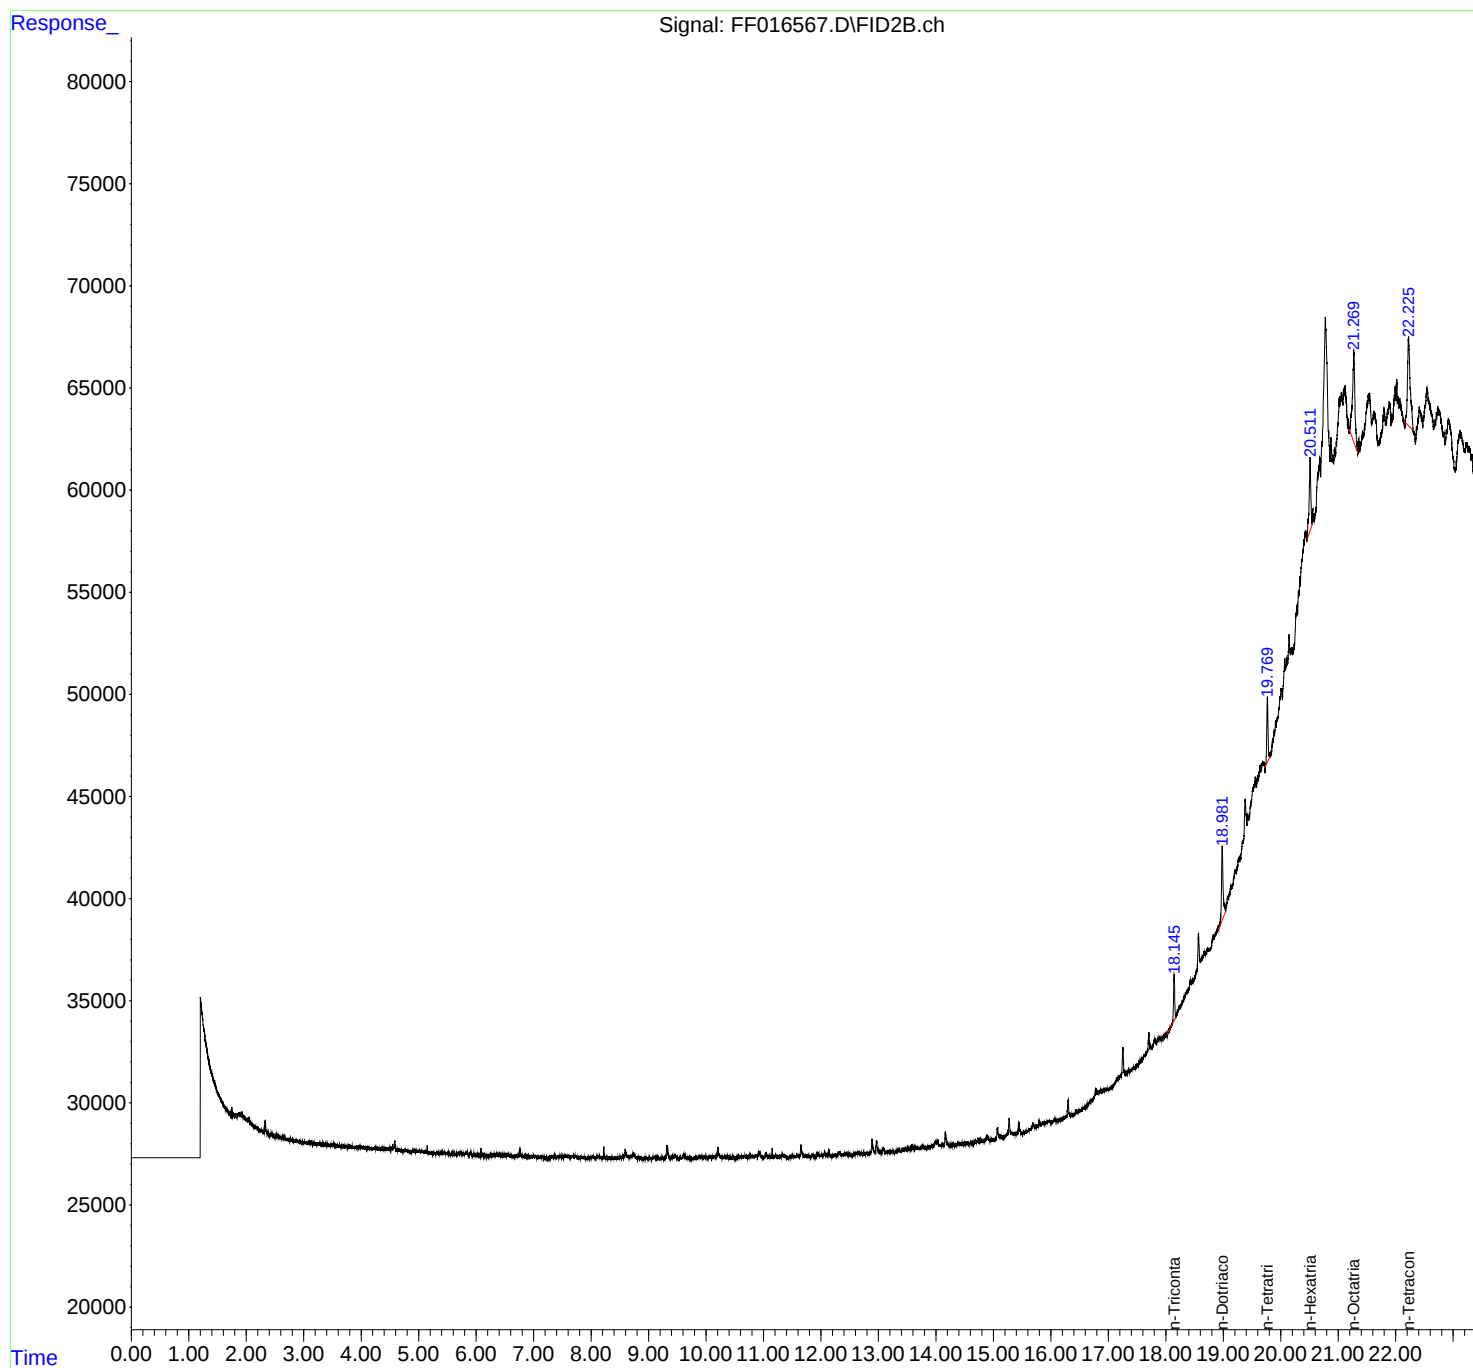


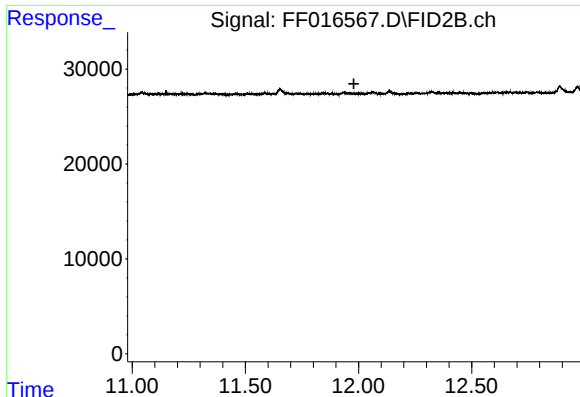

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.980 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :
I.BLK

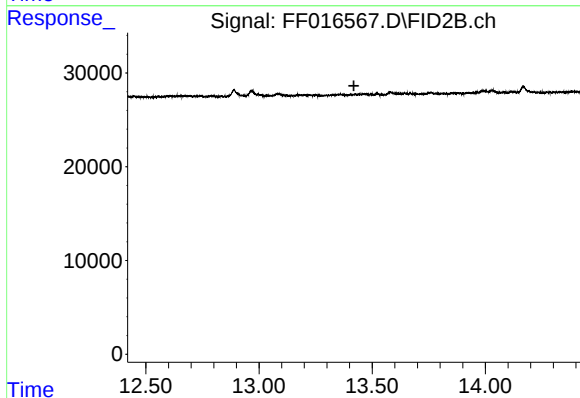


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.419 min
Response: 0
Conc: N.D.

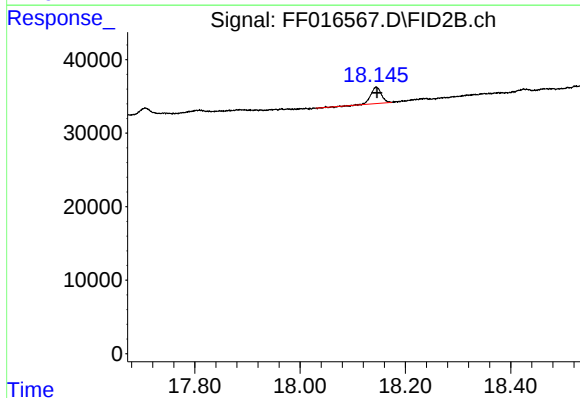


#17 n-Tricontane (C30)

R.T.: 18.145 min
Delta R.T.: -0.001 min
Response: 30760
Conc: 0.25 ug/ml

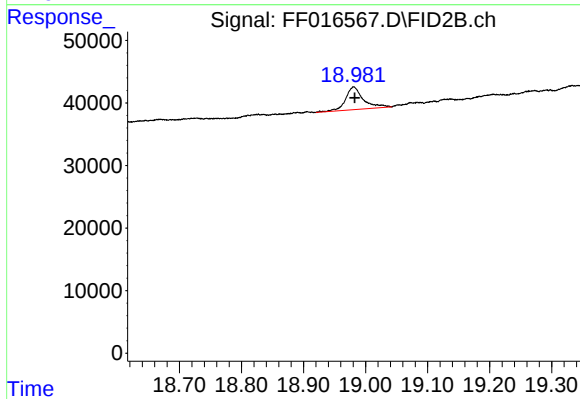

#18 n-Dotriacontane (C32)


R.T.: 18.981 min
Delta R.T.: -0.002 min
Response: 71919
Conc: 0.60 ug/ml

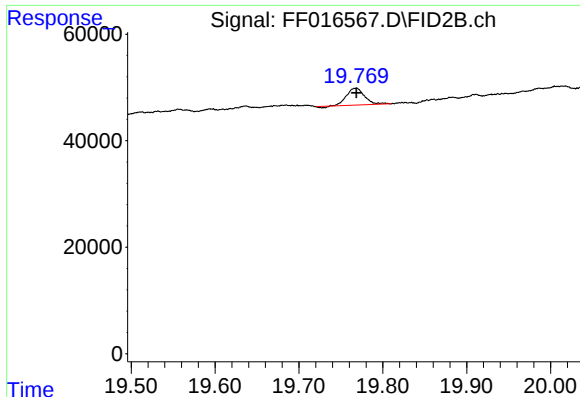

#19 n-Tetratriacontane (C34)


R.T.: 19.768 min
Delta R.T.: 0.000 min
Response: 46450
Conc: 0.43 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

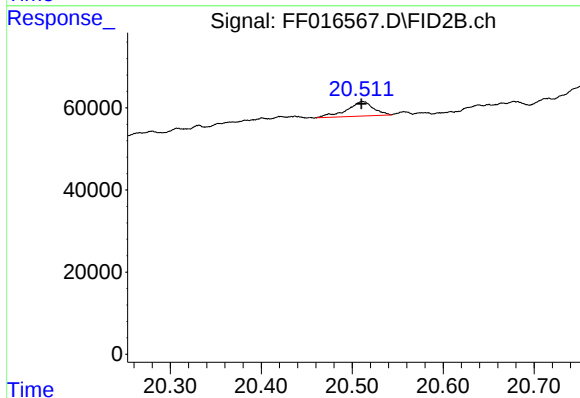


#20 n-Hexatriacontane (C36)

R.T.: 20.512 min
Delta R.T.: 0.001 min
Response: 71806
Conc: 0.77 ug/ml

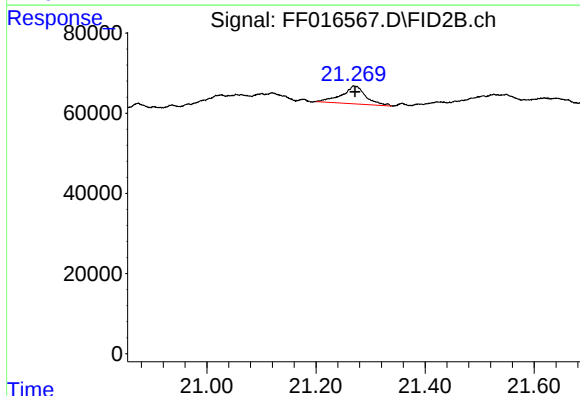

#21 n-Octatriacontane (C38)

R.T.: 21.271 min
Delta R.T.: -0.001 min
Response: 135645
Conc: 1.61 ug/ml

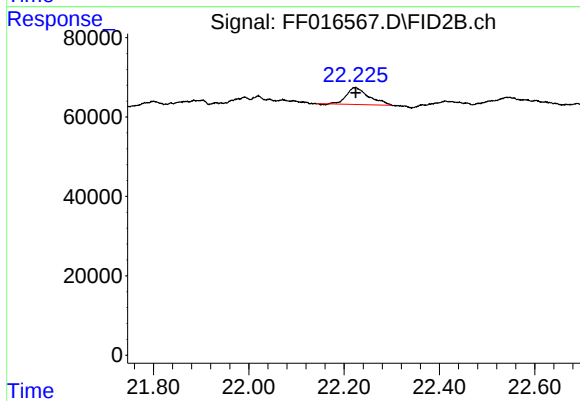

#22 n-Tetracontane (C40)

R.T.: 22.223 min
Delta R.T.: 0.000 min
Response: 137969
Conc: 1.76 ug/ml