

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102120\
 Data File : FF007753.D
 Signal(s) : FID2B.ch
 Acq On : 21 Oct 2020 13:45
 Operator : DD\AJ
 Sample : L4221-10 10X
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 22 01:28:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
 Quant Title :
 QLast Update : Mon Oct 05 15:41:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.729	152198	1.209 ug/ml
Target Compounds			
7) N-EICOSANE	12.698f	330346	2.222 ug/ml
10) N-TETRACOSANE	14.923	251682	1.745 ug/ml
11) N-HEXACOSANE	15.959	28331	0.204 ug/ml
12) N-OCTACOSANE	16.913	106913	0.798 ug/ml
13) N-TRIACONTANE	17.798	336748	2.604 ug/ml
14) N-DOTRIACONTANE	18.645	95382	0.793 ug/ml
15) N-TETRATRIACONTANE	19.470	427953	4.073 ug/ml
16) N-HEXATRIACONTANE	20.180	60618	0.635 ug/ml
17) N-OCTATRIACONTANE	20.919	62130	0.752 ug/ml
18) N-TETRACONTANE	21.802f	82160	0.941 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102120\
Data File : FF007753.D
Signal(s) : FID2B.ch
Acq On : 21 Oct 2020 13:45
Operator : DD\AJ
Sample : L4221-10 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 22 01:28:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
Quant Title :
QLast Update : Mon Oct 05 15:41:23 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

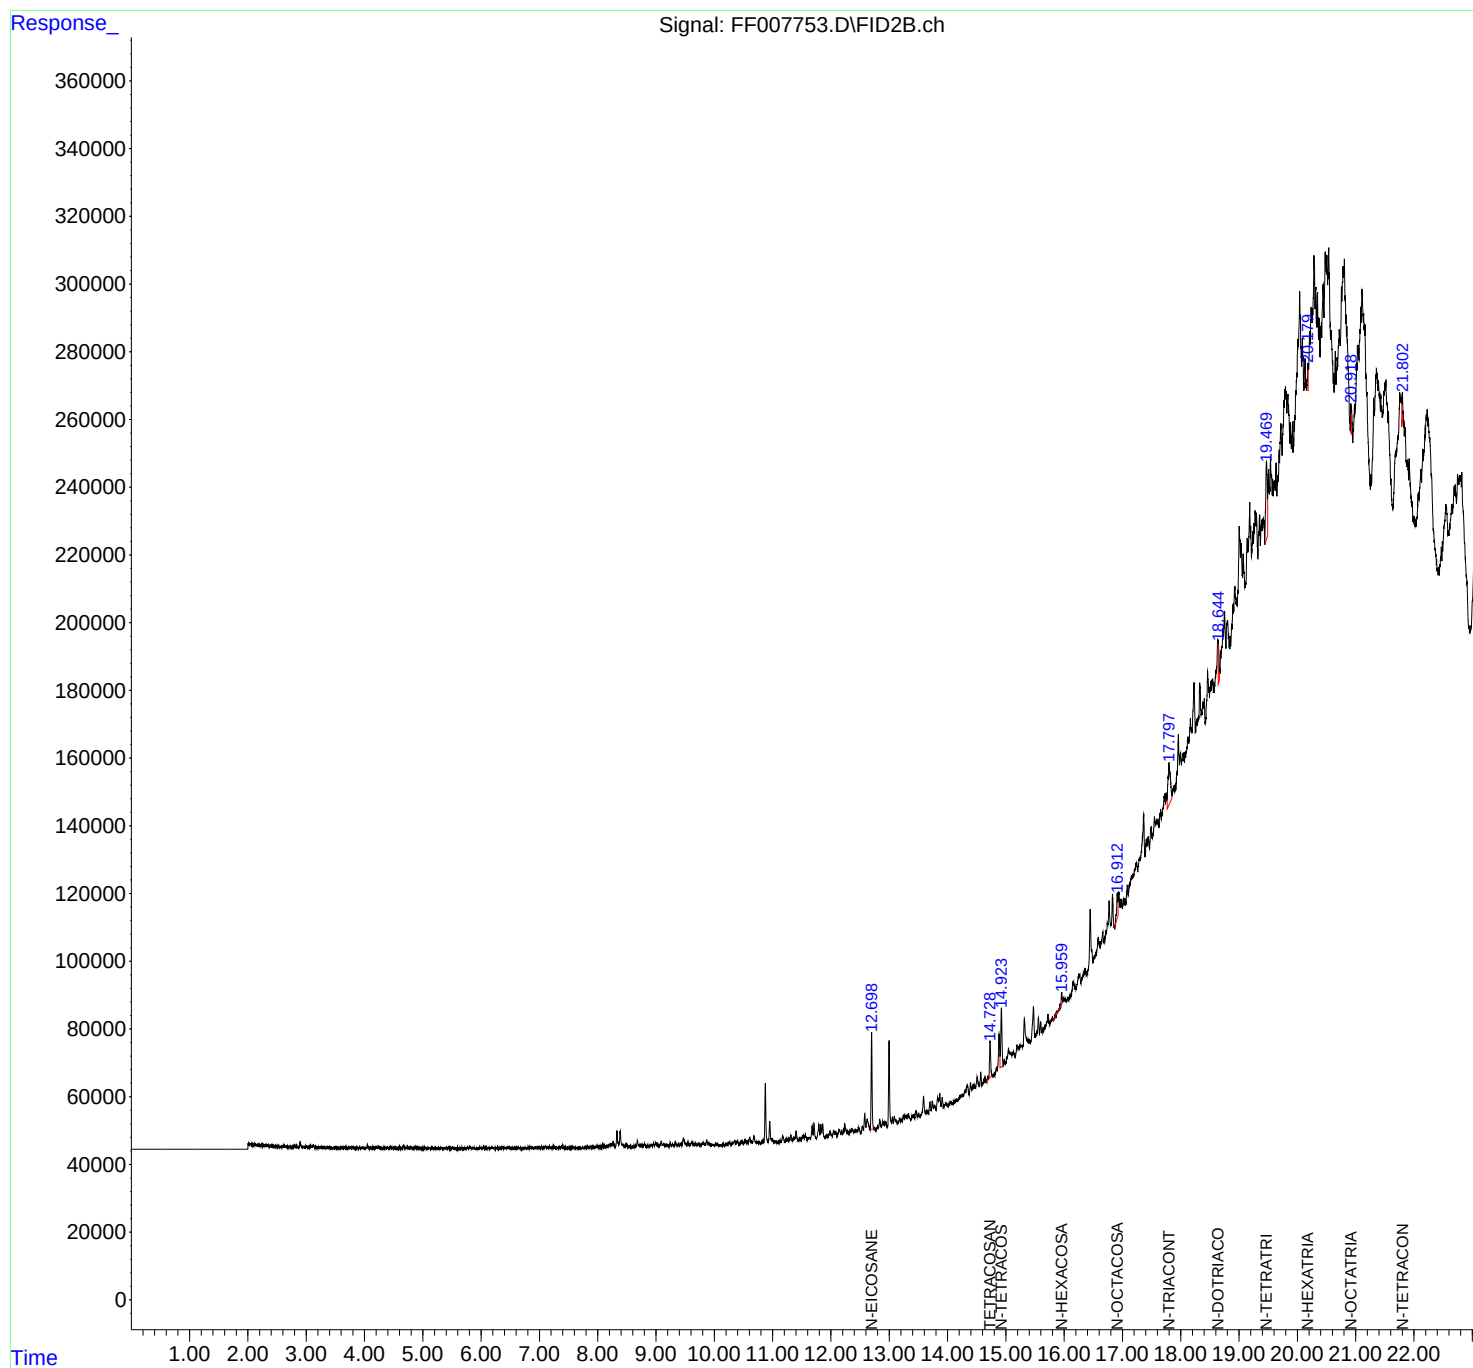

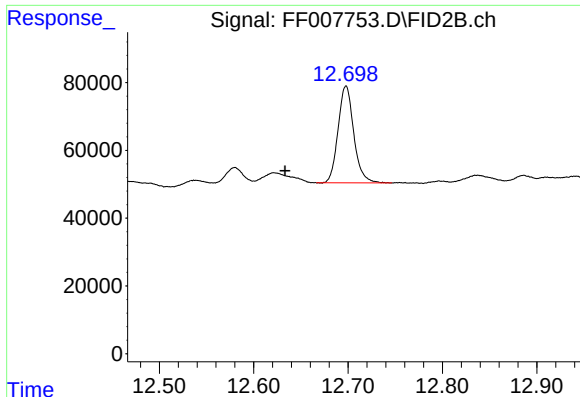


#7 N-EICOSANE

R.T.: 12.698 min
Delta R.T.: 0.065 min
Response: 330346
Conc: 2.22 ug/ml

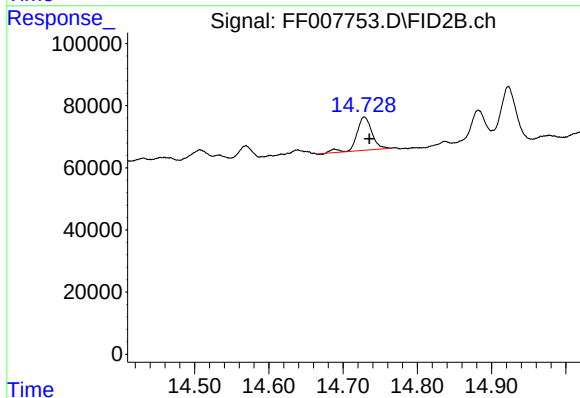


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.729 min
Delta R.T.: -0.007 min
Response: 152198
Conc: 1.21 ug/ml

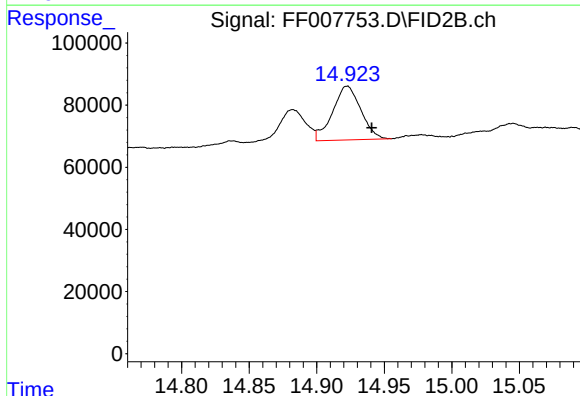


#10 N-TETRACOSANE

R.T.: 14.923 min
Delta R.T.: -0.018 min
Response: 251682
Conc: 1.74 ug/ml

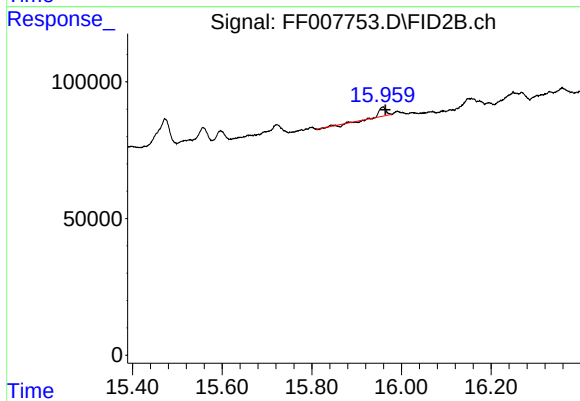


#11 N-HEXACOSANE

R.T.: 15.959 min
Delta R.T.: -0.005 min
Response: 28331
Conc: 0.20 ug/ml

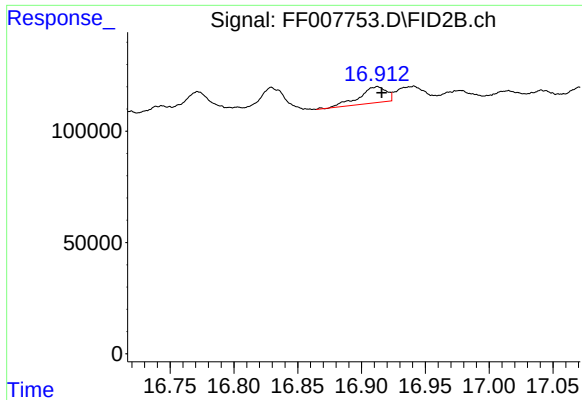


#12 N-OCTACOSANE

R.T.: 16.913 min
Delta R.T.: -0.003 min
Response: 106913
Conc: 0.80 ug/ml

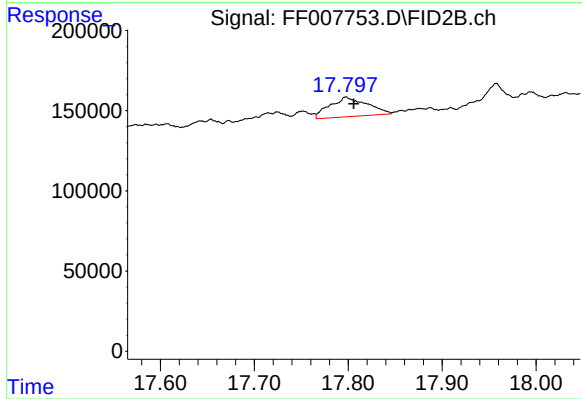


#13 N-TRIACONTANE

R.T.: 17.798 min
Delta R.T.: -0.008 min
Response: 336748
Conc: 2.60 ug/ml

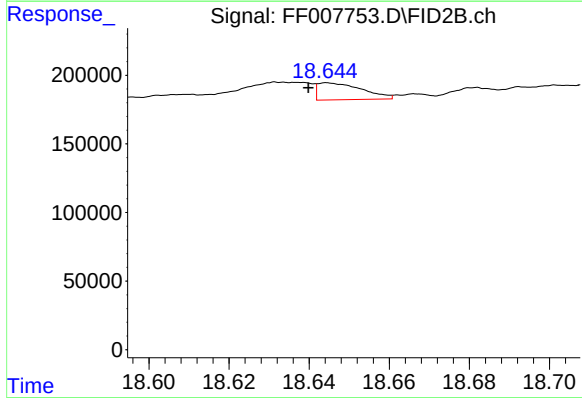


#14 N-DOTRIACONTANE

R.T.: 18.645 min
Delta R.T.: 0.005 min
Response: 95382
Conc: 0.79 ug/ml

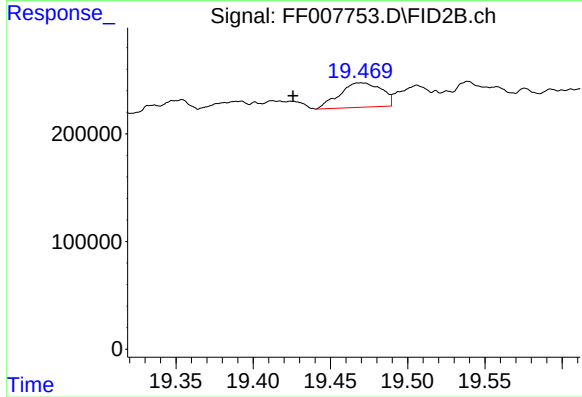


#15 N-TETRATRIACONTANE

R.T.: 19.470 min
Delta R.T.: 0.044 min
Response: 427953
Conc: 4.07 ug/ml

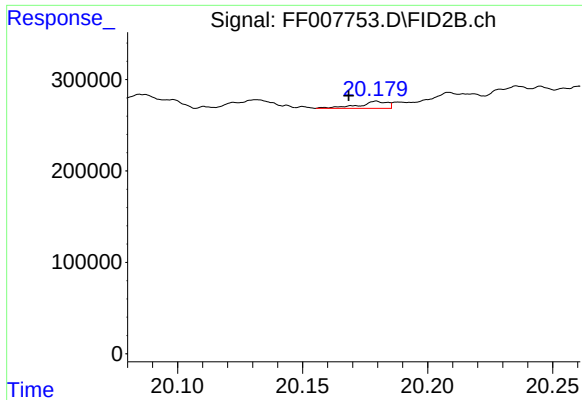


#16 N-HEXATRIACONTANE

R.T.: 20.180 min
Delta R.T.: 0.011 min
Response: 60618
Conc: 0.64 ug/ml

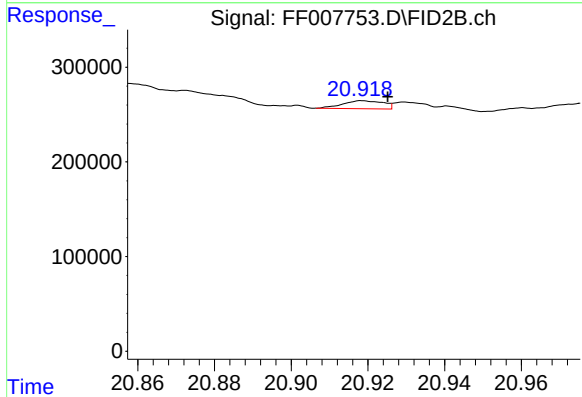

#17 N-OCTATRIACONTANE

R.T.: 20.919 min
Delta R.T.: -0.007 min
Response: 62130
Conc: 0.75 ug/ml

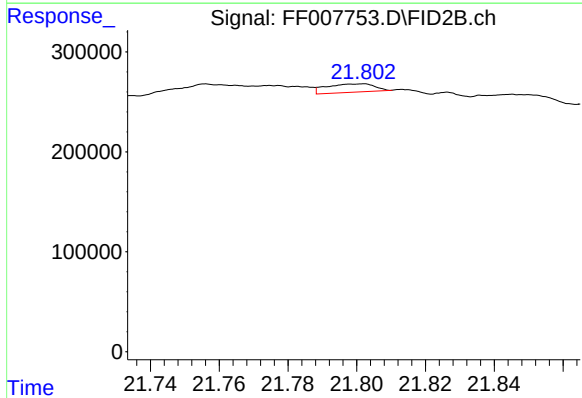

#18 N-TETRACONTANE

R.T.: 21.802 min
Delta R.T.: -0.067 min
Response: 82160
Conc: 0.94 ug/ml