

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102120\
Data File : FF007759.D
Signal(s) : FID2B.ch
Acq On : 21 Oct 2020 17:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 22 01:30:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
Quant Title :
QLast Update : Mon Oct 05 15:41:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.735	2057145	16.346 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.806	93110	0.720 ug/ml
14) N-DOTRIACONTANE	18.638	102788	0.854 ug/ml
15) N-TETRATRIACONTANE	19.428	75949	0.723 ug/ml
18) N-TETRACONTANE	21.913	183079	2.097 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102120\
Data File : FF007759.D
Signal(s) : FID2B.ch
Acq On : 21 Oct 2020 17:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 22 01:30:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
Quant Title :
QLast Update : Mon Oct 05 15:41:23 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

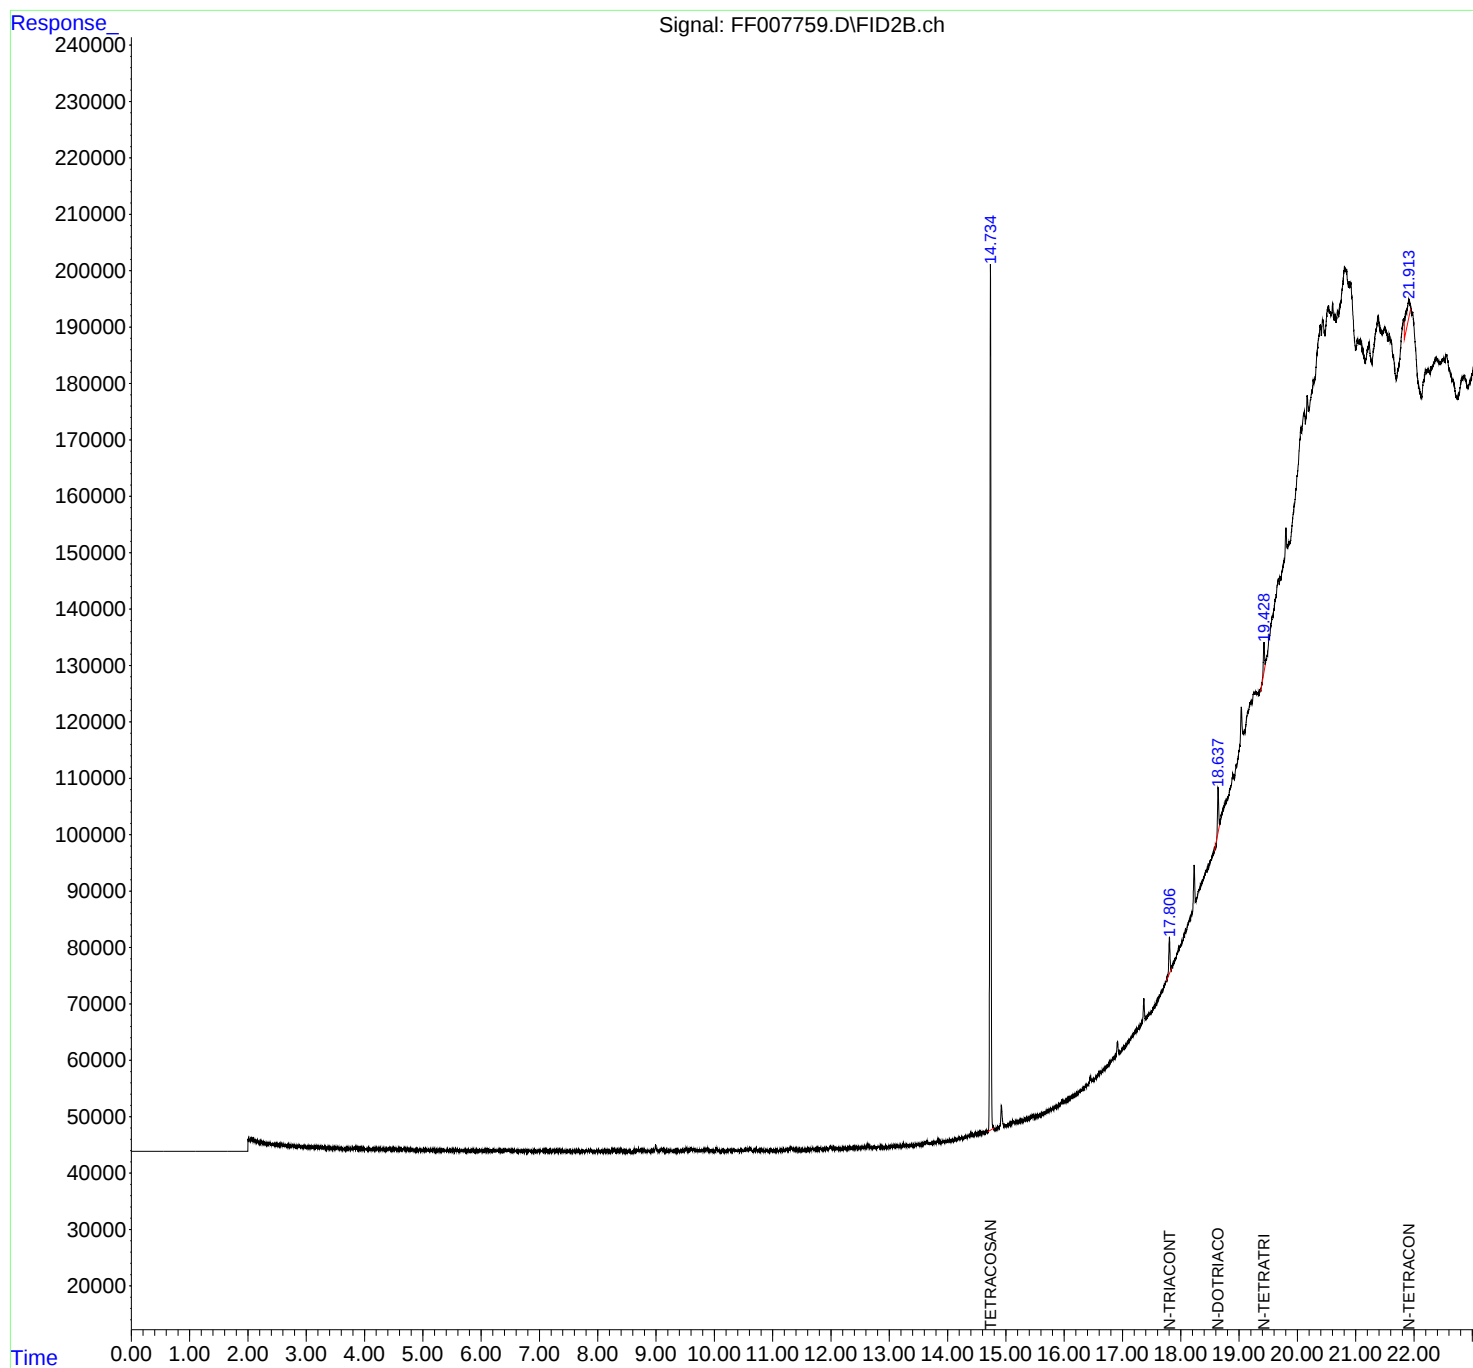

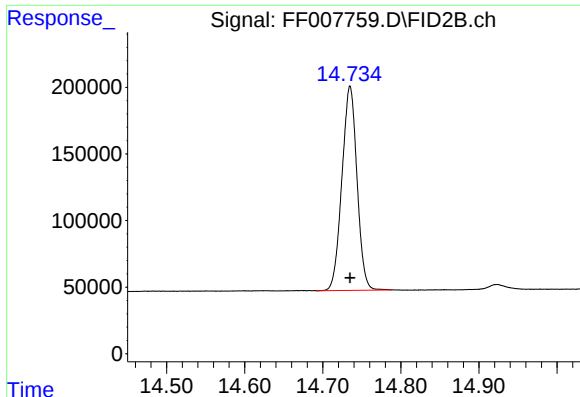


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.735 min
Delta R.T.: 0.000 min
Response: 2057145
Conc: 16.35 ug/ml

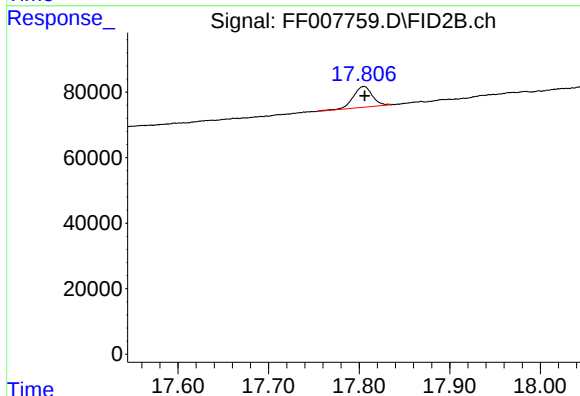


#13 N-TRIACONTANE

R.T.: 17.806 min
Delta R.T.: 0.000 min
Response: 93110
Conc: 0.72 ug/ml

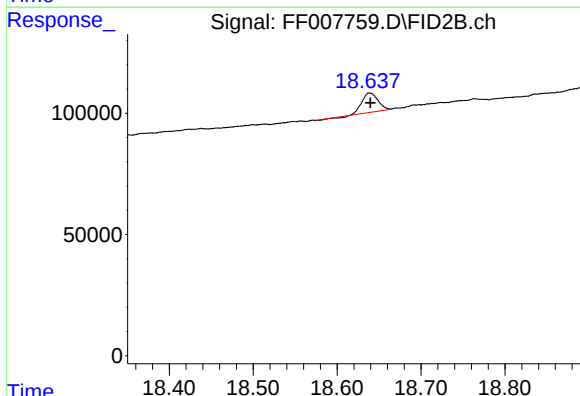


#14 N-DOTRIACONTANE

R.T.: 18.638 min
Delta R.T.: -0.002 min
Response: 102788
Conc: 0.85 ug/ml

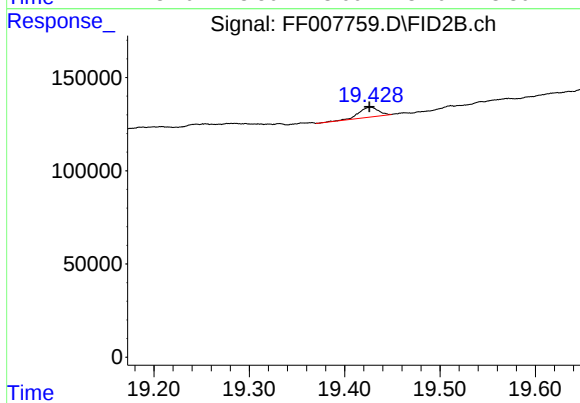

#15 N-TETRATRIACONTANE

R.T.: 19.428 min
Delta R.T.: 0.002 min
Response: 75949
Conc: 0.72 ug/ml

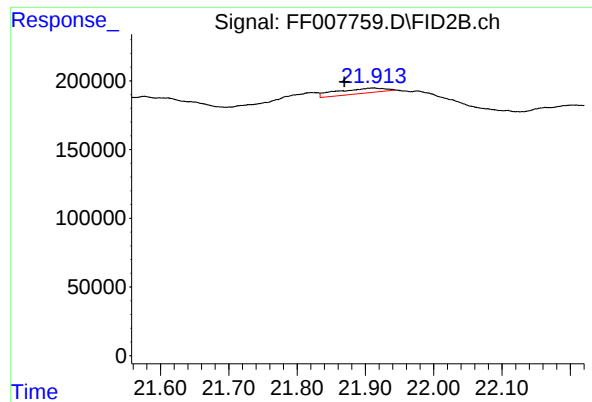

#18 N-TETRACONTANE

R.T.: 21.913 min
Delta R.T.: 0.044 min
Response: 183079
Conc: 2.10 ug/ml