

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102224\
Data File : FF014736.D
Signal(s) : FID2B.ch
Acq On : 22 Oct 2024 15:22
Operator : YP\AJ
Sample : P4473-01
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
TS-1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :Ankita Jodhani 10/23/2024

Integration File: autoint1.e
Quant Time: Oct 23 04:03:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102124.M
Quant Title :
QLast Update : Tue Oct 22 08:35:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.004	1939756	14.740 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102224\
Data File : FF014736.D
Signal(s) : FID2B.ch
Acq On : 22 Oct 2024 15:22
Operator : YP\AJ
Sample : P4473-01
Misc :
ALS Vial : 61 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
TS-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :Ankita Jodhani 10/23/2024

Integration File: autoint1.e
Quant Time: Oct 23 04:03:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102124.M
Quant Title :
QLast Update : Tue Oct 22 08:35:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

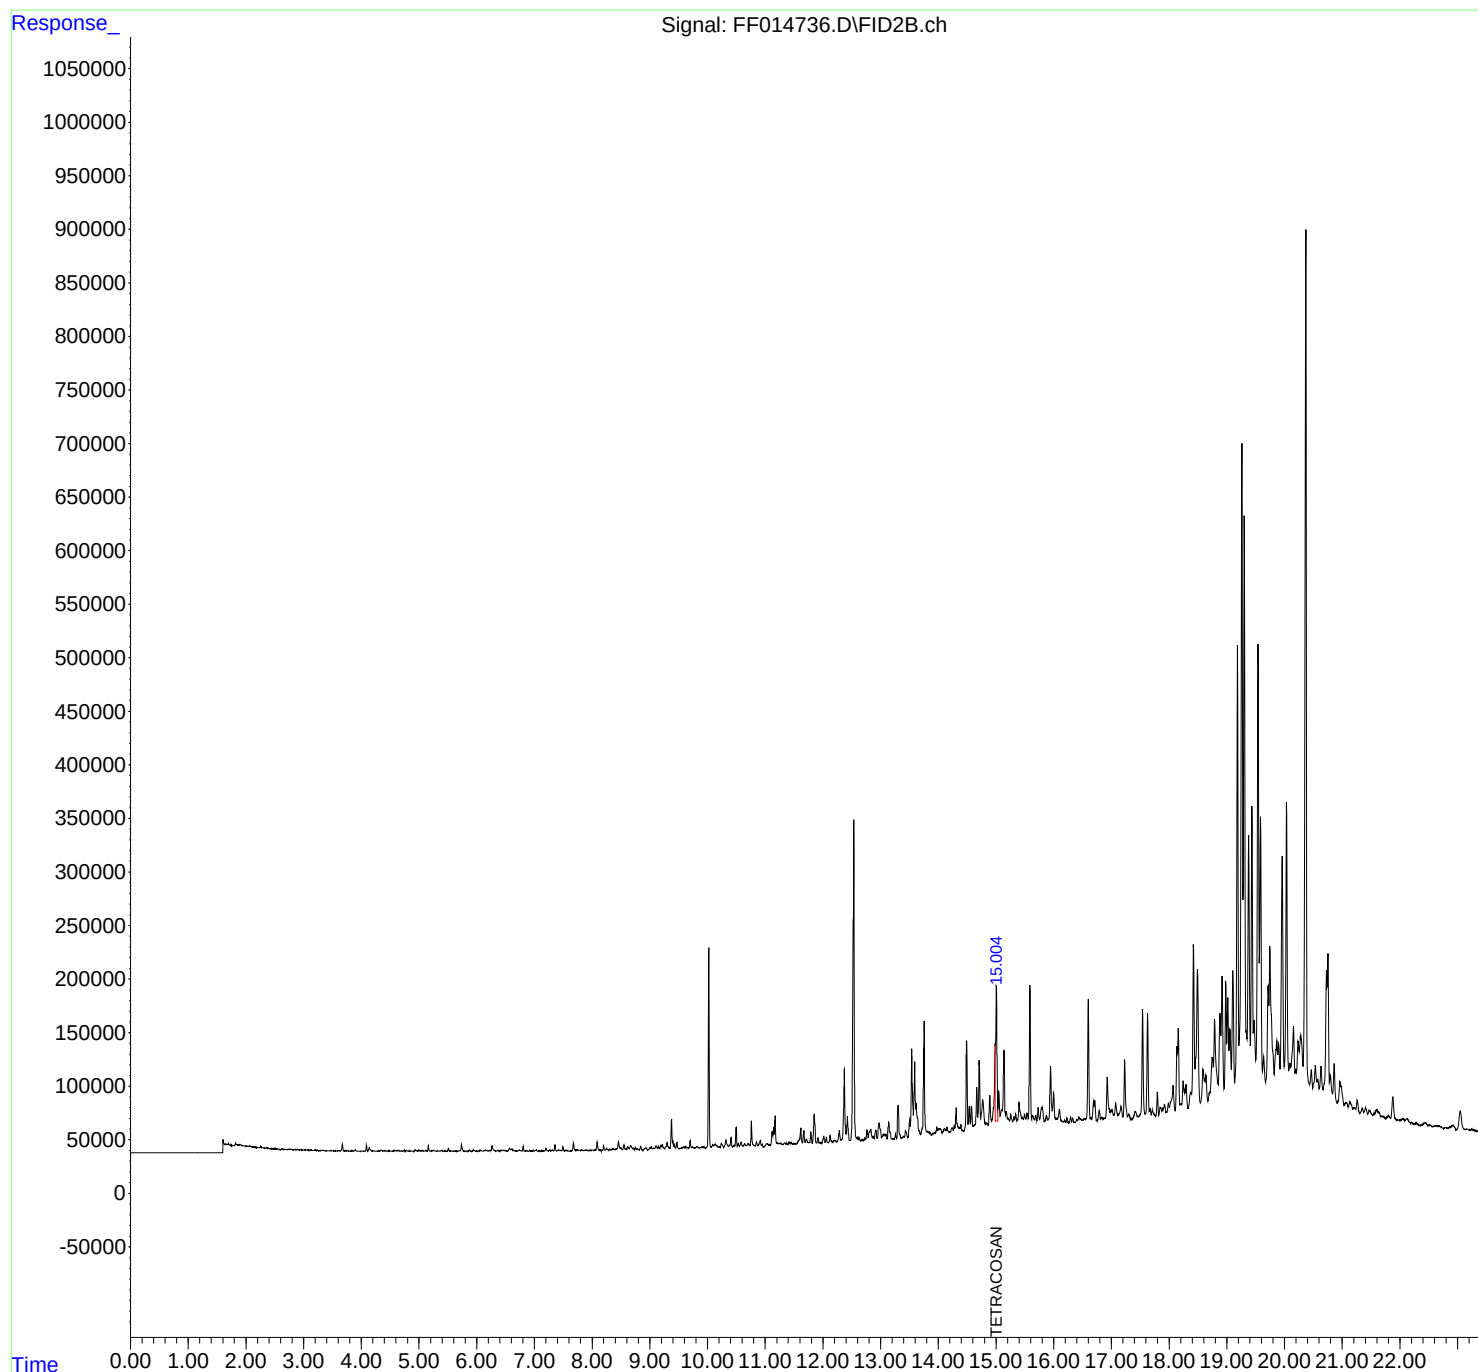

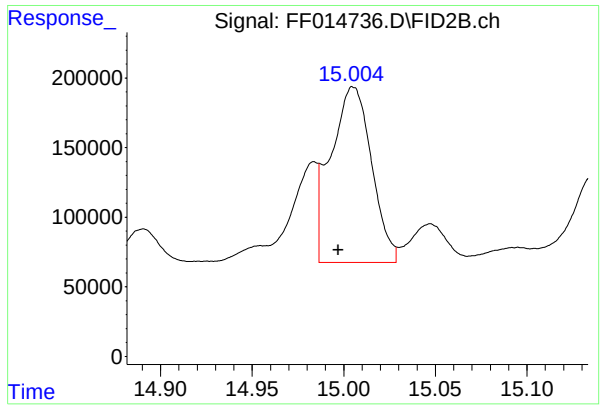

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.004 min
Delta R.T.: 0.007 min
Response: 1939756
Conc: 14.74 ug/ml

Instrument :
FID_F
ClientSampleId :
TS-1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :Ankita Jodhani 10/23/2024