

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102225\
Data File : FF016593.D
Signal(s) : FID2B.ch
Acq On : 22 Oct 2025 12:59
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 22 13:07:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102225.M
Quant Title :
QLast Update : Fri Oct 03 03:40:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.755	2015967	16.540 ug/ml
12)	N-OCTACOSANE	17.246	2025531	15.423 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102225\
Data File : FF016593.D
Signal(s) : FID2B.ch
Acq On : 22 Oct 2025 12:59
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 22 13:07:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102225.M
Quant Title :
QLast Update : Fri Oct 03 03:40:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

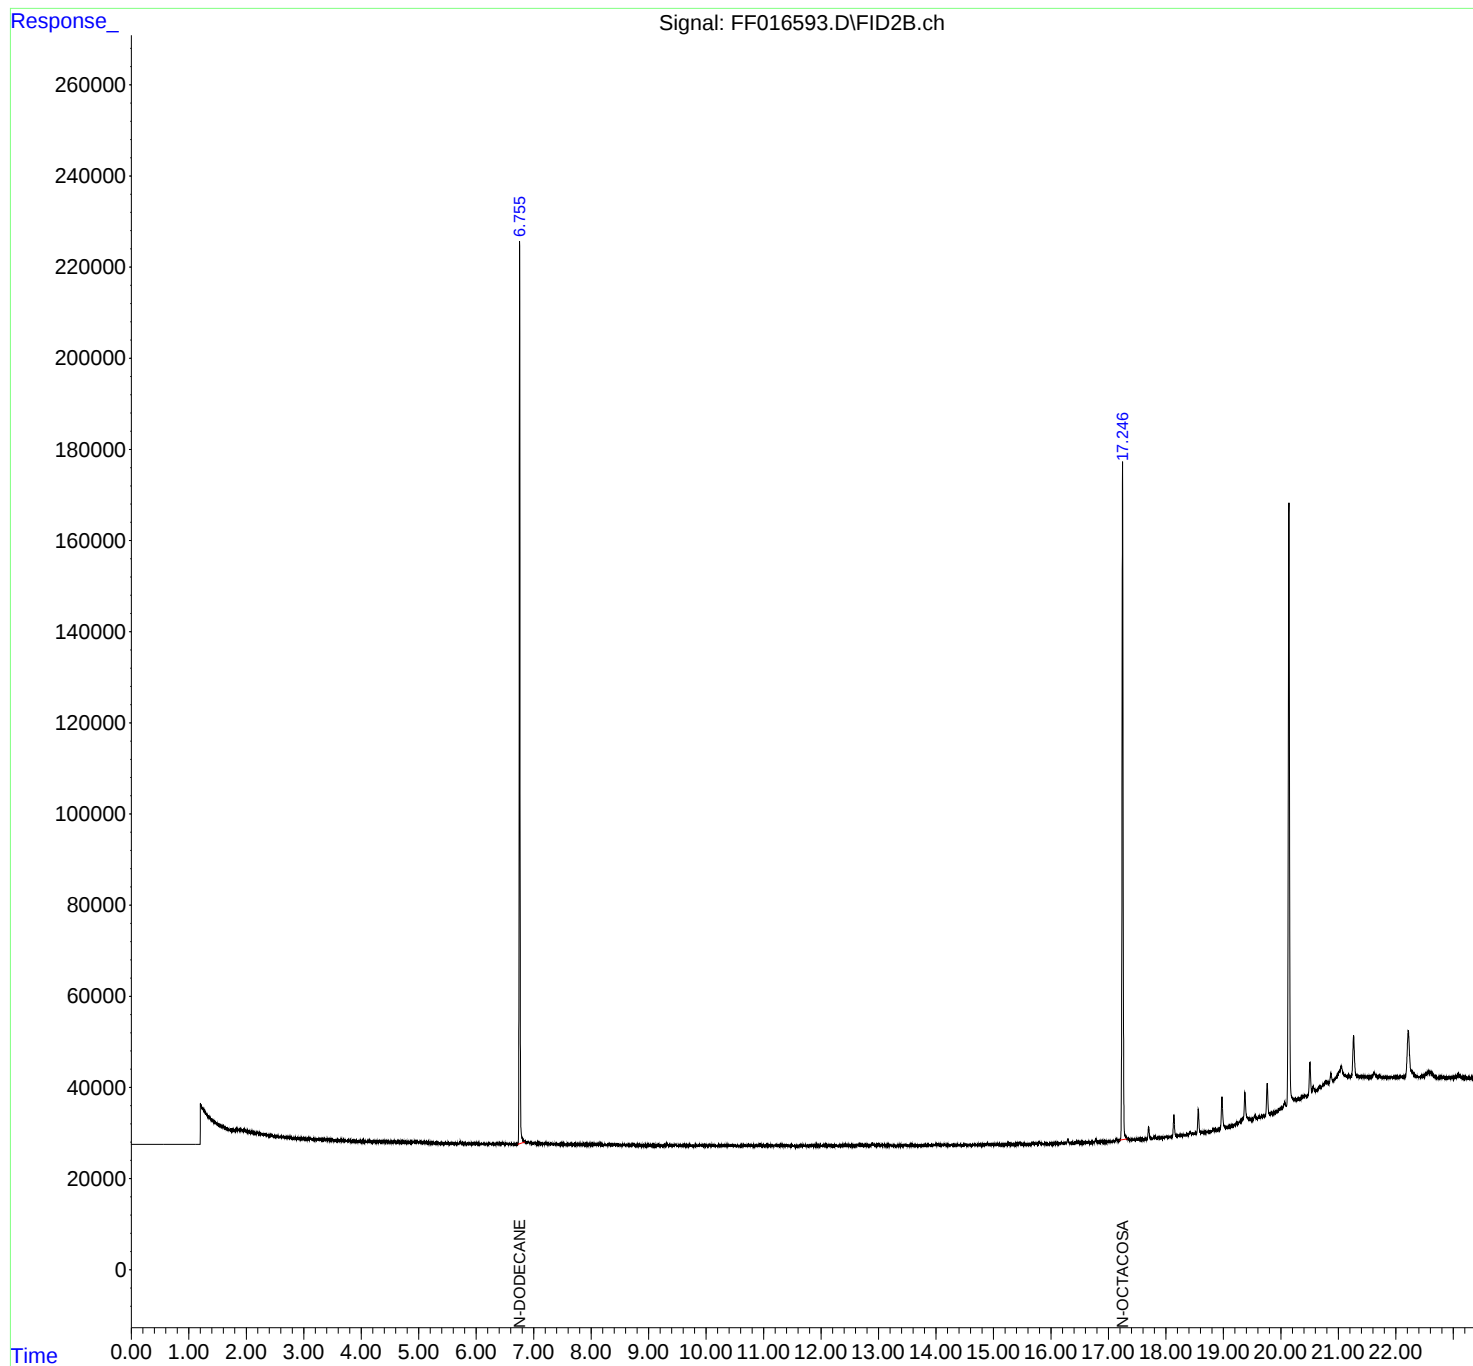


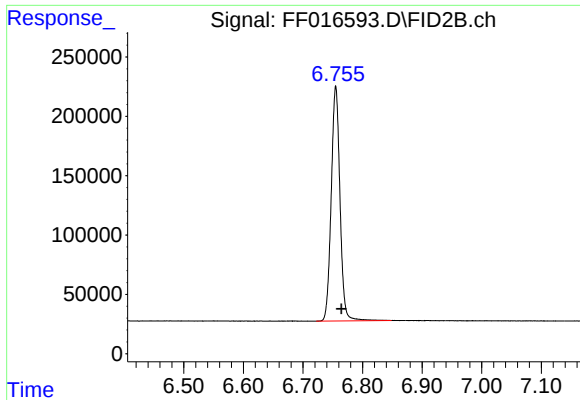

#3 N-DODECANE


R.T.: 6.755 min
Delta R.T.: -0.010 min
Response: 2015967
Conc: 16.54 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

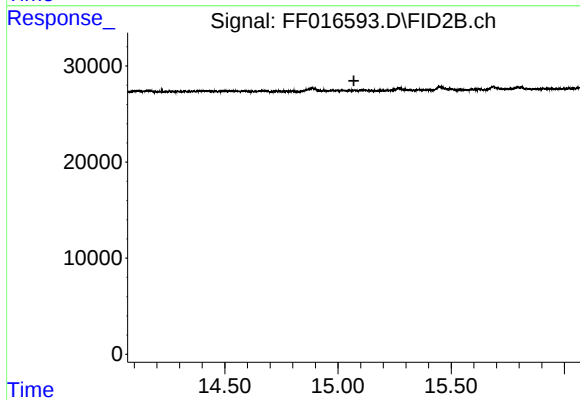

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.070 min
Response: 0
Conc: N.D.

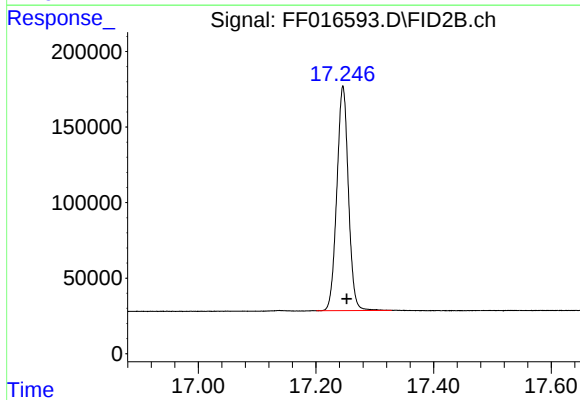

#12 N-OCTACOSANE

R.T.: 17.246 min
Delta R.T.: -0.006 min
Response: 2025531
Conc: 15.42 ug/ml