

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102225\
 Data File : FF016598.D
 Signal(s) : FID2B.ch
 Acq On : 22 Oct 2025 15:42
 Operator : YP\AJ
 Sample : Q3399-01MSD
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 COMP-ROLLOFFMSD

Integration File: autoint1.e
 Quant Time: Oct 23 01:20:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102225.M
 Quant Title :
 QLast Update : Fri Oct 03 03:40:27 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.061	1267907	10.780 ug/ml
Target Compounds			
2) N-DECANE	4.576	1663829	13.840 ug/ml
3) N-DODECANE	6.755	1766231	14.491 ug/ml
4) N-TETRADECANE	8.588	1822423	14.806 ug/ml
5) N-HEXADECANE	10.198	1916385	15.313 ug/ml
6) N-OCTADECANE	11.644	1948242	14.993 ug/ml
7) N-EICOSANE	12.958	2002721	15.019 ug/ml
8) N-DOCOSANE	14.159	1942208	14.817 ug/ml
10) N-TETRACOSANE	15.267	1906096	14.390 ug/ml
11) N-HEXACOSANE	16.291	1865851	14.128 ug/ml
12) N-OCTACOSANE	17.245	1861679	14.175 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102225\
Data File : FF016598.D
Signal(s) : FID2B.ch
Acq On : 22 Oct 2025 15:42
Operator : YP\AJ
Sample : Q3399-01MSD
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
COMP-ROLLOFFMSD

Integration File: autoint1.e
Quant Time: Oct 23 01:20:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102225.M
Quant Title :
QLast Update : Fri Oct 03 03:40:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

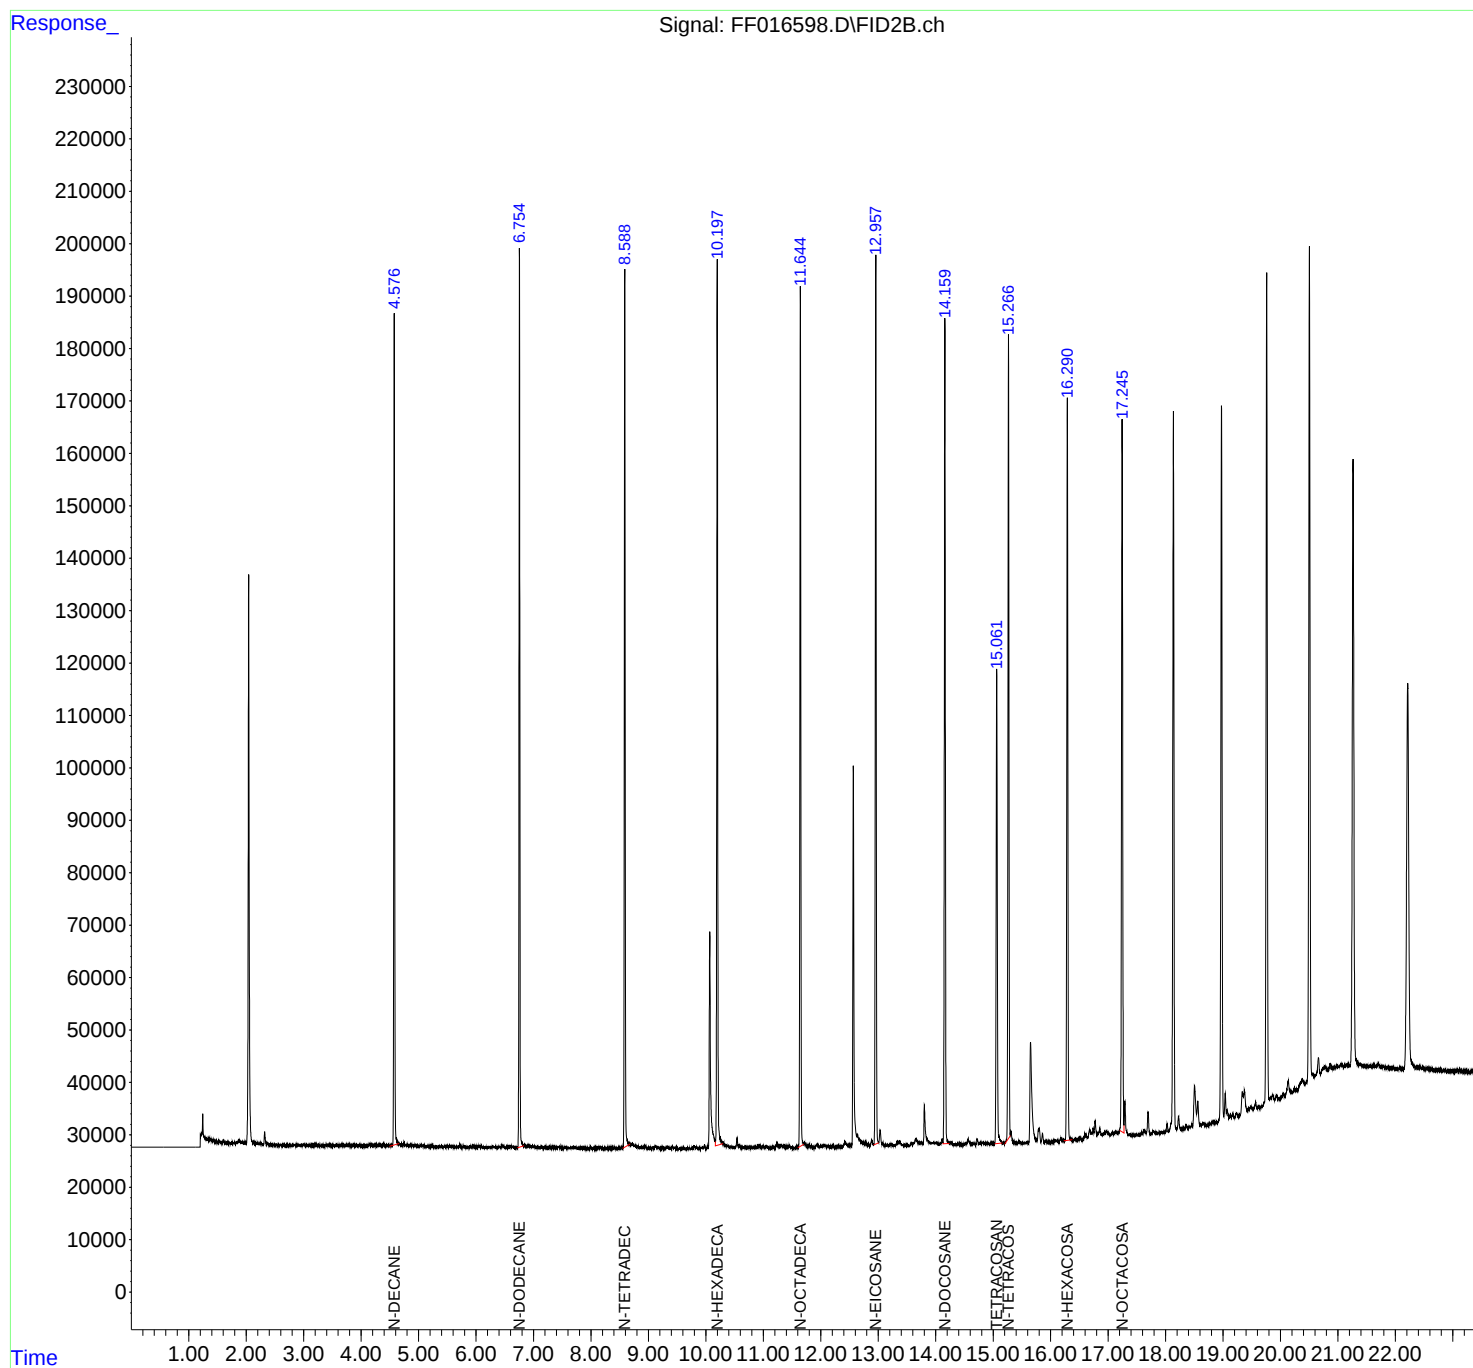


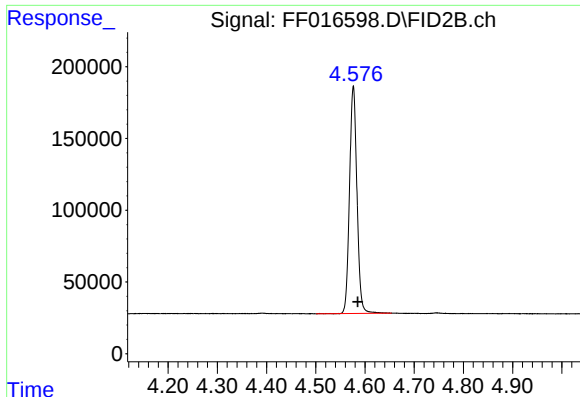

#2 N-DECANE


R.T.: 4.576 min
Delta R.T.: -0.009 min
Response: 1663829
Conc: 13.84 ug/ml

Instrument :
FID_F
ClientSampleId :
COMP-ROLLOFFMSD

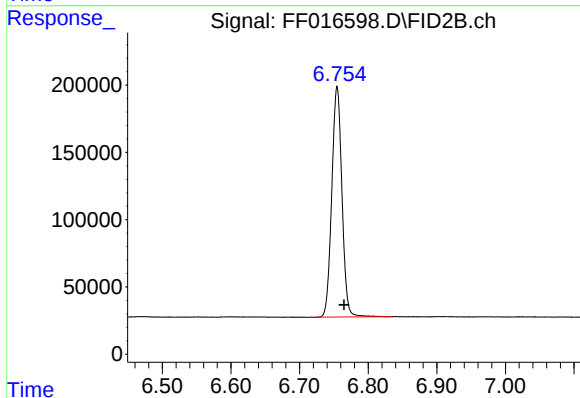


#3 N-DODECANE

R.T.: 6.755 min
Delta R.T.: -0.010 min
Response: 1766231
Conc: 14.49 ug/ml

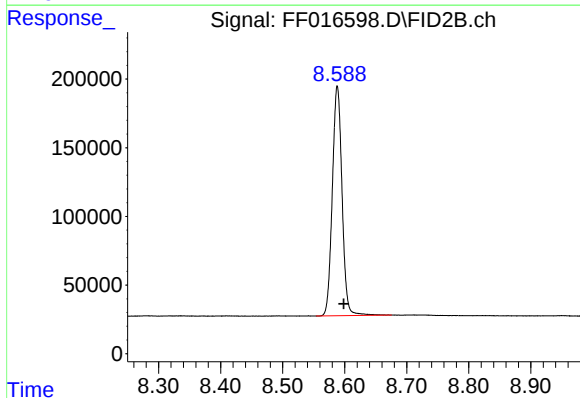


#4 N-TETRADECANE

R.T.: 8.588 min
Delta R.T.: -0.010 min
Response: 1822423
Conc: 14.81 ug/ml

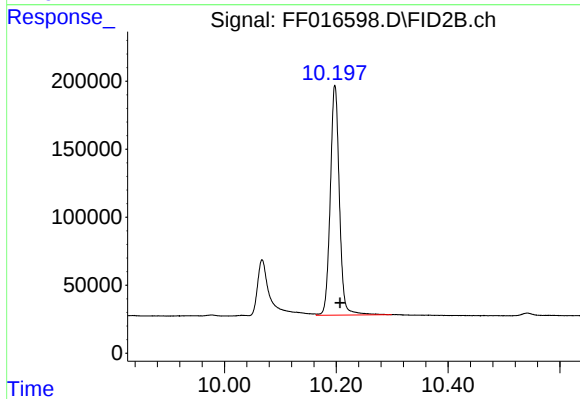

#5 N-HEXADECANE


R.T.: 10.198 min
Delta R.T.: -0.009 min
Response: 1916385
Conc: 15.31 ug/ml

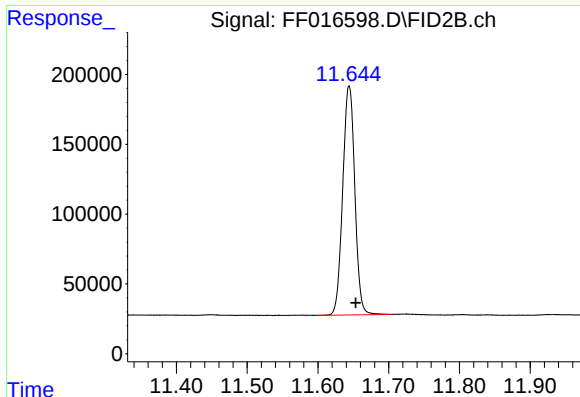

#6 N-OCTADECANE


R.T.: 11.644 min
Delta R.T.: -0.009 min
Response: 1948242
Conc: 14.99 ug/ml

Instrument :
FID_F
ClientSampleId :
COMP-ROLLOFFMSD

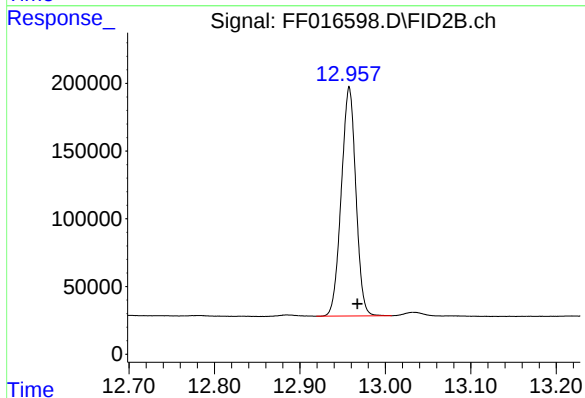


#7 N-EICOSANE

R.T.: 12.958 min
Delta R.T.: -0.010 min
Response: 2002721
Conc: 15.02 ug/ml

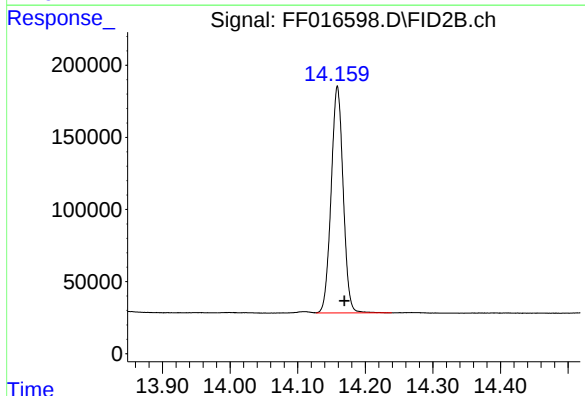


#8 N-DOCOSANE

R.T.: 14.159 min
Delta R.T.: -0.010 min
Response: 1942208
Conc: 14.82 ug/ml

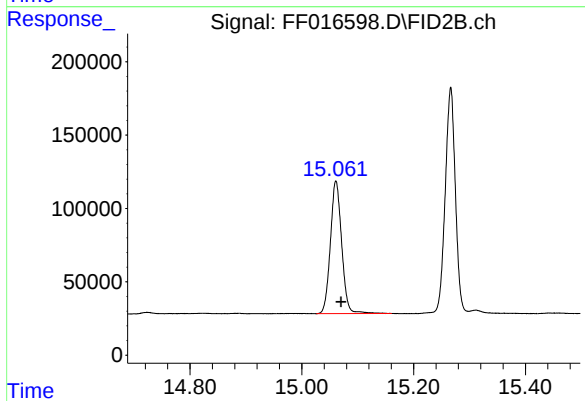

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.061 min
Delta R.T.: -0.009 min
Response: 1267907
Conc: 10.78 ug/ml

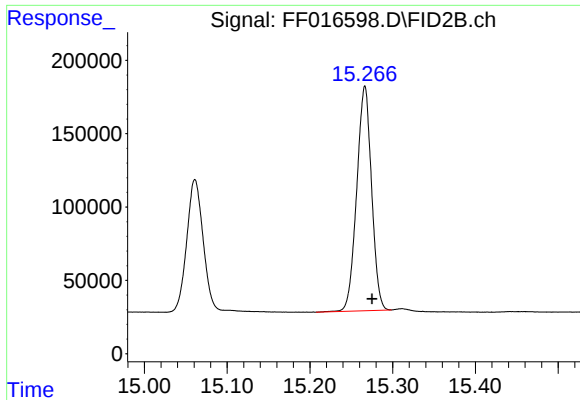

#10 N-TETRACOSANE


R.T.: 15.267 min
Delta R.T.: -0.009 min
Response: 1906096
Conc: 14.39 ug/ml

Instrument :
FID_F
ClientSampleId :
COMP-ROLLOFFMSD

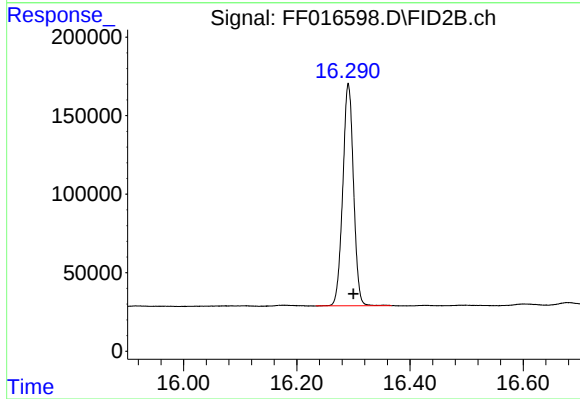

#11 N-HEXACOSANE

R.T.: 16.291 min
Delta R.T.: -0.009 min
Response: 1865851
Conc: 14.13 ug/ml

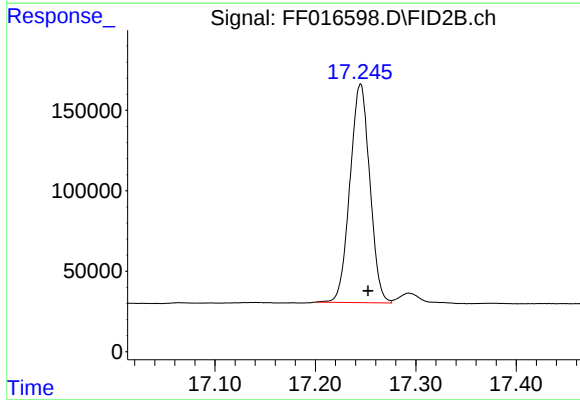

#12 N-OCTACOSANE

R.T.: 17.245 min
Delta R.T.: -0.007 min
Response: 1861679
Conc: 14.18 ug/ml