

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102418\
 Data File : FF002456.D
 Signal(s) : FID2B.ch
 Acq On : 24 Oct 2018 11:02
 Operator : AJ\SJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 25 03:39:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
 Quant Title :
 QLast Update : Fri Oct 12 13:21:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.665	23426433	168.546 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.183	25790143	164.811 ug/ml
5)	N-HEXADECANE	9.804	26255918	167.057 ug/ml
6)	N-OCTADECANE	11.251	26562660	167.141 ug/ml
7)	N-EICOSANE	12.563	26475923	167.160 ug/ml
8)	N-DOCOSANE	13.764	26401879	167.350 ug/ml
10)	N-TETRACOSANE	14.871	26259523	167.845 ug/ml
11)	N-HEXACOSANE	15.895	26265606	168.678 ug/ml
12)	N-OCTACOSANE	16.847	26140374	168.522 ug/ml
13)	N-TRIACONTANE	17.737	26052773	167.870 ug/ml
14)	N-DOTRIACONTANE	18.571	25213491	162.609 ug/ml
15)	N-TETRATRIACONTANE	19.356	24114476	163.720 ug/ml
16)	N-HEXATRIACONTANE	20.098	21462242	156.464 ug/ml
17)	N-OCTATRIACONTANE	20.840	16958271	140.300 ug/ml
18)	N-TETRACONTANE	21.751	13916597	116.814 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102418\
Data File : FF002456.D
Signal(s) : FID2B.ch
Acq On : 24 Oct 2018 11:02
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 25 03:39:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

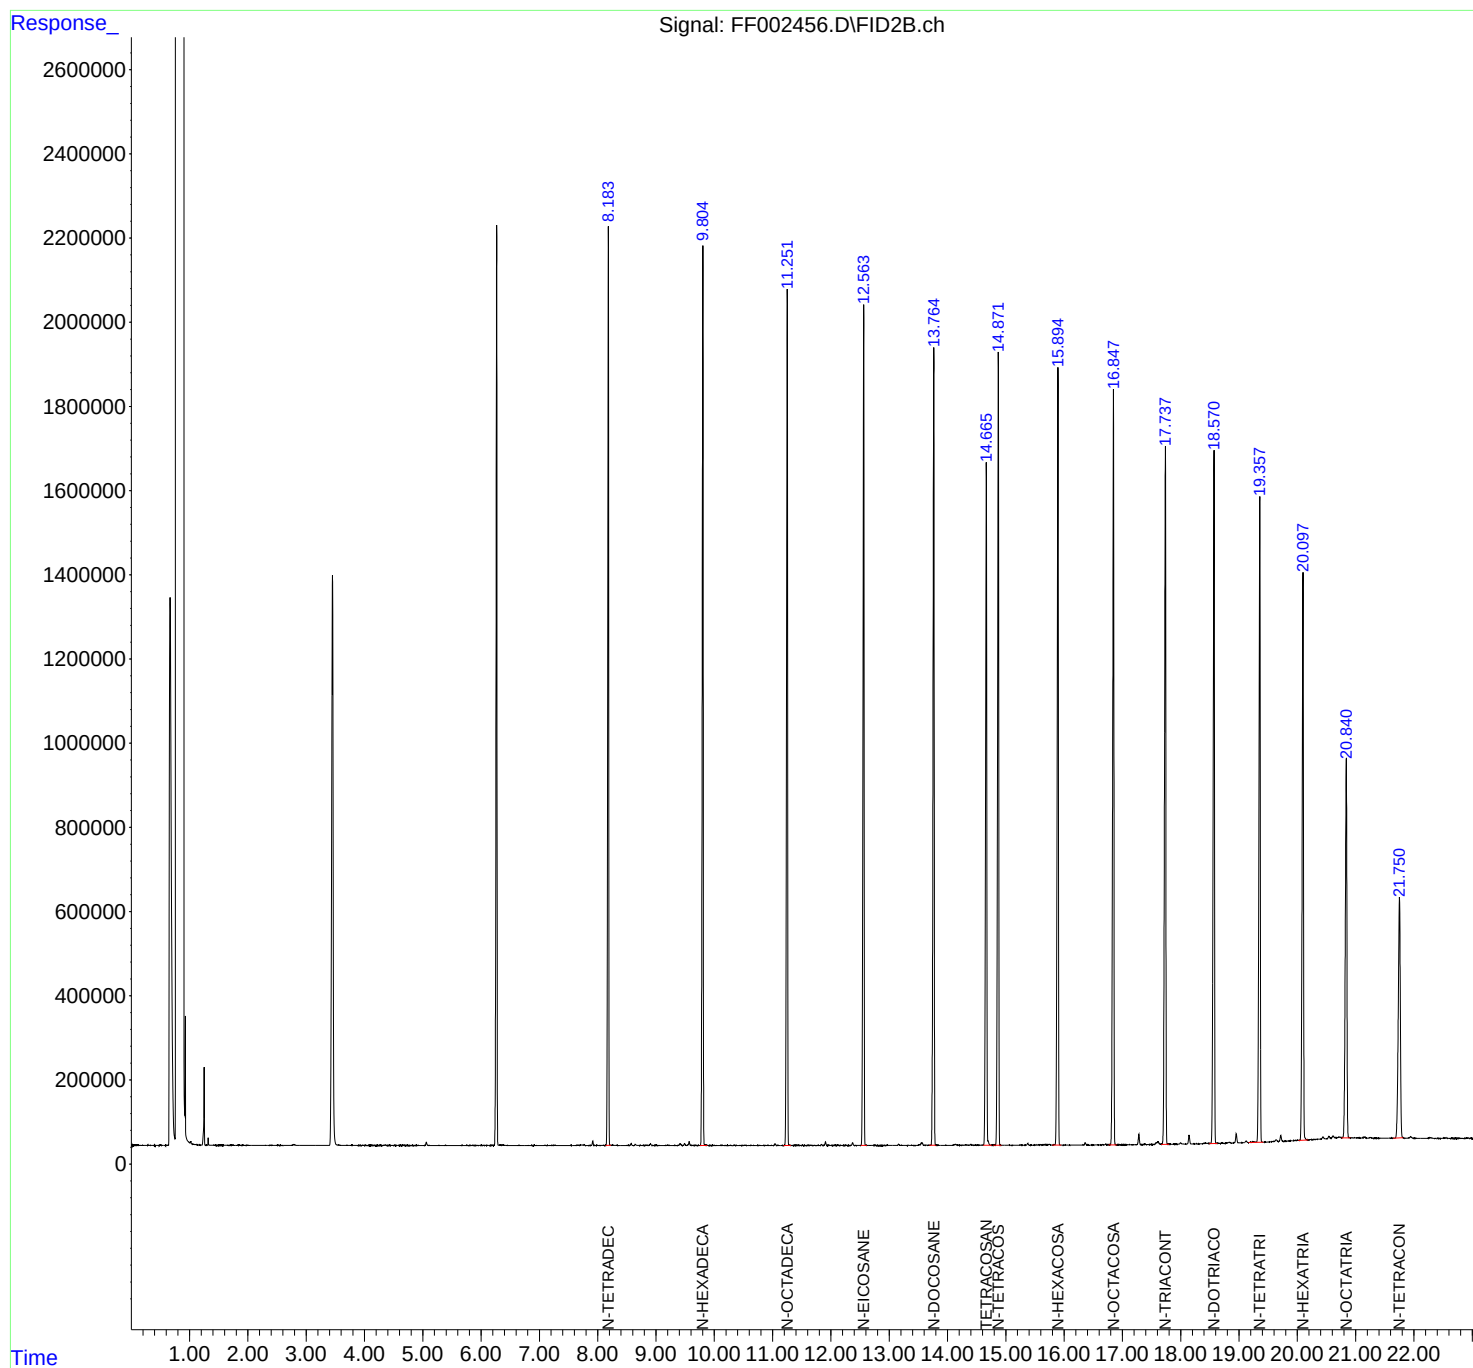

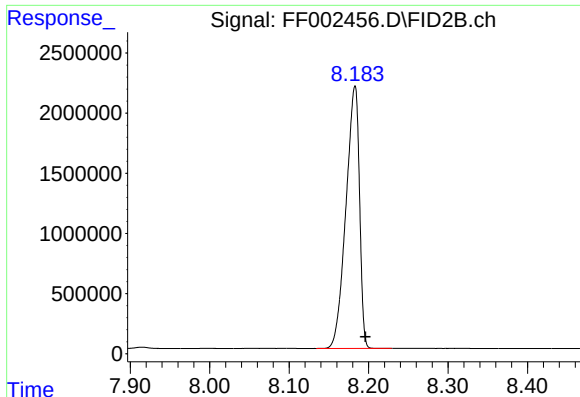


#4 N-TETRADECANE

R.T.: 8.183 min
Delta R.T.: -0.013 min
Response: 25790143
Conc: 164.81 ug/ml

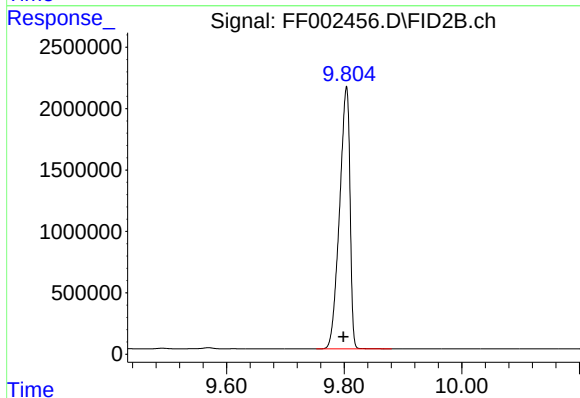


#5 N-HEXADECANE

R.T.: 9.804 min
Delta R.T.: 0.005 min
Response: 26255918
Conc: 167.06 ug/ml

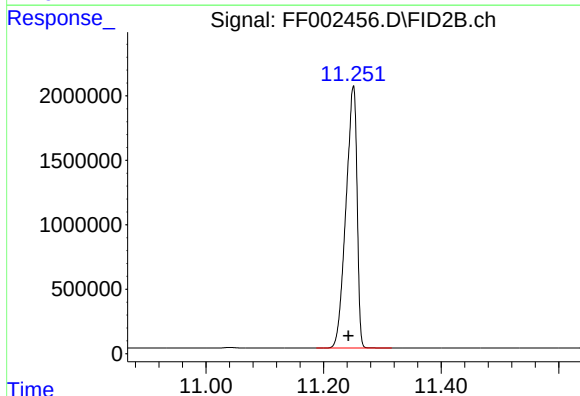


#6 N-OCTADECANE

R.T.: 11.251 min
Delta R.T.: 0.008 min
Response: 26562660
Conc: 167.14 ug/ml

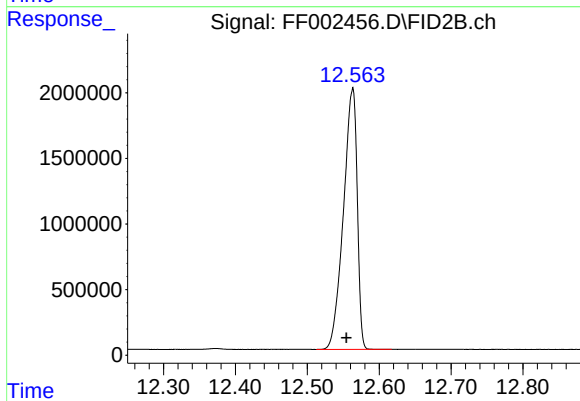


#7 N-EICOSANE

R.T.: 12.563 min
Delta R.T.: 0.009 min
Response: 26475923
Conc: 167.16 ug/ml

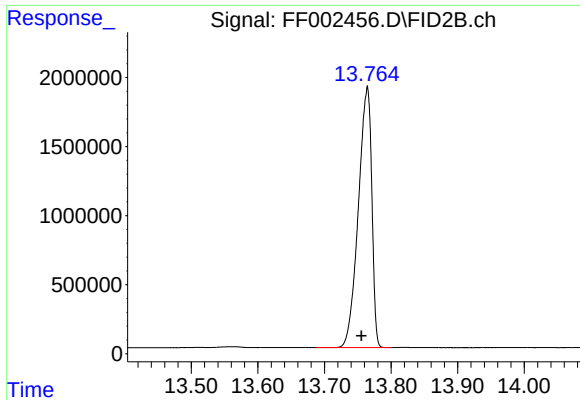


#8 N-DOCOSANE

R.T.: 13.764 min
Delta R.T.: 0.009 min
Response: 26401879
Conc: 167.35 ug/ml

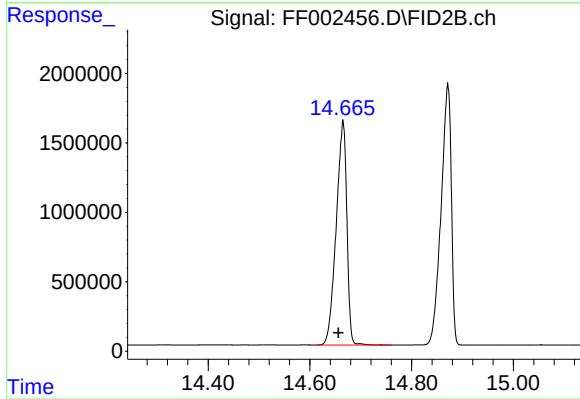


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.665 min
Delta R.T.: 0.009 min
Response: 23426433
Conc: 168.55 ug/ml

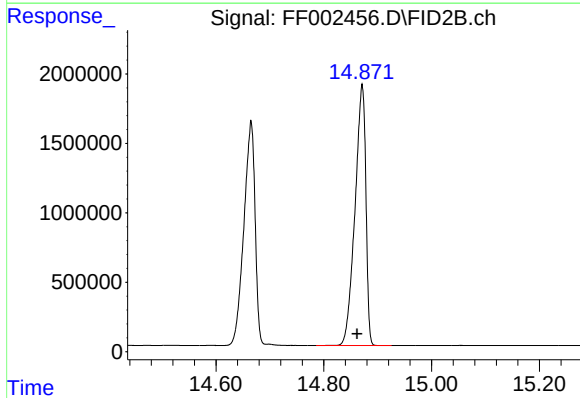


#10 N-TETRACOSANE

R.T.: 14.871 min
Delta R.T.: 0.009 min
Response: 26259523
Conc: 167.84 ug/ml

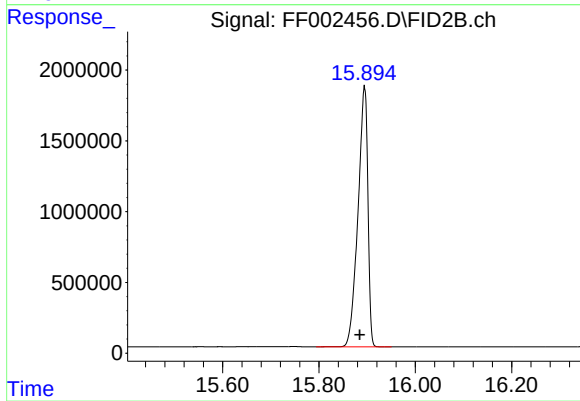


#11 N-HEXACOSANE

R.T.: 15.895 min
Delta R.T.: 0.010 min
Response: 26265606
Conc: 168.68 ug/ml

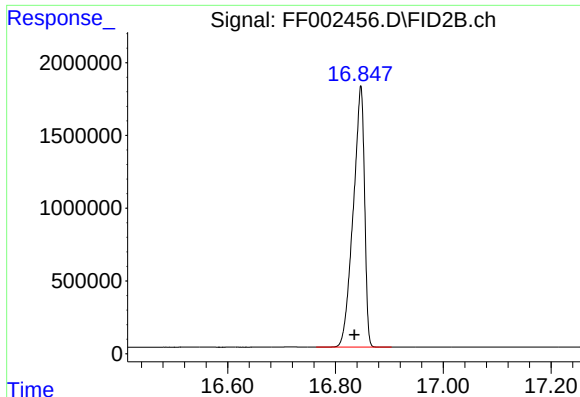


#12 N-OCTACOSANE

R.T.: 16.847 min
Delta R.T.: 0.012 min
Response: 26140374
Conc: 168.52 ug/ml

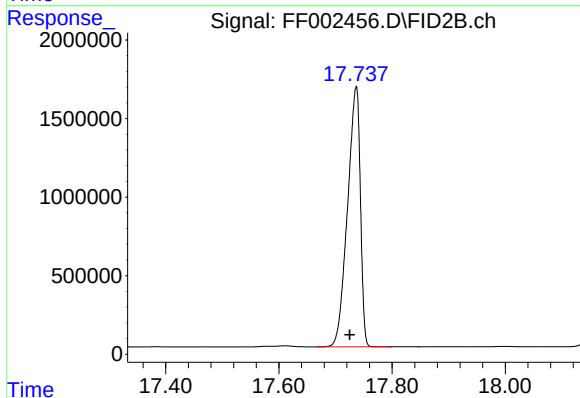


#13 N-TRIACONTANE

R.T.: 17.737 min
Delta R.T.: 0.012 min
Response: 26052773
Conc: 167.87 ug/ml

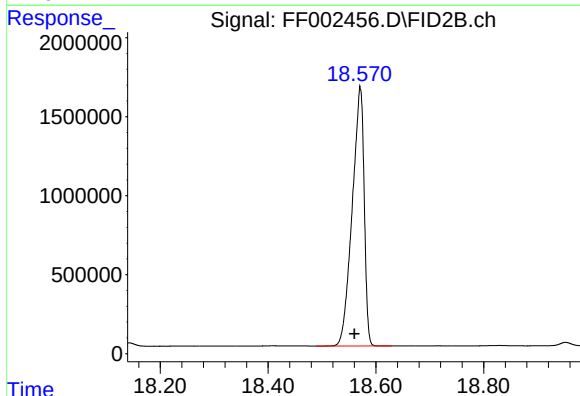


#14 N-DOTRIACONTANE

R.T.: 18.571 min
Delta R.T.: 0.011 min
Response: 25213491
Conc: 162.61 ug/ml

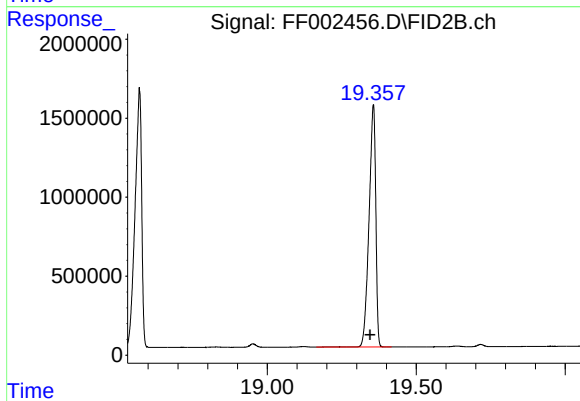


#15 N-TETRATRIACONTANE

R.T.: 19.356 min
Delta R.T.: 0.011 min
Response: 24114476
Conc: 163.72 ug/ml

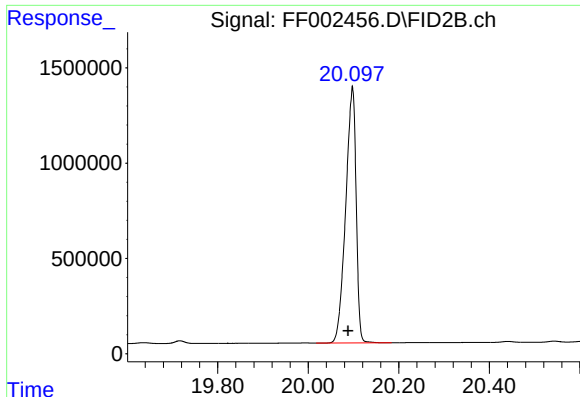


#16 N-HEXATRIACONTANE

R.T.: 20.098 min
Delta R.T.: 0.010 min
Response: 21462242
Conc: 156.46 ug/ml

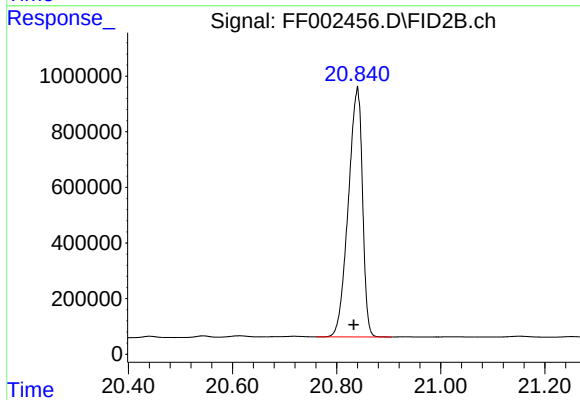

#17 N-OCTATRIACONTANE

R.T.: 20.840 min
Delta R.T.: 0.007 min
Response: 16958271
Conc: 140.30 ug/ml

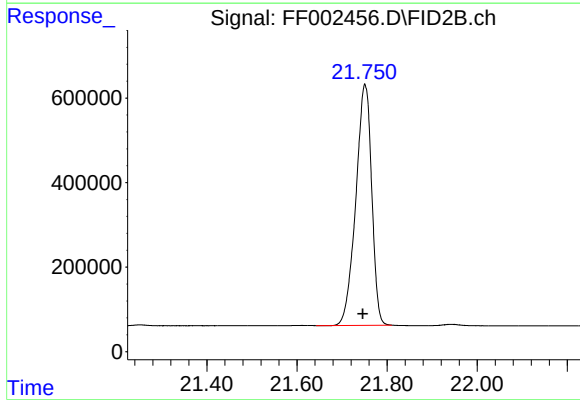

#18 N-TETRACONTANE

R.T.: 21.751 min
Delta R.T.: 0.005 min
Response: 13916597
Conc: 116.81 ug/ml