

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102418\
 Data File : FF002467.D
 Signal(s) : FID2B.ch
 Acq On : 24 Oct 2018 16:46
 Operator : AJ\SJ
 Sample : J5198-25 10X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 25 03:42:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
 Quant Title :
 QLast Update : Fri Oct 12 13:21:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.657	188258	1.354 ug/ml
Target Compounds				
7)	N-EICOSANE	12.610f	988536	6.241 ug/ml
8)	N-DOCOSANE	13.776	162760	1.032 ug/ml
10)	N-TETRACOSANE	14.830	503403	3.218 ug/ml
12)	N-OCTACOSANE	16.833	224804	1.449 ug/ml
13)	N-TRIACONTANE	17.727	319523	2.059 ug/ml
14)	N-DOTRIACONTANE	18.558	176065	1.135 ug/ml
15)	N-TETRATRIACONTANE	19.350	502534	3.412 ug/ml
16)	N-HEXATRIACONTANE	20.107	965326	7.037 ug/ml
17)	N-OCTATRIACONTANE	20.806	1279730	10.588 ug/ml
18)	N-TETRACONTANE	21.768	66073	0.555 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102418\
Data File : FF002467.D
Signal(s) : FID2B.ch
Acq On : 24 Oct 2018 16:46
Operator : AJ\SJ
Sample : J5198-25 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 25 03:42:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

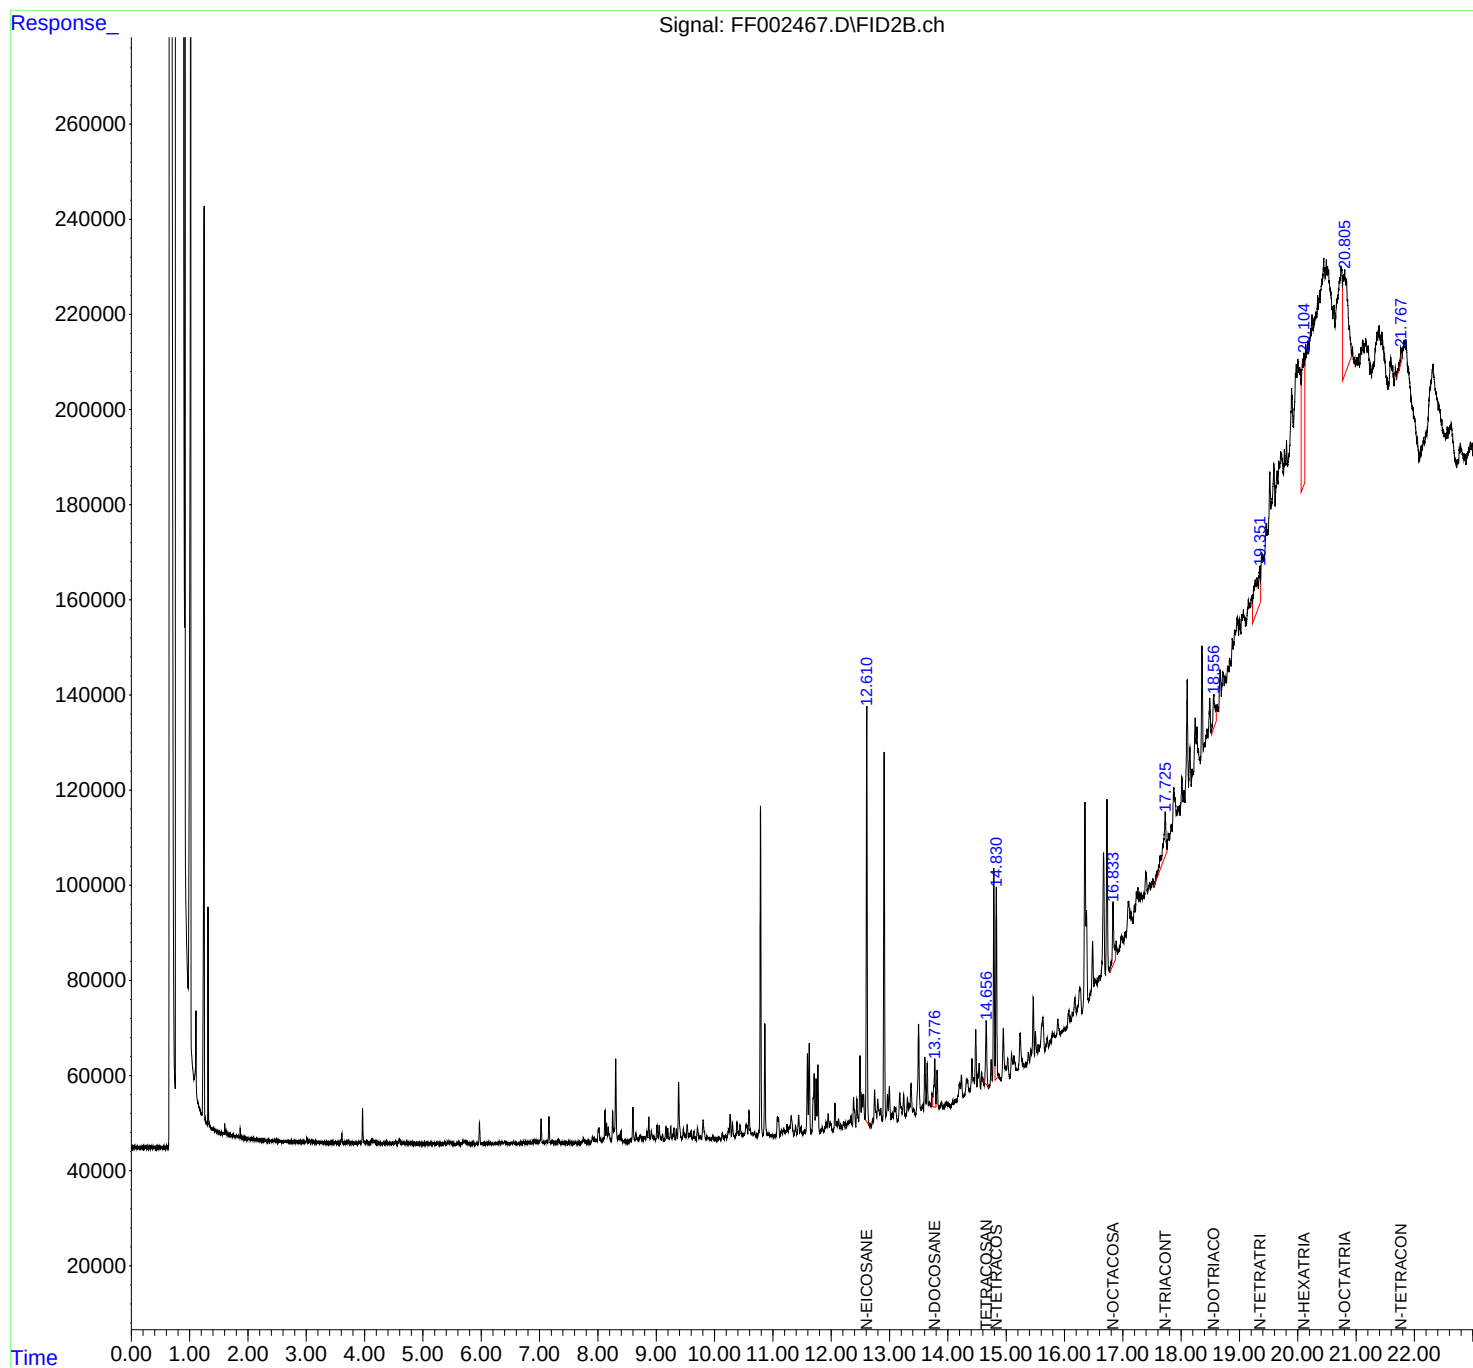

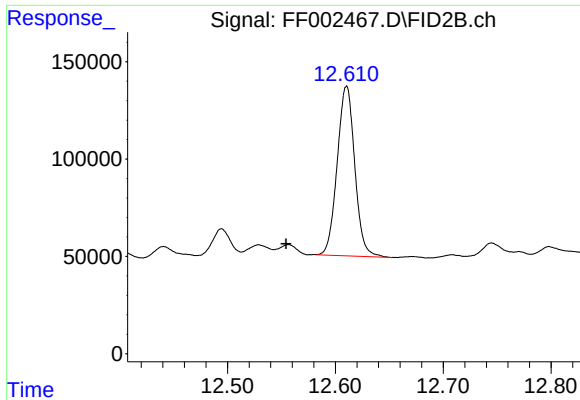


#7 N-EICOSANE

R.T.: 12.610 min
Delta R.T.: 0.056 min
Response: 988536
Conc: 6.24 ug/ml

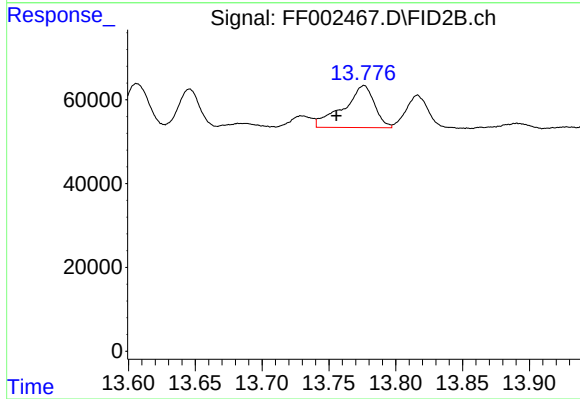


#8 N-DOCOSANE

R.T.: 13.776 min
Delta R.T.: 0.021 min
Response: 162760
Conc: 1.03 ug/ml

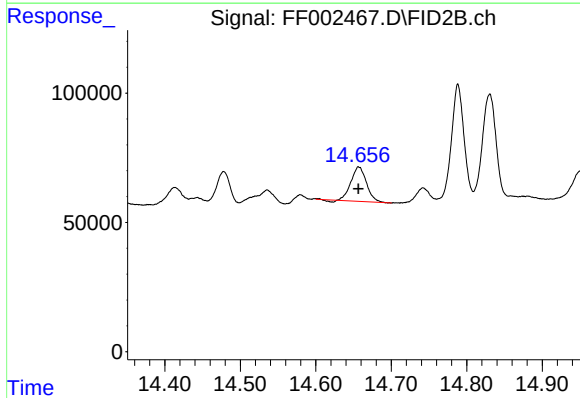


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.657 min
Delta R.T.: 0.000 min
Response: 188258
Conc: 1.35 ug/ml

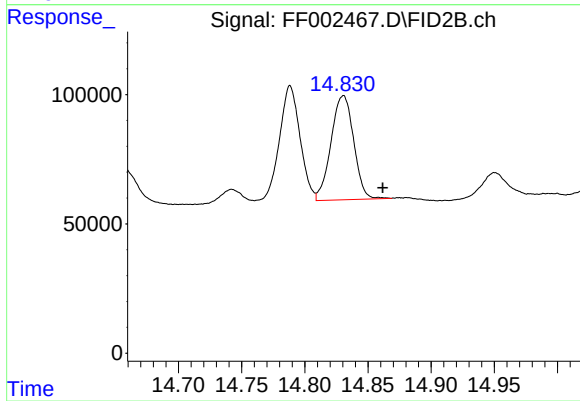


#10 N-TETRACOSANE

R.T.: 14.830 min
Delta R.T.: -0.031 min
Response: 503403
Conc: 3.22 ug/ml

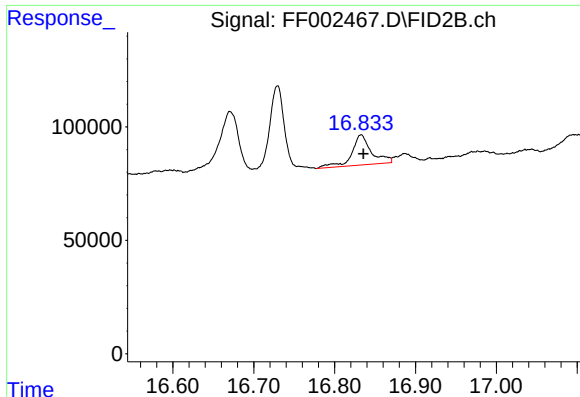


#12 N-OCTACOSANE

R.T.: 16.833 min
Delta R.T.: -0.003 min
Response: 224804
Conc: 1.45 ug/ml

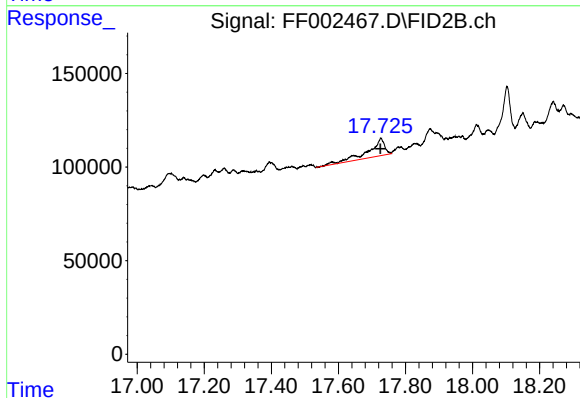


#13 N-TRIACONTANE

R.T.: 17.727 min
Delta R.T.: 0.002 min
Response: 319523
Conc: 2.06 ug/ml

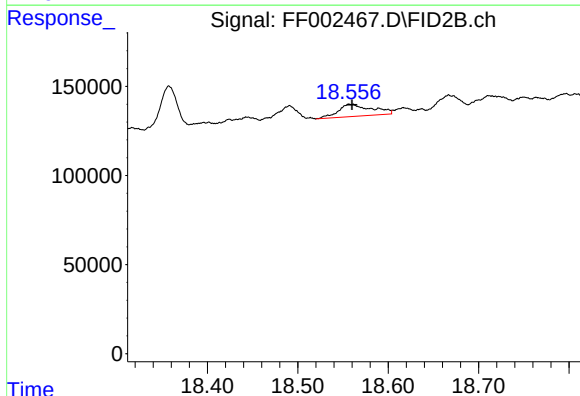


#14 N-DOTRIACONTANE

R.T.: 18.558 min
Delta R.T.: -0.002 min
Response: 176065
Conc: 1.14 ug/ml

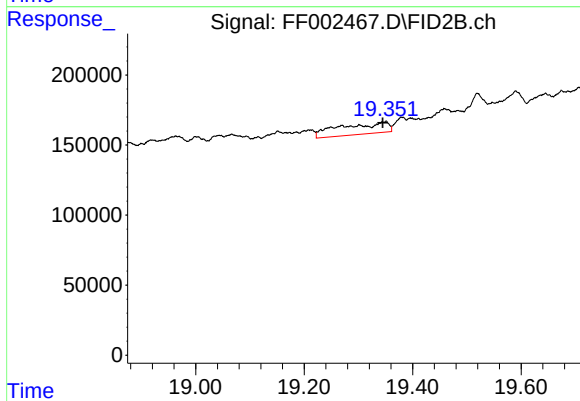


#15 N-TETRATRIACONTANE

R.T.: 19.350 min
Delta R.T.: 0.004 min
Response: 502534
Conc: 3.41 ug/ml

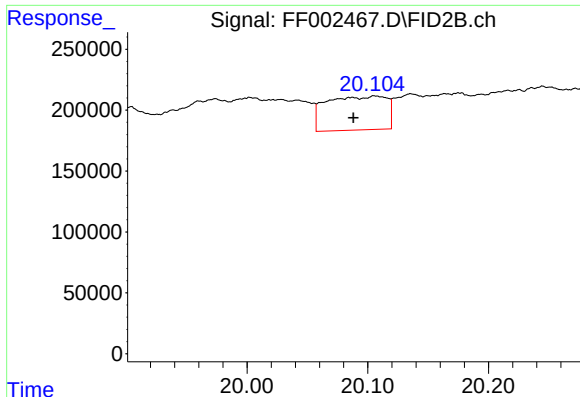


#16 N-HEXATRIACONTANE

R.T.: 20.107 min
Delta R.T.: 0.019 min
Response: 965326
Conc: 7.04 ug/ml

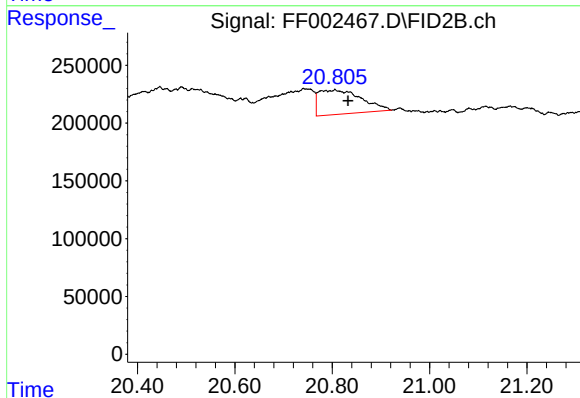

#17 N-OCTATRIACONTANE

R.T.: 20.806 min
Delta R.T.: -0.027 min
Response: 1279730
Conc: 10.59 ug/ml

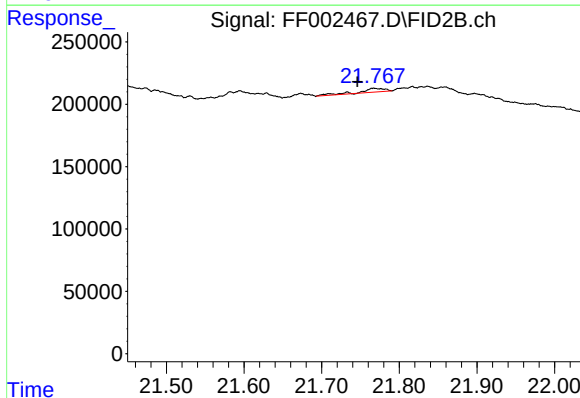

#18 N-TETRACONTANE

R.T.: 21.768 min
Delta R.T.: 0.021 min
Response: 66073
Conc: 0.55 ug/ml