

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102418\
 Data File : FF002473.D
 Signal(s) : FID2B.ch
 Acq On : 24 Oct 2018 19:51
 Operator : AJ\SJ
 Sample : J5610-01 5X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 25 03:43:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
 Quant Title :
 QLast Update : Fri Oct 12 13:21:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.656	259065	1.864 ug/ml
Target Compounds			
4) N-TETRADECANE	8.253f	121479	0.776 ug/ml
5) N-HEXADECANE	9.800	107245	0.682 ug/ml
7) N-EICOSANE	12.607f	314289	1.984 ug/ml
10) N-TETRACOSANE	14.828	126887	0.811 ug/ml
11) N-HEXACOSANE	15.883	151922	0.976 ug/ml
12) N-OCTACOSANE	16.833	257995	1.663 ug/ml
13) N-TRIACONTANE	17.724	260002	1.675 ug/ml
14) N-DOTRIACONTANE	18.559	171013	1.103 ug/ml
15) N-TETRATRIACONTANE	19.343	119515	0.811 ug/ml
16) N-HEXATRIACONTANE	20.089	301211	2.196 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102418\
Data File : FF002473.D
Signal(s) : FID2B.ch
Acq On : 24 Oct 2018 19:51
Operator : AJ\SJ
Sample : J5610-01 5X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 25 03:43:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

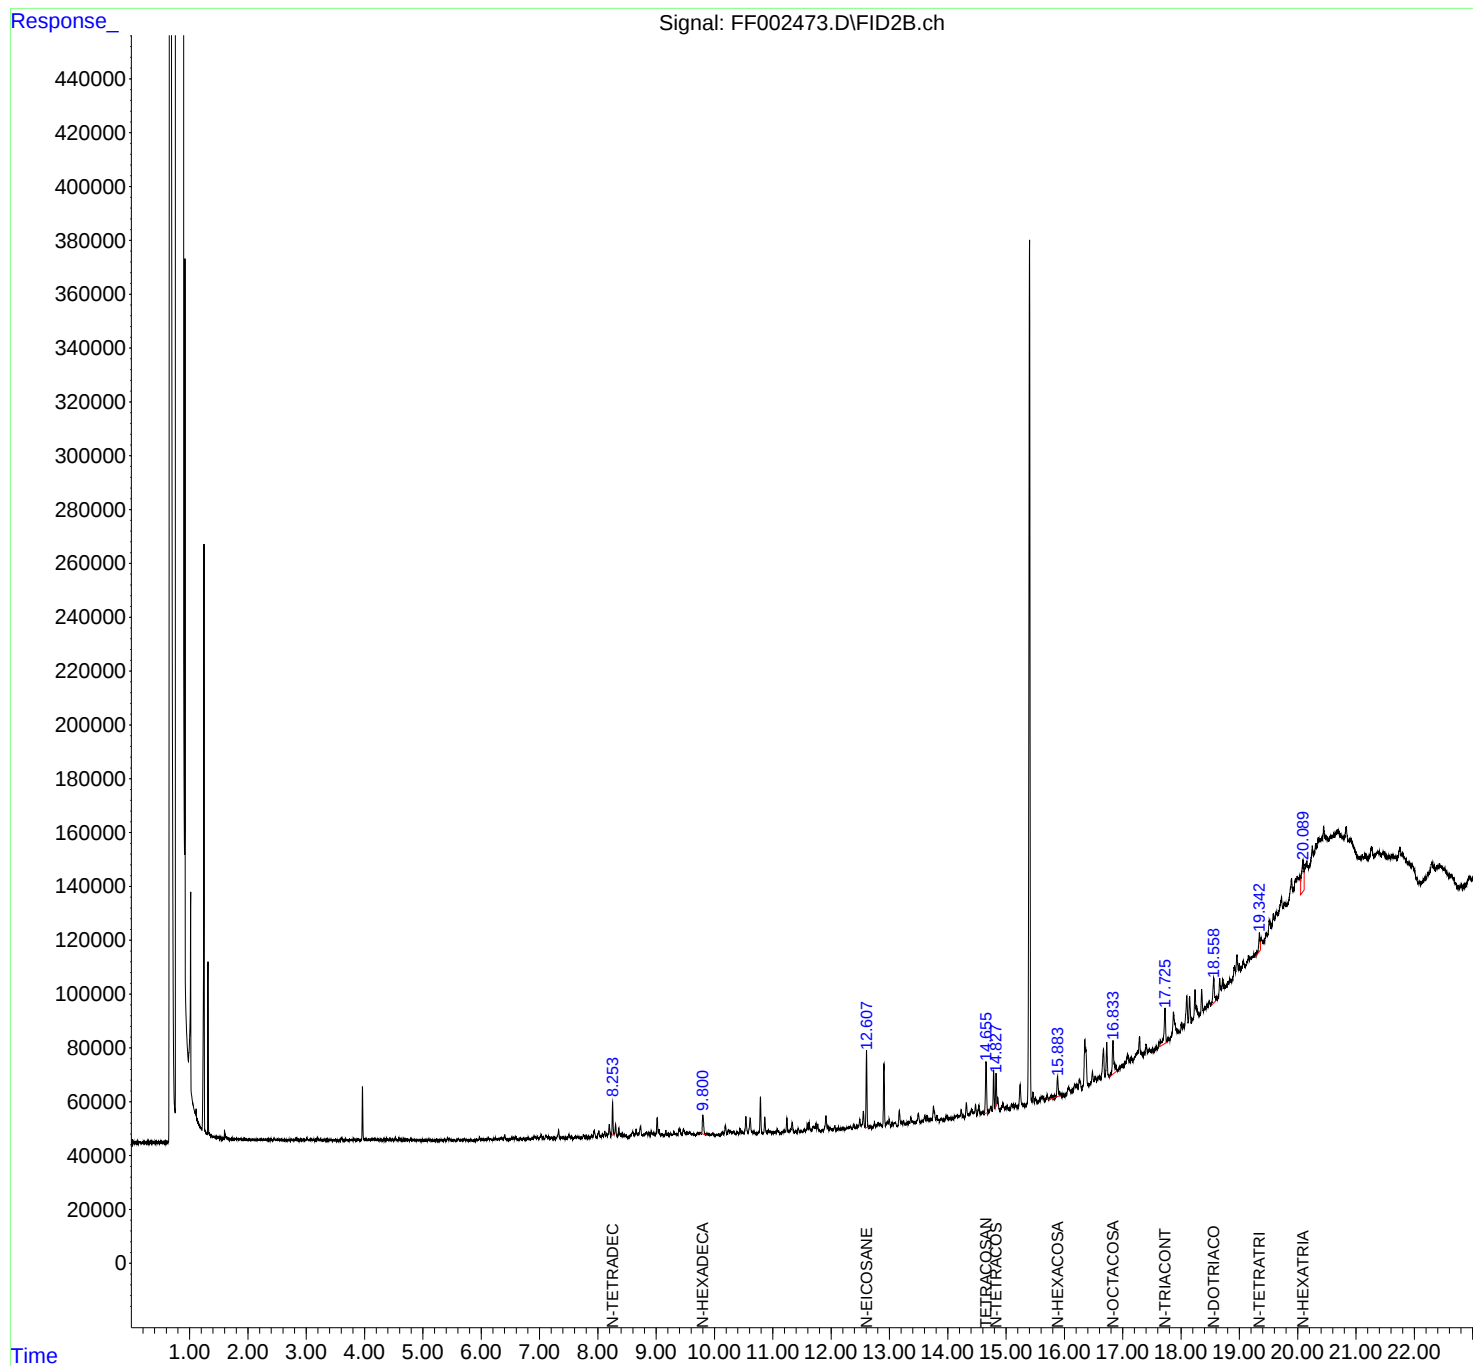

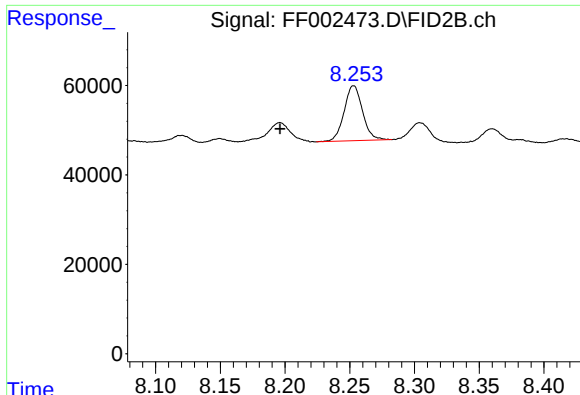


#4 N-TETRADECANE

R.T.: 8.253 min
Delta R.T.: 0.057 min
Response: 121479
Conc: 0.78 ug/ml

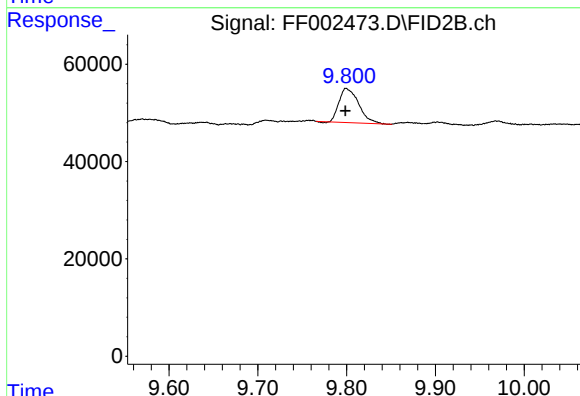


#5 N-HEXADECANE

R.T.: 9.800 min
Delta R.T.: 0.000 min
Response: 107245
Conc: 0.68 ug/ml

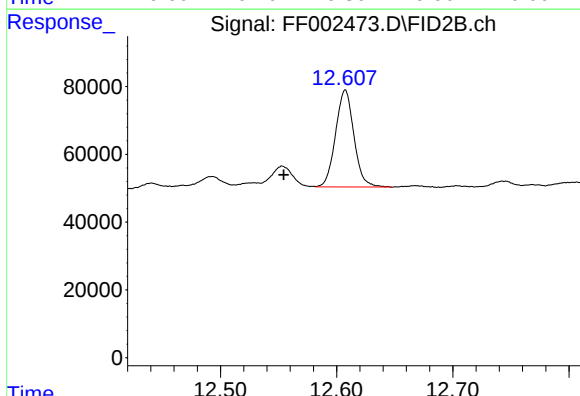


#7 N-EICOSANE

R.T.: 12.607 min
Delta R.T.: 0.053 min
Response: 314289
Conc: 1.98 ug/ml

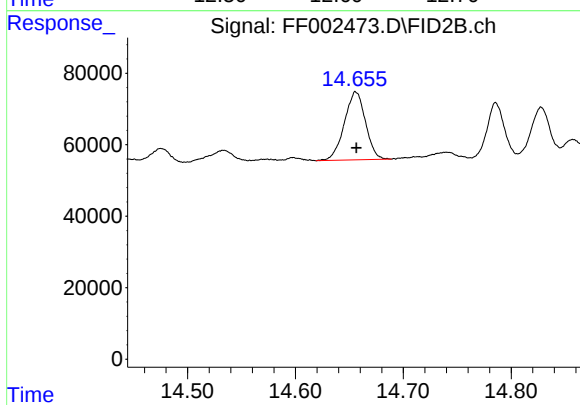


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.656 min
Delta R.T.: 0.000 min
Response: 259065
Conc: 1.86 ug/ml

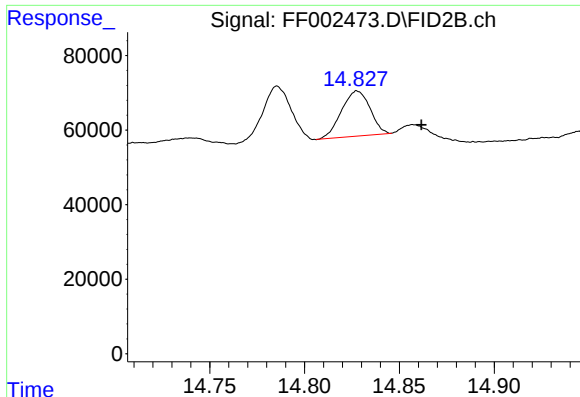


#10 N-TETRACOSANE

R.T.: 14.828 min
Delta R.T.: -0.034 min
Response: 126887
Conc: 0.81 ug/ml

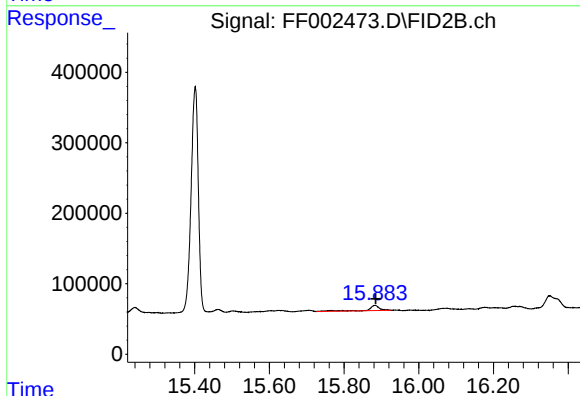


#11 N-HEXACOSANE

R.T.: 15.883 min
Delta R.T.: -0.002 min
Response: 151922
Conc: 0.98 ug/ml

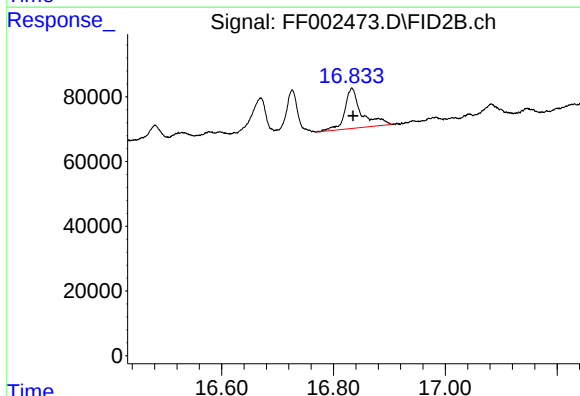


#12 N-OCTACOSANE

R.T.: 16.833 min
Delta R.T.: -0.002 min
Response: 257995
Conc: 1.66 ug/ml

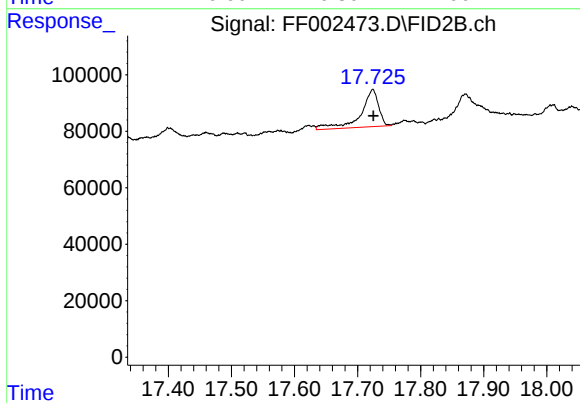


#13 N-TRIACONTANE

R.T.: 17.724 min
Delta R.T.: 0.000 min
Response: 260002
Conc: 1.68 ug/ml

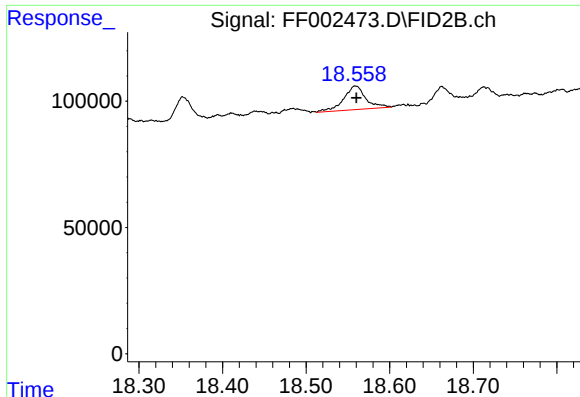


#14 N-DOTRIACONTANE

R.T.: 18.559 min
Delta R.T.: 0.000 min
Response: 171013
Conc: 1.10 ug/ml

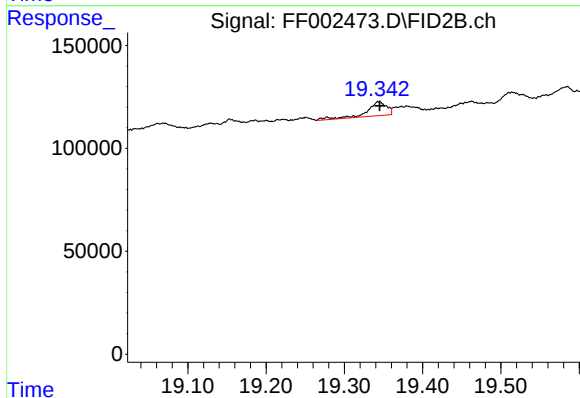

#15 N-TETRATRIACONTANE

R.T.: 19.343 min
Delta R.T.: -0.002 min
Response: 119515
Conc: 0.81 ug/ml

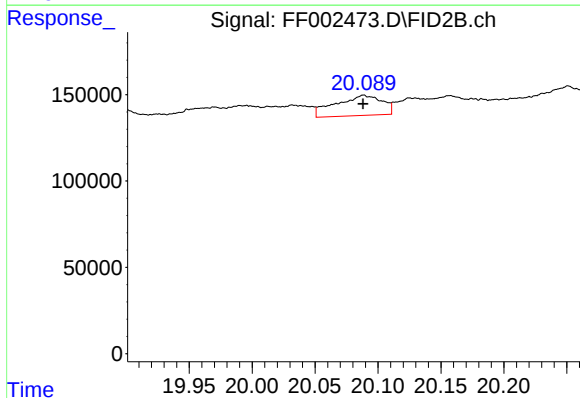

#16 N-HEXATRIACONTANE

R.T.: 20.089 min
Delta R.T.: 0.000 min
Response: 301211
Conc: 2.20 ug/ml