

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102418\
 Data File : FF002474.D
 Signal(s) : FID2B.ch
 Acq On : 24 Oct 2018 20:22
 Operator : AJ\SJ
 Sample : J5610-05 5X
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 25 03:43:55 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
 Quant Title :
 QLast Update : Fri Oct 12 13:21:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.655	320409	2.305 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.253f	161383	1.031 ug/ml
7)	N-EICOSANE	12.608f	354834	2.240 ug/ml
10)	N-TETRACOSANE	14.829	190092	1.215 ug/ml
12)	N-OCTACOSANE	16.833	213699	1.378 ug/ml
13)	N-TRIACONTANE	17.723	317154	2.044 ug/ml
14)	N-DOTRIACONTANE	18.556	206339	1.331 ug/ml
15)	N-TETRATRIACONTANE	19.347	163623	1.111 ug/ml
16)	N-HEXATRIACONTANE	20.093	104237	0.760 ug/ml
18)	N-TETRACONTANE	21.772	128116	1.075 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102418\
Data File : FF002474.D
Signal(s) : FID2B.ch
Acq On : 24 Oct 2018 20:22
Operator : AJ\SJ
Sample : J5610-05 5X
Misc :
ALS Vial : 67 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 25 03:43:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

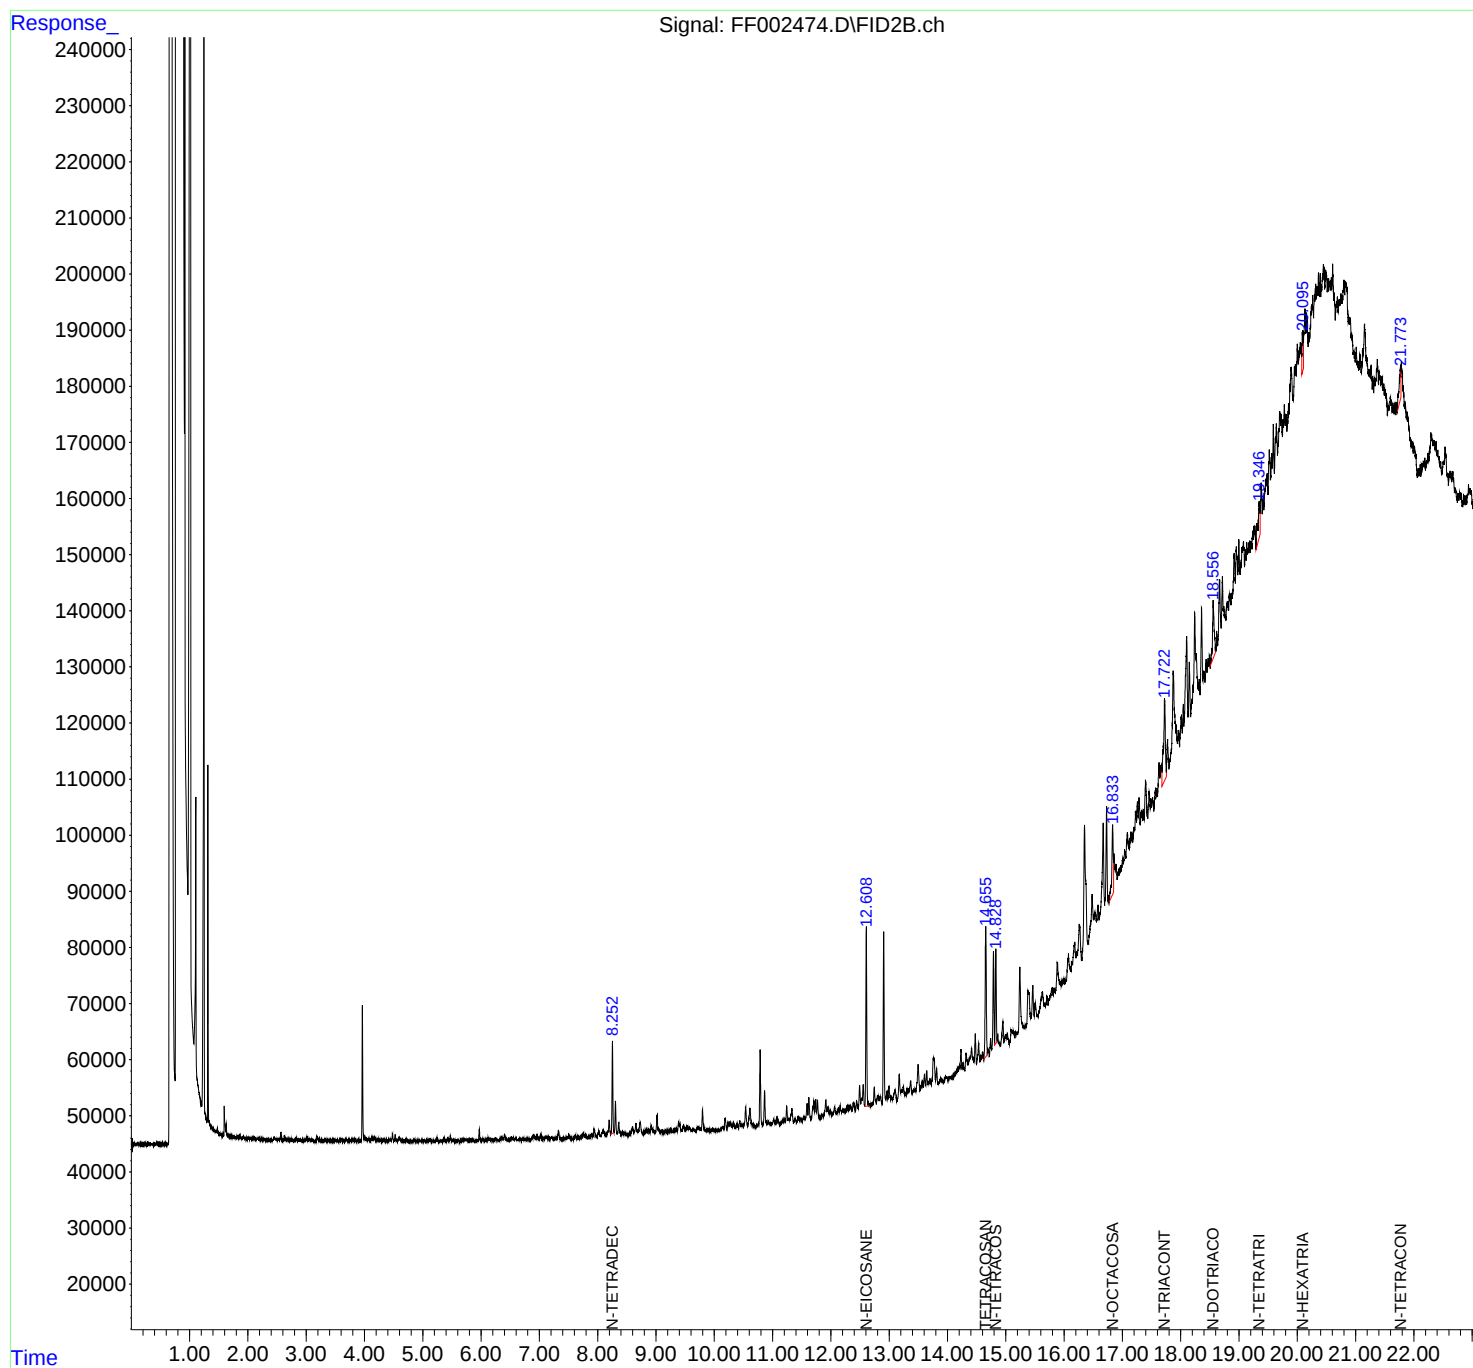

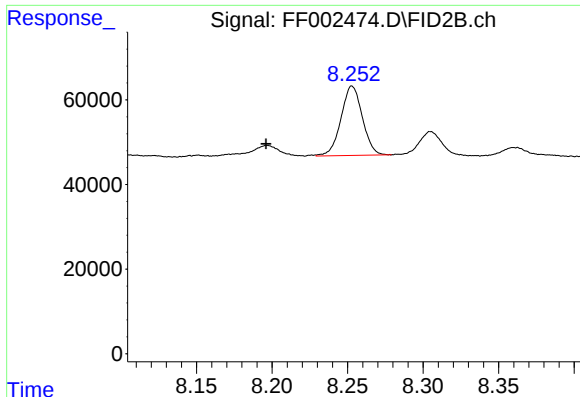


#4 N-TETRADECANE

R.T.: 8.253 min
Delta R.T.: 0.057 min
Response: 161383
Conc: 1.03 ug/ml

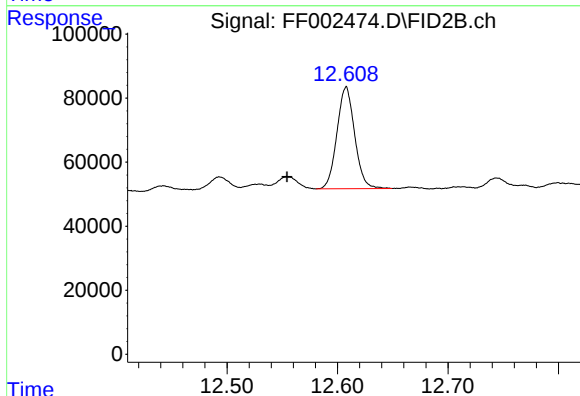


#7 N-EICOSANE

R.T.: 12.608 min
Delta R.T.: 0.053 min
Response: 354834
Conc: 2.24 ug/ml

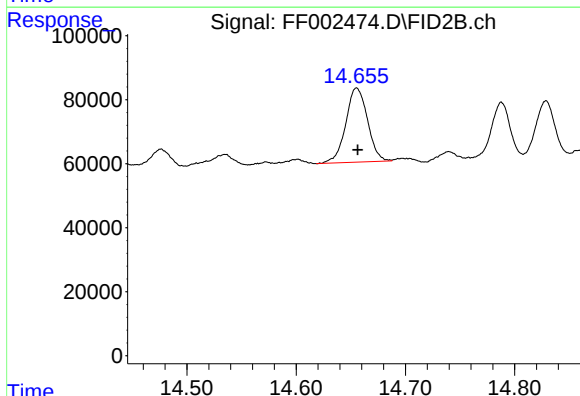


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.655 min
Delta R.T.: -0.001 min
Response: 320409
Conc: 2.31 ug/ml

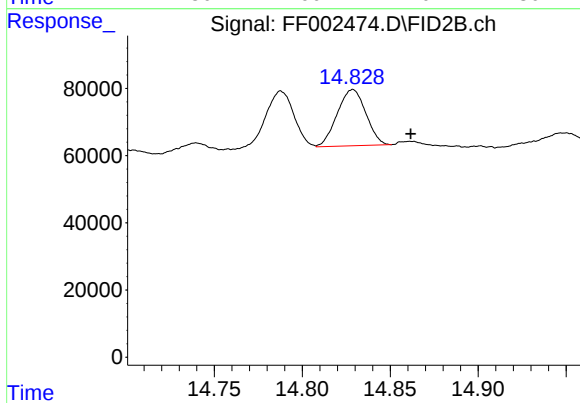


#10 N-TETRACOSANE

R.T.: 14.829 min
Delta R.T.: -0.033 min
Response: 190092
Conc: 1.22 ug/ml

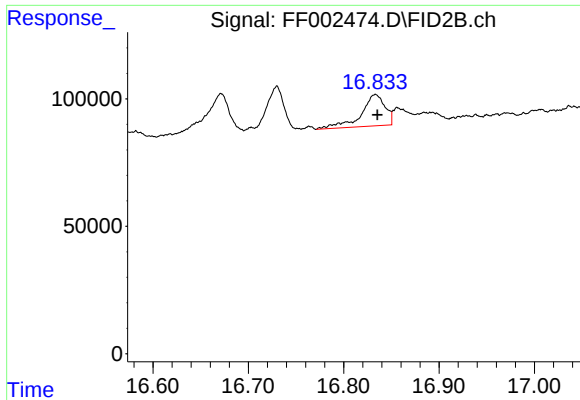


#12 N-OCTACOSANE

R.T.: 16.833 min
Delta R.T.: -0.002 min
Response: 213699
Conc: 1.38 ug/ml

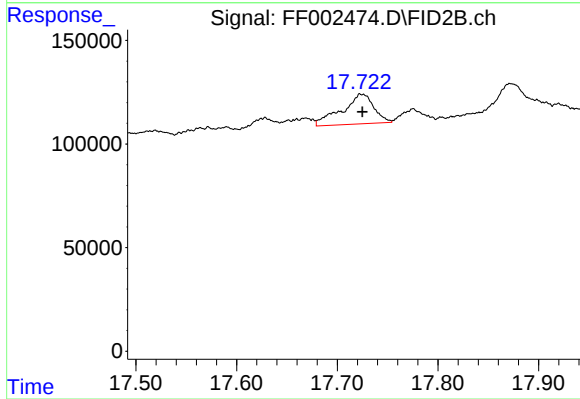


#13 N-TRIACONTANE

R.T.: 17.723 min
Delta R.T.: -0.002 min
Response: 317154
Conc: 2.04 ug/ml

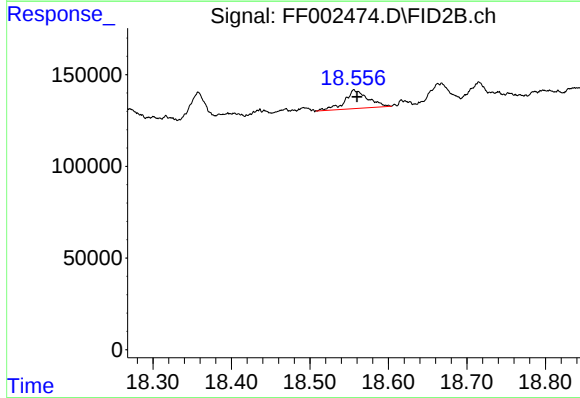


#14 N-DOTRIACONTANE

R.T.: 18.556 min
Delta R.T.: -0.004 min
Response: 206339
Conc: 1.33 ug/ml

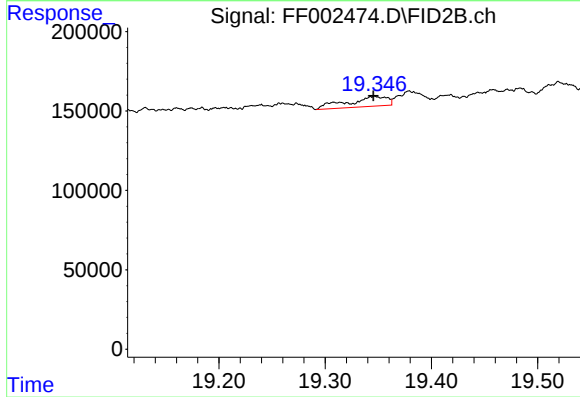


#15 N-TETRATRIACONTANE

R.T.: 19.347 min
Delta R.T.: 0.001 min
Response: 163623
Conc: 1.11 ug/ml

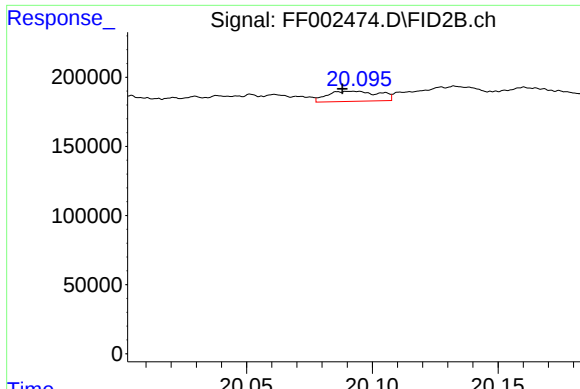

#16 N-HEXATRIACONTANE

R.T.: 20.093 min
Delta R.T.: 0.004 min
Response: 104237
Conc: 0.76 ug/ml

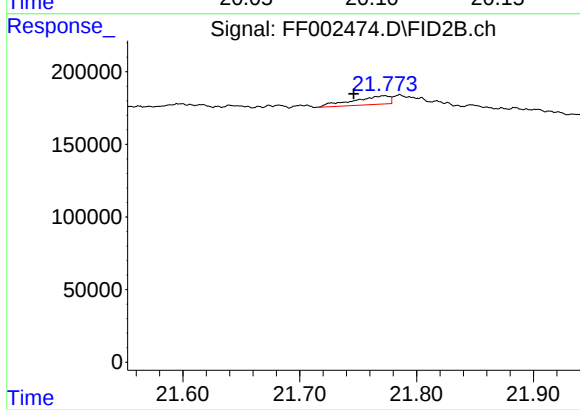

#18 N-TETRACONTANE

R.T.: 21.772 min
Delta R.T.: 0.026 min
Response: 128116
Conc: 1.08 ug/ml