

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102418\
Data File : FF002476.D
Signal(s) : FID2B.ch
Acq On : 24 Oct 2018 21:24
Operator : AJ\SJ
Sample : J5622-01 5X
Misc :
ALS Vial : 69 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 25 03:44:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.656	474204	3.412 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.254f	172054	1.100 ug/ml
14)	N-DOTRIACONTANE	18.559	133165	0.859 ug/ml
15)	N-TETRATRIACONTANE	19.343	64899	0.441 ug/ml
16)	N-HEXATRIACONTANE	20.088	35355	0.258 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102418\
Data File : FF002476.D
Signal(s) : FID2B.ch
Acq On : 24 Oct 2018 21:24
Operator : AJ\SJ
Sample : J5622-01 5X
Misc :
ALS Vial : 69 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 25 03:44:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

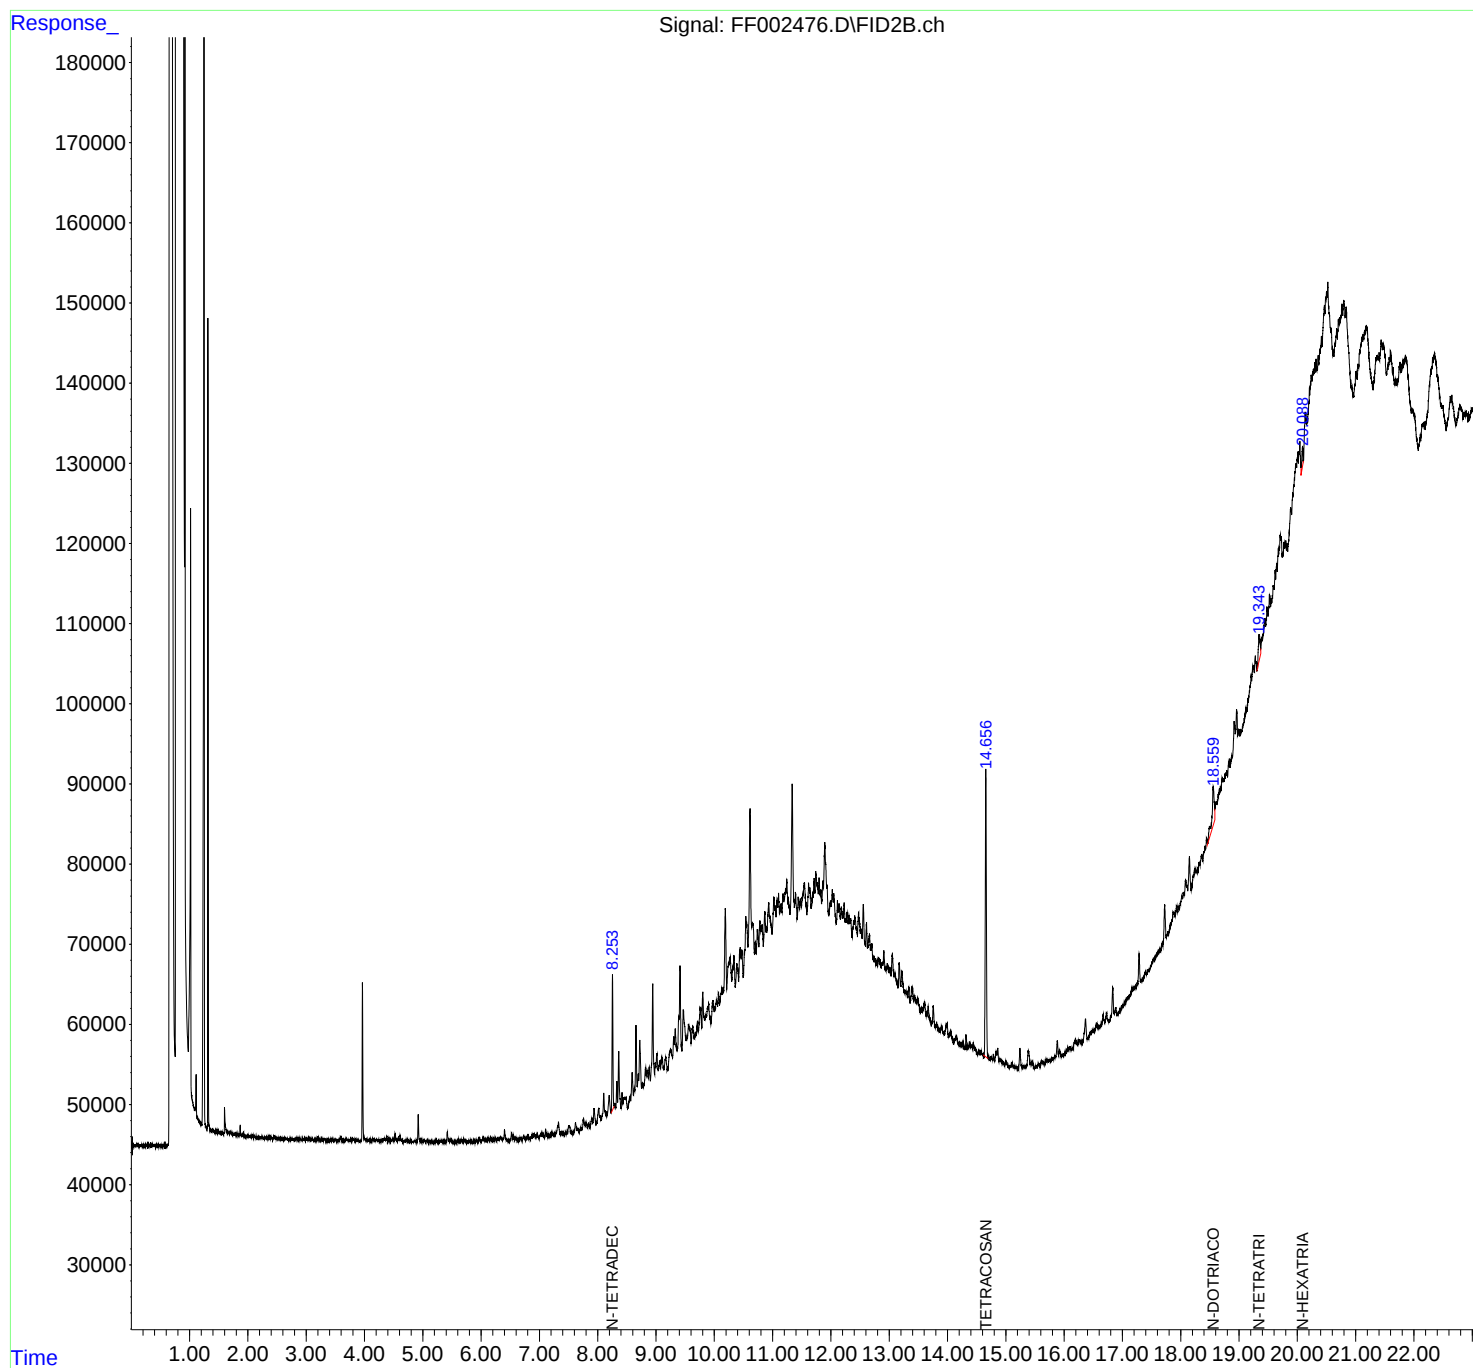

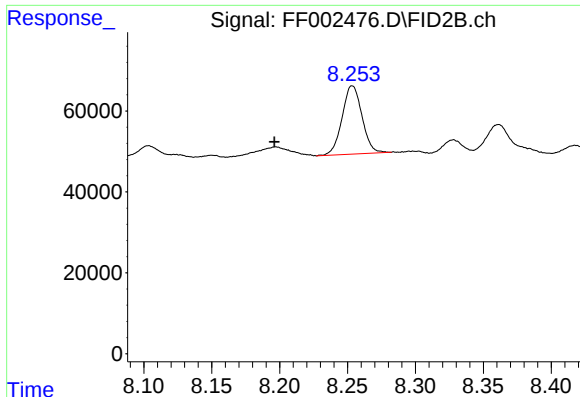


#4 N-TETRADECANE

R.T.: 8.254 min
Delta R.T.: 0.057 min
Response: 172054
Conc: 1.10 ug/ml

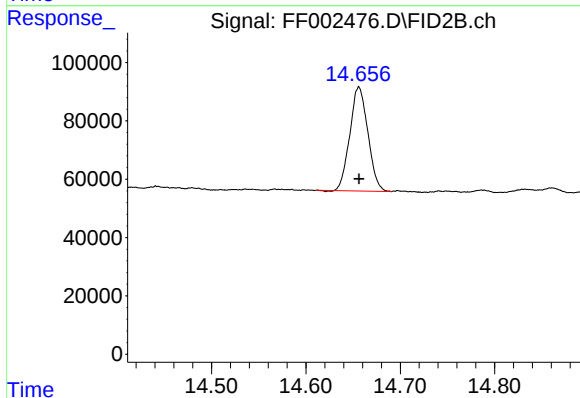


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.656 min
Delta R.T.: 0.000 min
Response: 474204
Conc: 3.41 ug/ml

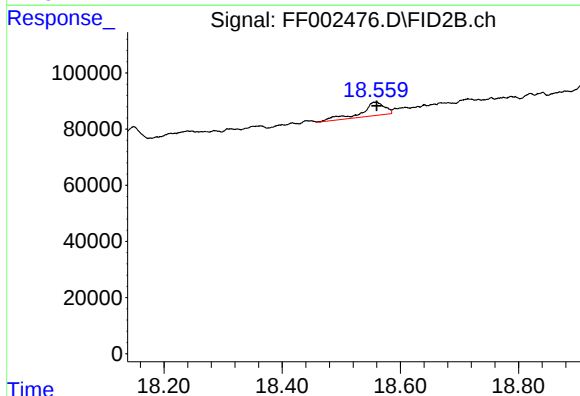


#14 N-DOTRIACONTANE

R.T.: 18.559 min
Delta R.T.: -0.001 min
Response: 133165
Conc: 0.86 ug/ml

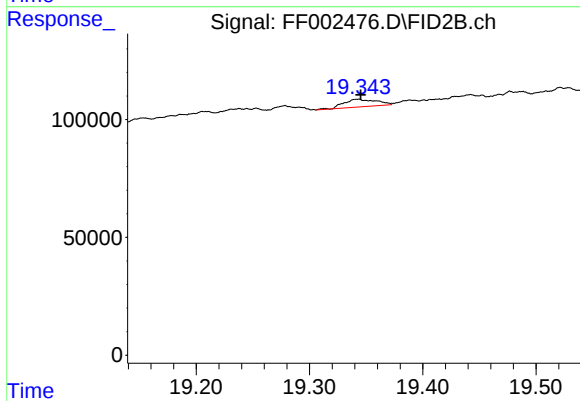

#15 N-TETRATRIACONTANE

R.T.: 19.343 min
Delta R.T.: -0.002 min
Response: 64899
Conc: 0.44 ug/ml

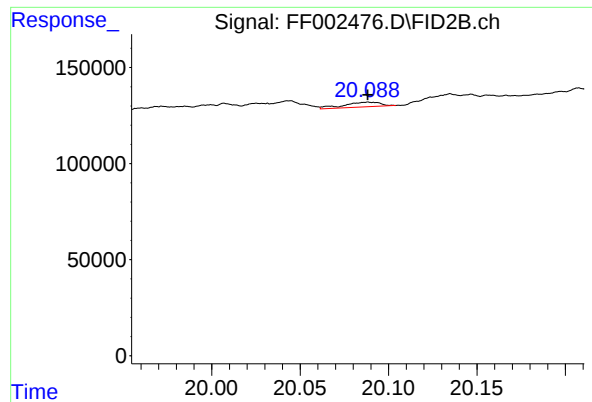

#16 N-HEXATRIACONTANE

R.T.: 20.088 min
Delta R.T.: 0.000 min
Response: 35355
Conc: 0.26 ug/ml