

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102419\
 Data File : FF005877.D
 Signal(s) : FID2B.ch
 Acq On : 24 Oct 2019 15:02
 Operator : DD\AJ
 Sample : PB124244BS
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 25 00:44:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100219.M
 Quant Title :
 QLast Update : Thu Oct 03 04:07:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.676	2969541	22.839 ug/ml
Target Compounds			
2) N-DECANE	4.421	3414857	21.992 ug/ml
3) N-DODECANE	6.441	3611452	22.932 ug/ml
4) N-TETRADECANE	8.235	3678022	23.403 ug/ml
5) N-HEXADECANE	9.832	3788449	24.033 ug/ml
6) N-OCTADECANE	11.273	3641438	23.470 ug/ml
7) N-EICOSANE	12.582	3548559	22.919 ug/ml
8) N-DOCOSANE	13.779	3492870	23.015 ug/ml
10) N-TETRACOSANE	14.881	3547682	23.842 ug/ml
11) N-HEXACOSANE	15.900	3448580	23.638 ug/ml
12) N-OCTACOSANE	16.849	3597862	25.263 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102419\
Data File : FF005877.D
Signal(s) : FID2B.ch
Acq On : 24 Oct 2019 15:02
Operator : DD\AJ
Sample : PB124244BS
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 25 00:44:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100219.M
Quant Title :
QLast Update : Thu Oct 03 04:07:51 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

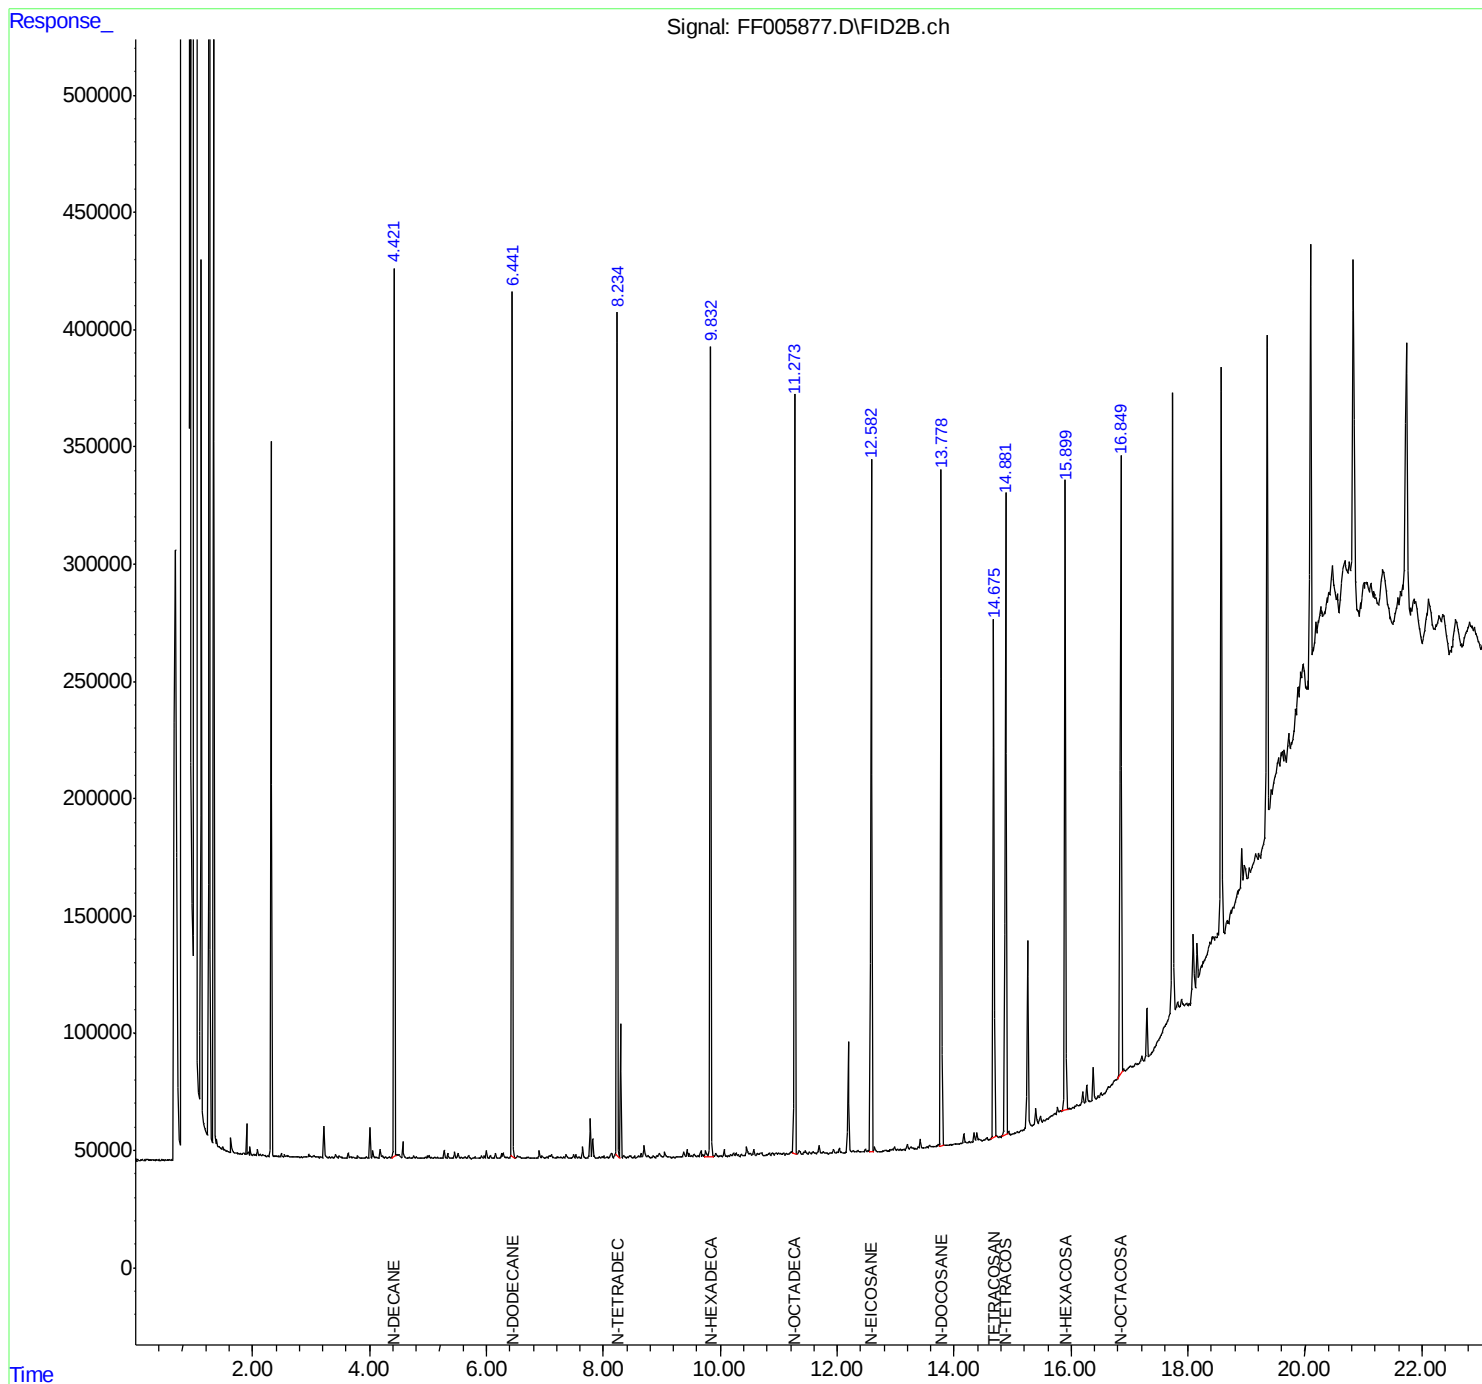

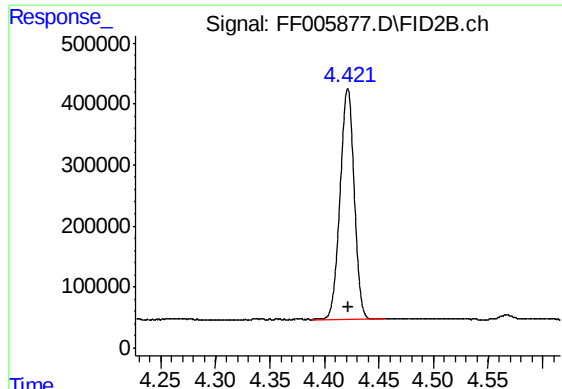


#2 N-DECANE

R.T.: 4.421 min
Delta R.T.: 0.000 min
Response: 3414857
Conc: 21.99 ug/ml

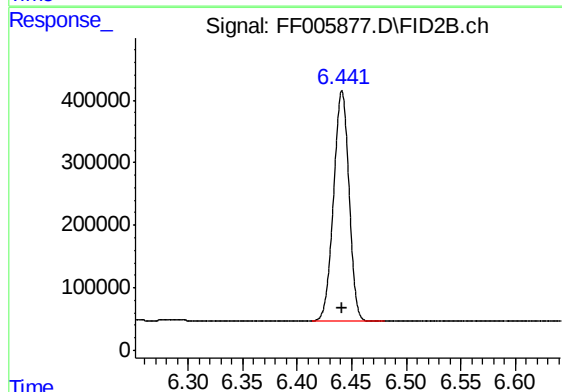


#3 N-DODECANE

R.T.: 6.441 min
Delta R.T.: 0.000 min
Response: 3611452
Conc: 22.93 ug/ml

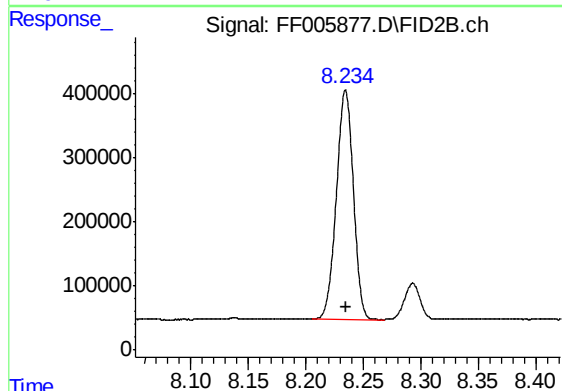


#4 N-TETRADECANE

R.T.: 8.235 min
Delta R.T.: 0.000 min
Response: 3678022
Conc: 23.40 ug/ml

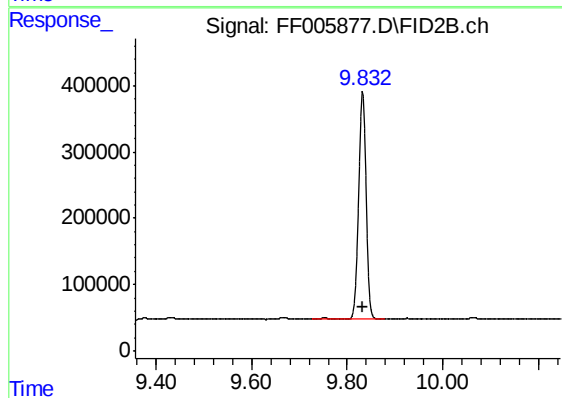


#5 N-HEXADECANE

R.T.: 9.832 min
Delta R.T.: -0.001 min
Response: 3788449
Conc: 24.03 ug/ml

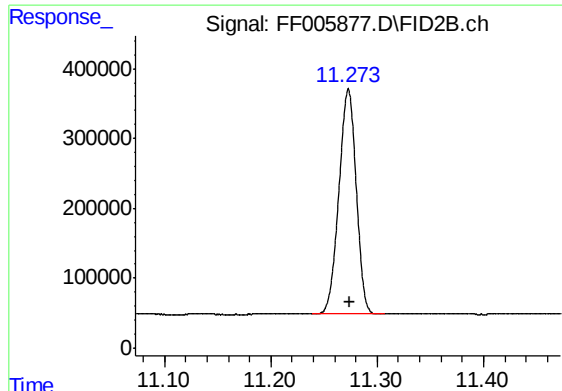


#6 N-OCTADECANE

R.T.: 11.273 min
Delta R.T.: -0.002 min
Response: 3641438
Conc: 23.47 ug/ml

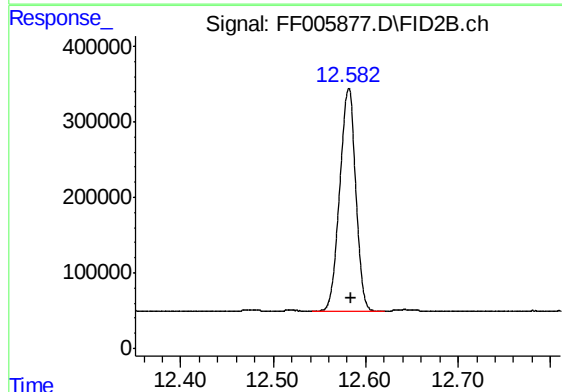


#7 N-EICOSANE

R.T.: 12.582 min
Delta R.T.: -0.002 min
Response: 3548559
Conc: 22.92 ug/ml

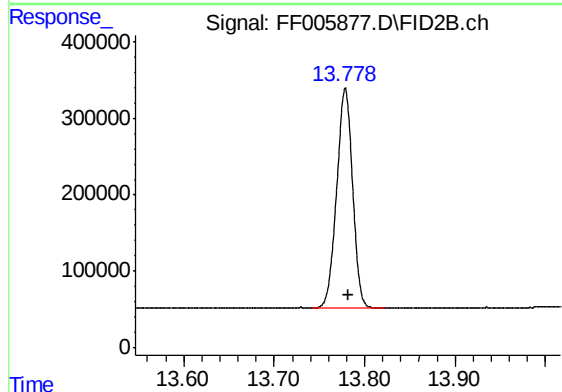


#8 N-DOCOSANE

R.T.: 13.779 min
Delta R.T.: -0.003 min
Response: 3492870
Conc: 23.02 ug/ml

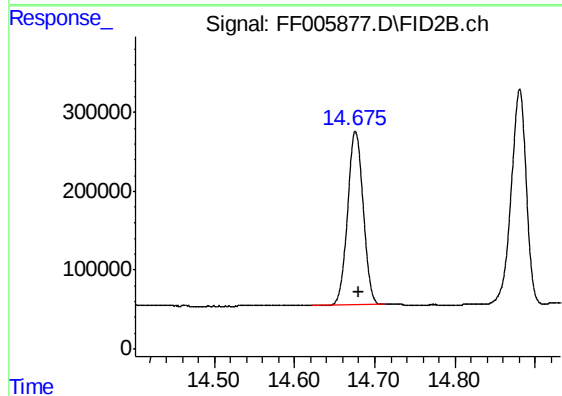


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.676 min
Delta R.T.: -0.004 min
Response: 2969541
Conc: 22.84 ug/ml

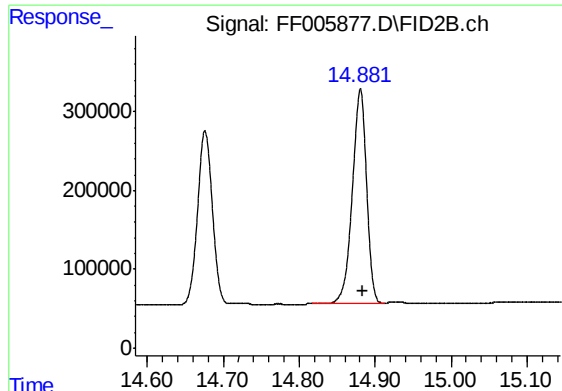


#10 N-TETRACOSANE

R.T.: 14.881 min
Delta R.T.: -0.004 min
Response: 3547682
Conc: 23.84 ug/ml

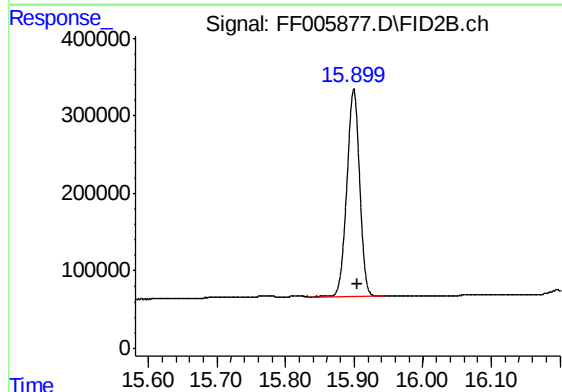

#11 N-HEXACOSANE

R.T.: 15.900 min
Delta R.T.: -0.006 min
Response: 3448580
Conc: 23.64 ug/ml

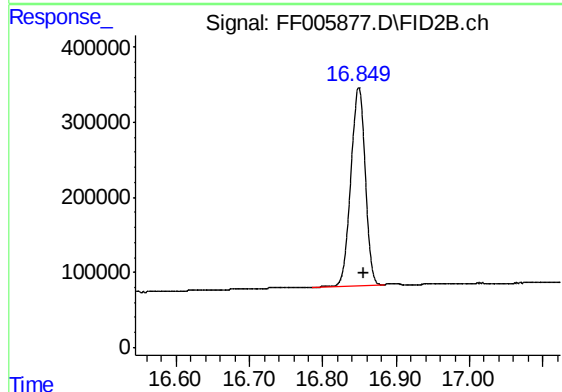

#12 N-OCTACOSANE

R.T.: 16.849 min
Delta R.T.: -0.006 min
Response: 3597862
Conc: 25.26 ug/ml