

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102424\
Data File : FF014763.D
Signal(s) : FID2B.ch
Acq On : 24 Oct 2024 16:35
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 25 04:37:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102124.M
Quant Title :
QLast Update : Tue Oct 22 08:35:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.010	2244176	17.053 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.069	56138	0.383 ug/ml
14) N-DOTRIACONTANE	18.901	83226	0.579 ug/ml
15) N-TETRATRIACONTANE	19.683	57775	0.421 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102424\
Data File : FF014763.D
Signal(s) : FID2B.ch
Acq On : 24 Oct 2024 16:35
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 25 04:37:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102124.M
Quant Title :
QLast Update : Tue Oct 22 08:35:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

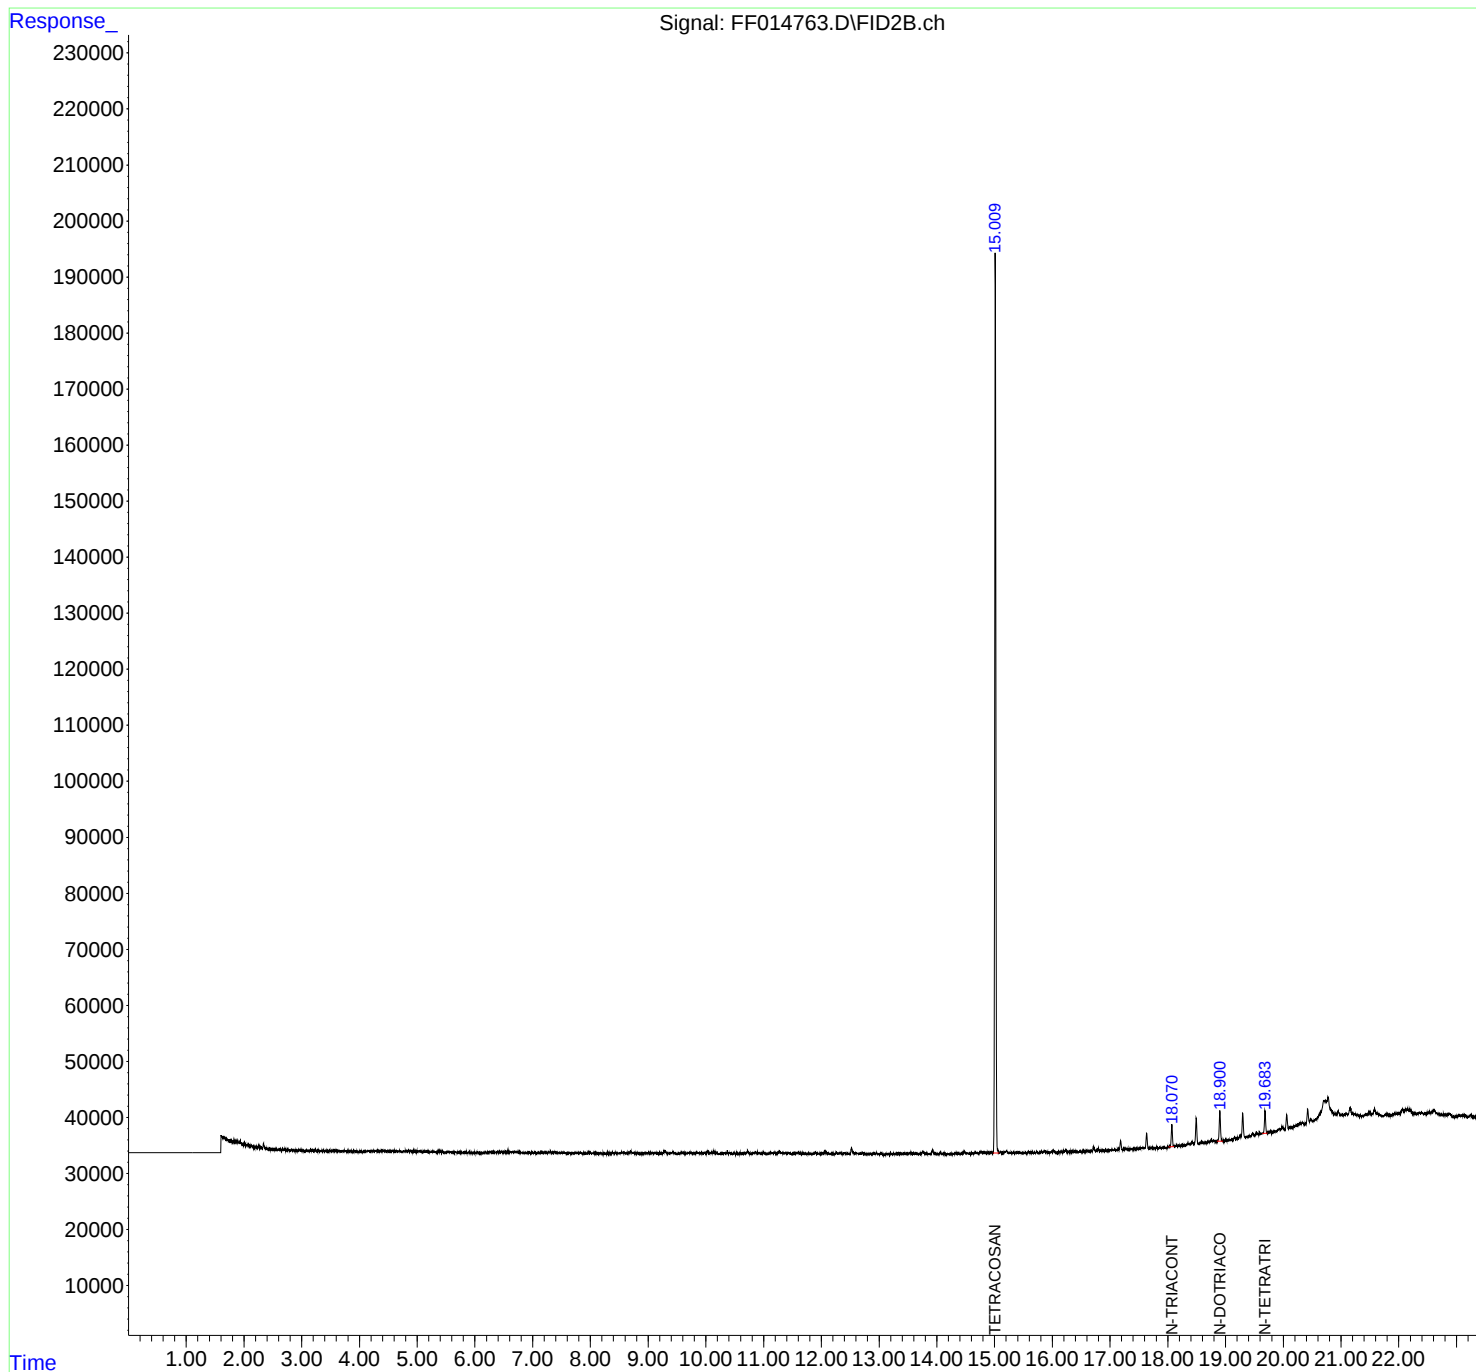


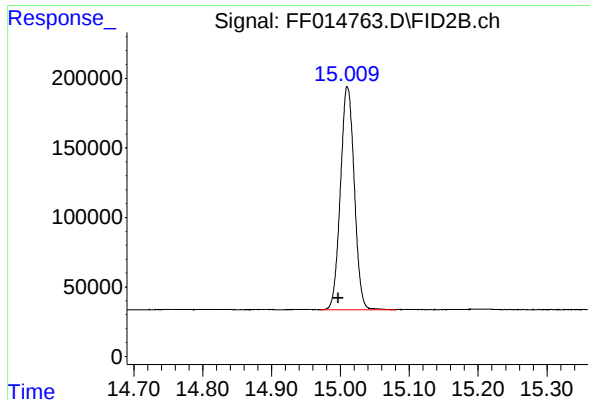

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.010 min
Delta R.T.: 0.013 min
Response: 2244176
Conc: 17.05 ug/ml

Instrument :
FID_F
ClientSampleId :

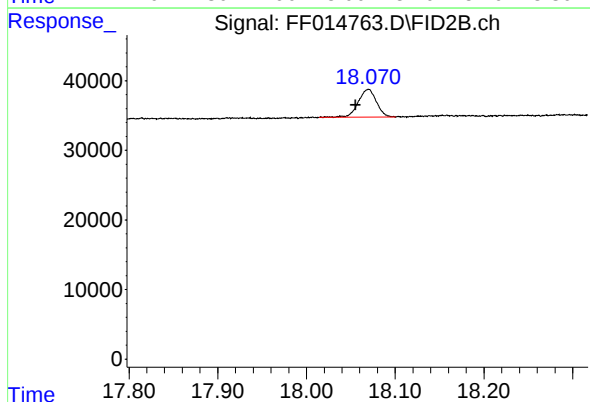


#13 N-TRIACONTANE

R.T.: 18.069 min
Delta R.T.: 0.014 min
Response: 56138
Conc: 0.38 ug/ml

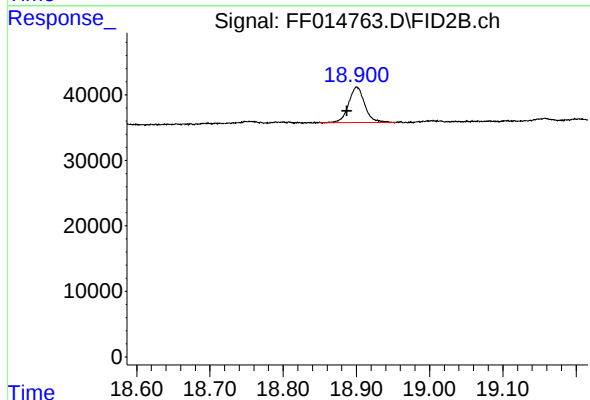

#14 N-DOTRIACONTANE

R.T.: 18.901 min
Delta R.T.: 0.014 min
Response: 83226
Conc: 0.58 ug/ml

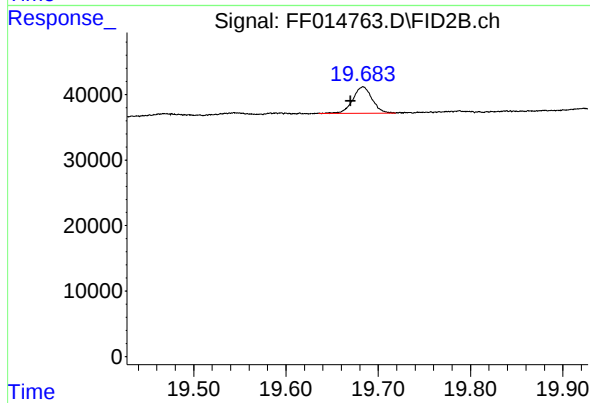

#15 N-TETRATRIACONTANE

R.T.: 19.683 min
Delta R.T.: 0.013 min
Response: 57775
Conc: 0.42 ug/ml