

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102424\
Data File : FF014758.D
Signal(s) : FID2B.ch
Acq On : 24 Oct 2024 13:32
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2024
Supervised By :Ankita Jodhani 10/25/2024

Integration File: autoint1.e
Quant Time: Oct 25 04:36:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102124.M
Quant Title :
QLast Update : Tue Oct 22 08:35:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.730	2999070	20.667 ug/ml
12) N-OCTACOSANE	17.182	2880294	19.934 ug/mlm

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102424\
Data File : FF014758.D
Signal(s) : FID2B.ch
Acq On : 24 Oct 2024 13:32
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2024
Supervised By :Ankita Jodhani 10/25/2024

Integration File: autoint1.e
Quant Time: Oct 25 04:36:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102124.M
Quant Title :
QLast Update : Tue Oct 22 08:35:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

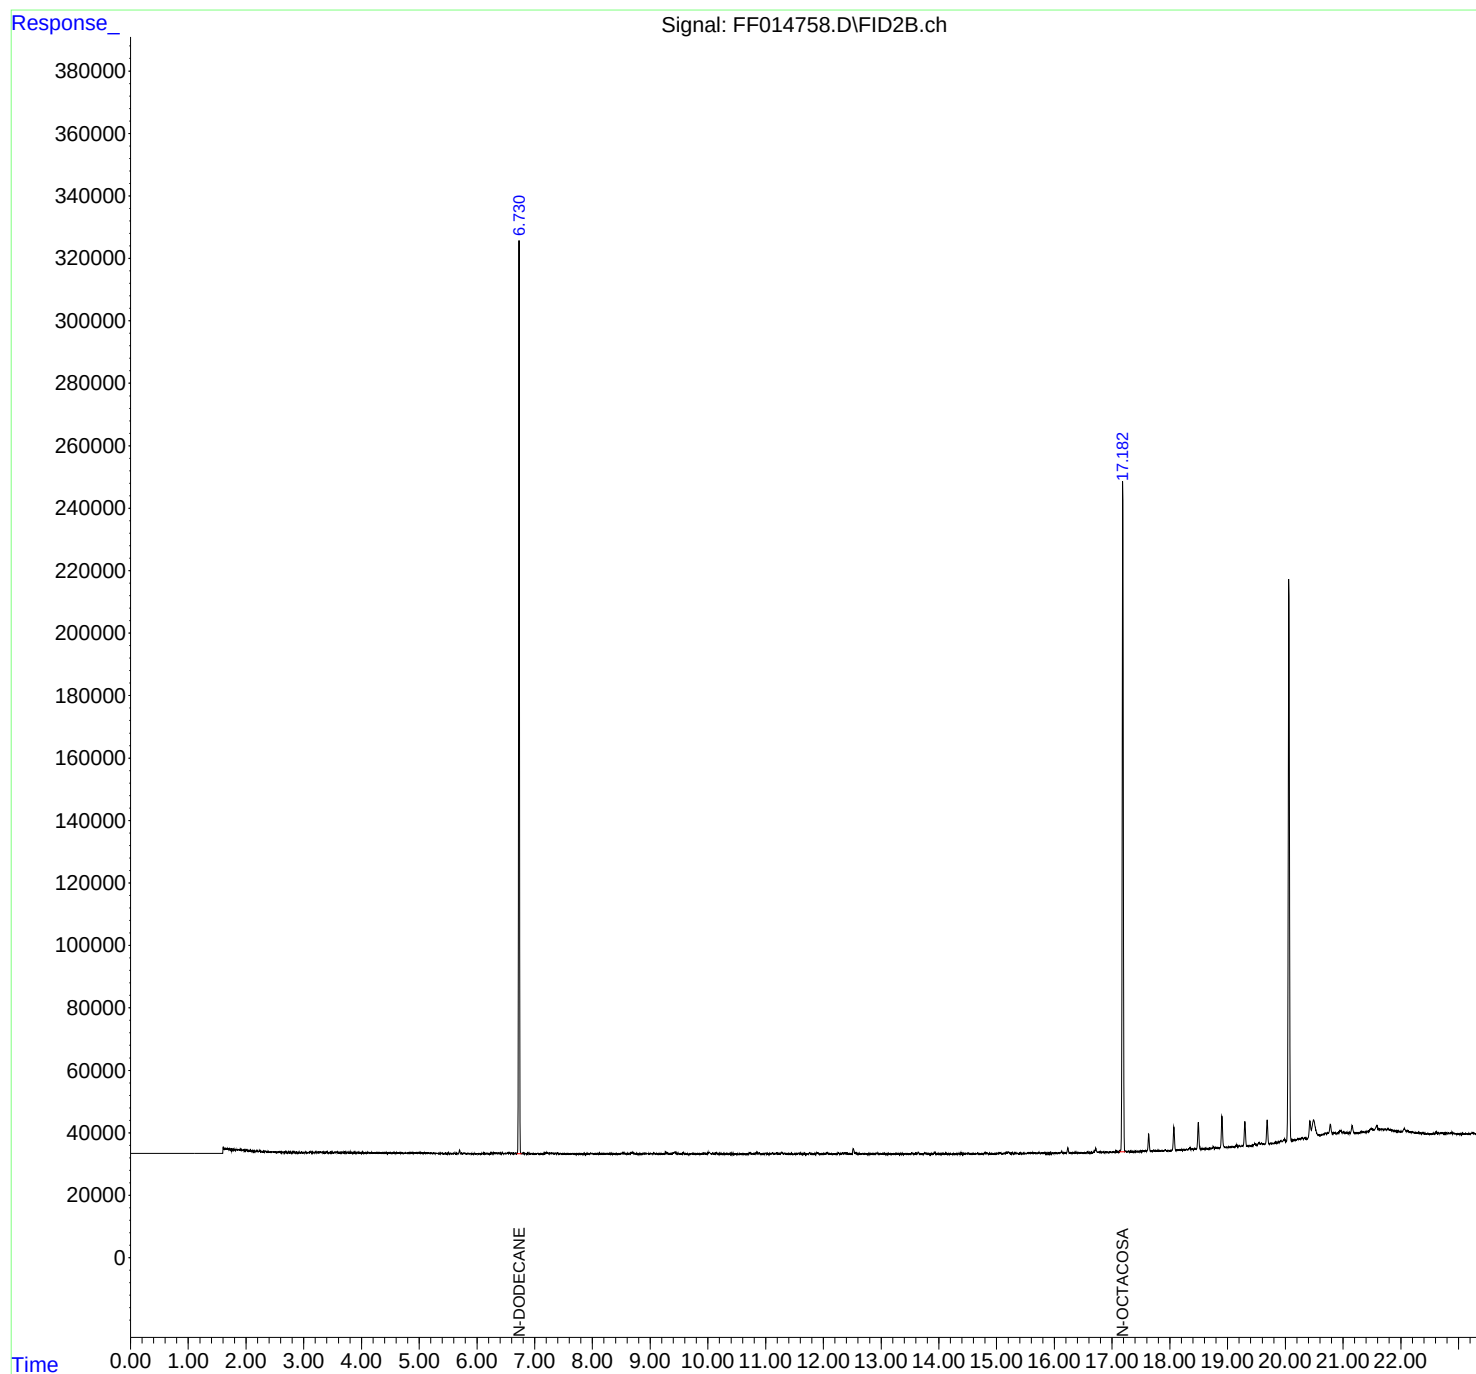

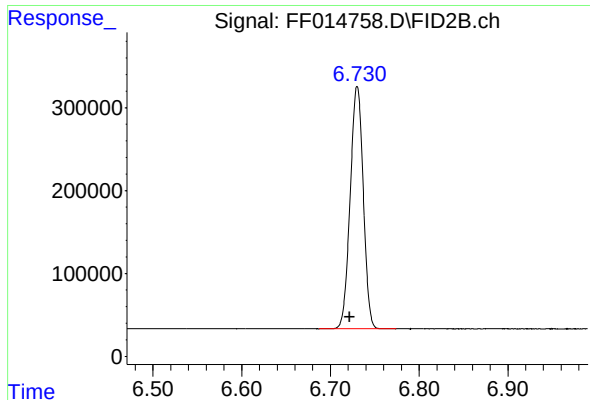

#3 N-DODECANE

R.T.: 6.730 min
Delta R.T.: 0.009 min
Response: 2999070
Conc: 20.67 ug/ml


Instrument :

FID_F

ClientSampleId :


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2024
Supervised By :Ankita Jodhani 10/25/2024

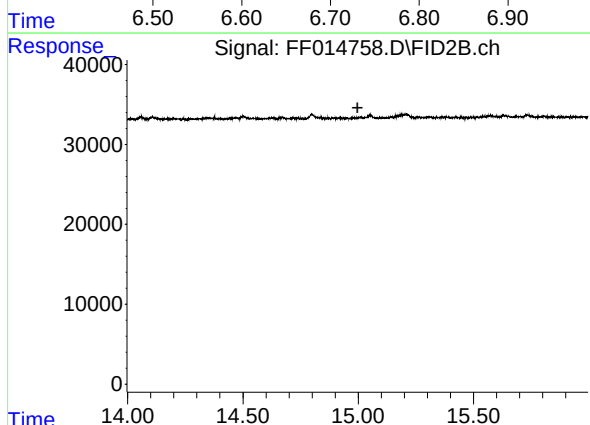

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.997 min
Response: 0
Conc: N.D.

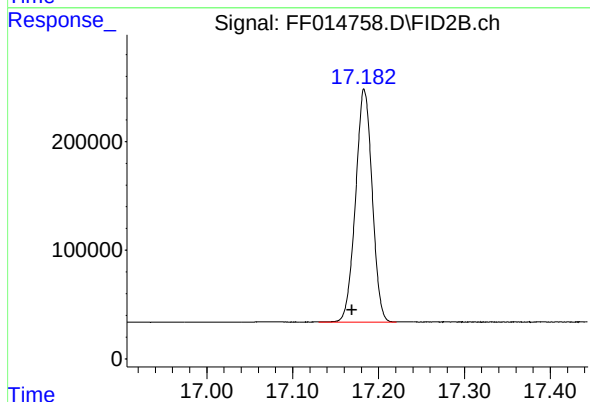

#12 N-OCTACOSANE

R.T.: 17.182 min
Delta R.T.: 0.013 min
Response: 2880294
Conc: 19.93 ug/ml m