

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102523\
Data File : FF013625.D
Signal(s) : FID2B.ch
Acq On : 25 Oct 2023 22:23
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 26 00:43:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101623.M
Quant Title :
QLast Update : Mon Oct 16 12:53:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.970	1940505	15.519 ug/ml
Target Compounds				
15)	N-TETRATRIACONTANE	19.646	92222	0.883 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102523\
Data File : FF013625.D
Signal(s) : FID2B.ch
Acq On : 25 Oct 2023 22:23
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 26 00:43:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101623.M
Quant Title :
QLast Update : Mon Oct 16 12:53:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

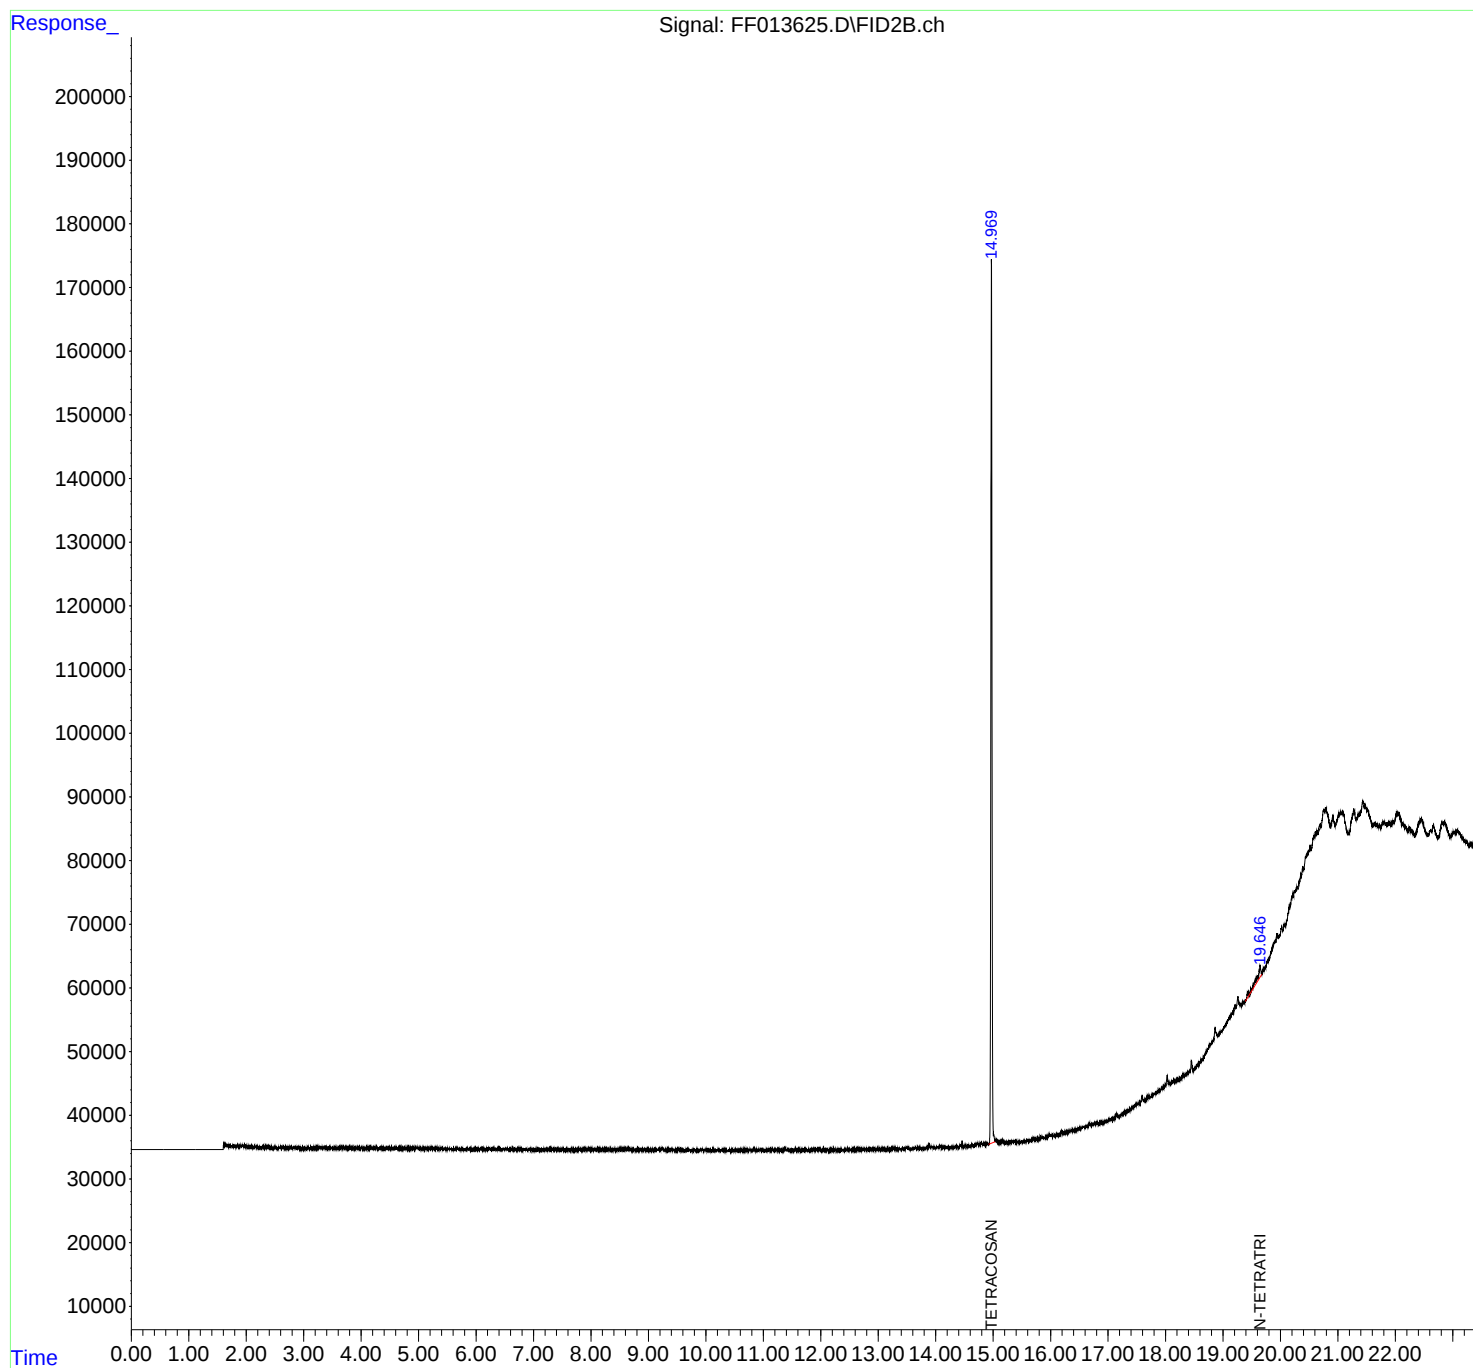


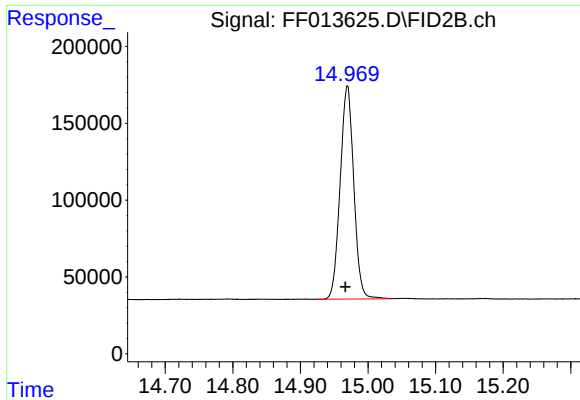

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.970 min
Delta R.T.: 0.003 min
Response: 1940505
Conc: 15.52 ug/ml

Instrument :
FID_F
ClientSampleId :

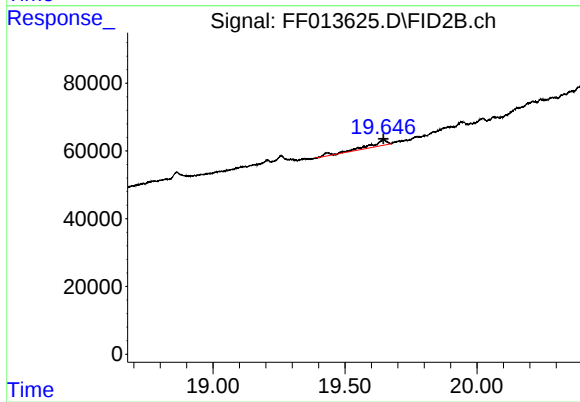

#15 N-TETRATRIACONTANE

R.T.: 19.646 min
Delta R.T.: 0.000 min
Response: 92222
Conc: 0.88 ug/ml