

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102524\
 Data File : FF014786.D
 Signal(s) : FID2B.ch
 Acq On : 25 Oct 2024 12:17
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 26 04:03:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102124.M
 Quant Title :
 QLast Update : Tue Oct 22 08:35:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.011	2232188	16.962 ug/ml
Target Compounds			
12) N-OCTACOSANE	17.182	59356	0.411 ug/ml
13) N-TRIACONTANE	18.070	140895	0.962 ug/ml
14) N-DOTRIACONTANE	18.902	199493	1.387 ug/ml
15) N-TETRATRIACONTANE	19.685	144044	1.050 ug/ml
16) N-HEXATRIACONTANE	20.424	75712	0.584 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102524\
Data File : FF014786.D
Signal(s) : FID2B.ch
Acq On : 25 Oct 2024 12:17
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 26 04:03:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102124.M
Quant Title :
QLast Update : Tue Oct 22 08:35:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

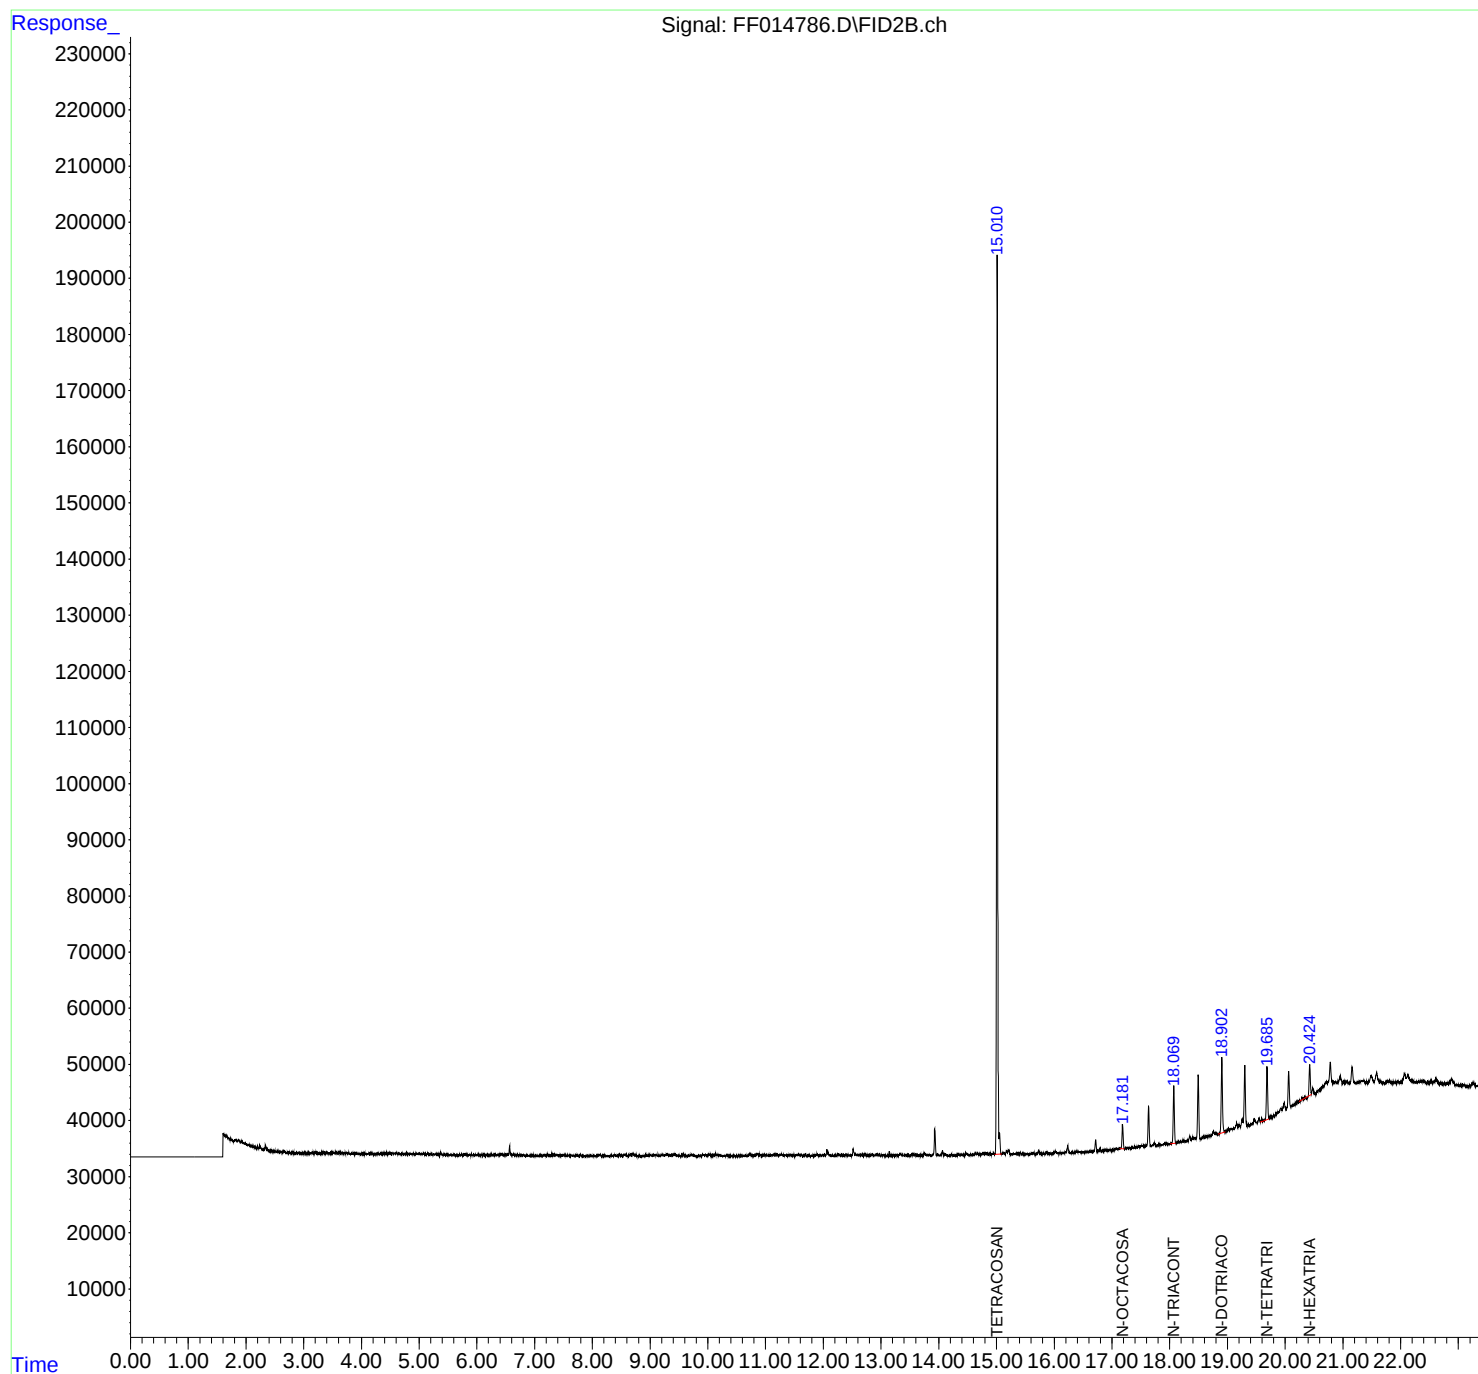


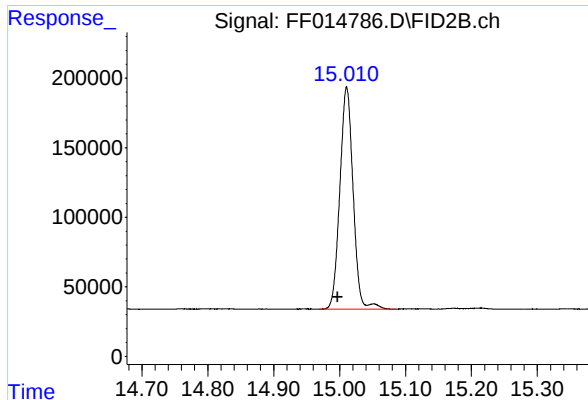

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.011 min
Delta R.T.: 0.014 min
Response: 2232188
Conc: 16.96 ug/ml

Instrument :
FID_F
ClientSampleId :

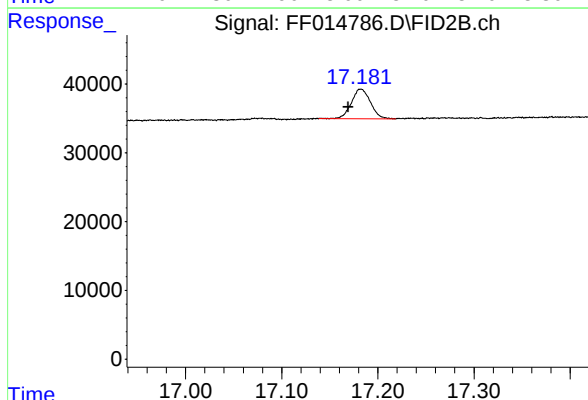


#12 N-OCTACOSANE

R.T.: 17.182 min
Delta R.T.: 0.013 min
Response: 59356
Conc: 0.41 ug/ml

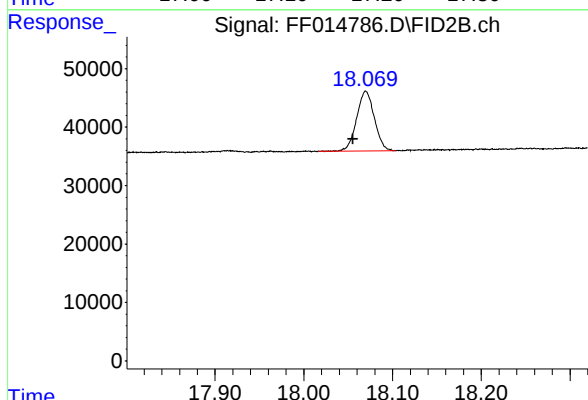


#13 N-TRIACONTANE

R.T.: 18.070 min
Delta R.T.: 0.015 min
Response: 140895
Conc: 0.96 ug/ml

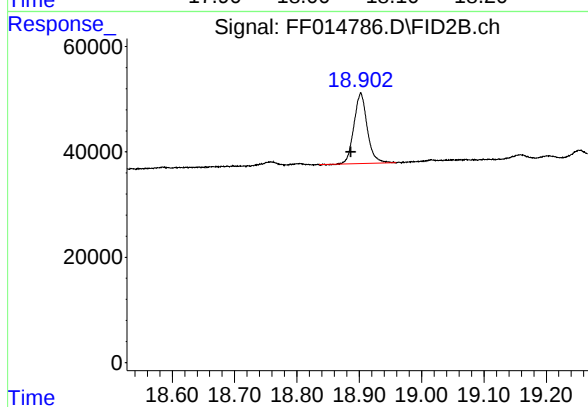

#14 N-DOTRIACONTANE


R.T.: 18.902 min
Delta R.T.: 0.015 min
Response: 199493
Conc: 1.39 ug/ml

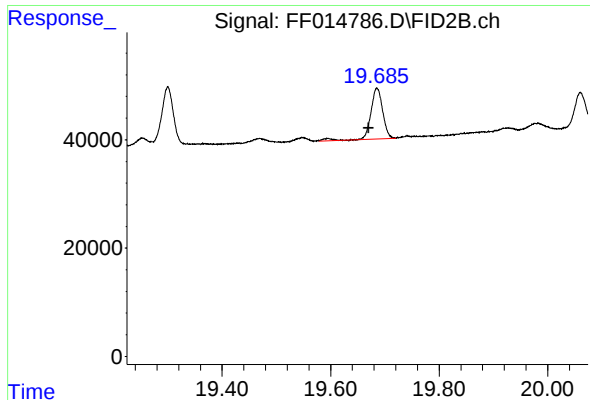

#15 N-TETRATRIACONTANE

R.T.: 19.685 min
Delta R.T.: 0.015 min
Response: 144044
Conc: 1.05 ug/ml

Instrument :
FID_F
ClientSampleId :

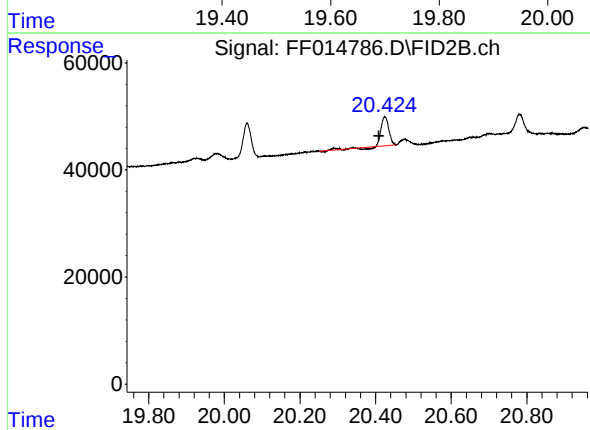

#16 N-HEXATRIACONTANE

R.T.: 20.424 min
Delta R.T.: 0.016 min
Response: 75712
Conc: 0.58 ug/ml