

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102621\
Data File : FF009185.D
Signal(s) : FID2B.ch
Acq On : 26 Oct 2021 10:31
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 27 01:26:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
16)	N-HEXATRIACONTANE	20.139	137643	1.548 ug/ml
18)	N-TETRACONTANE	21.776	708134	8.716 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102621\
Data File : FF009185.D
Signal(s) : FID2B.ch
Acq On : 26 Oct 2021 10:31
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 27 01:26:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

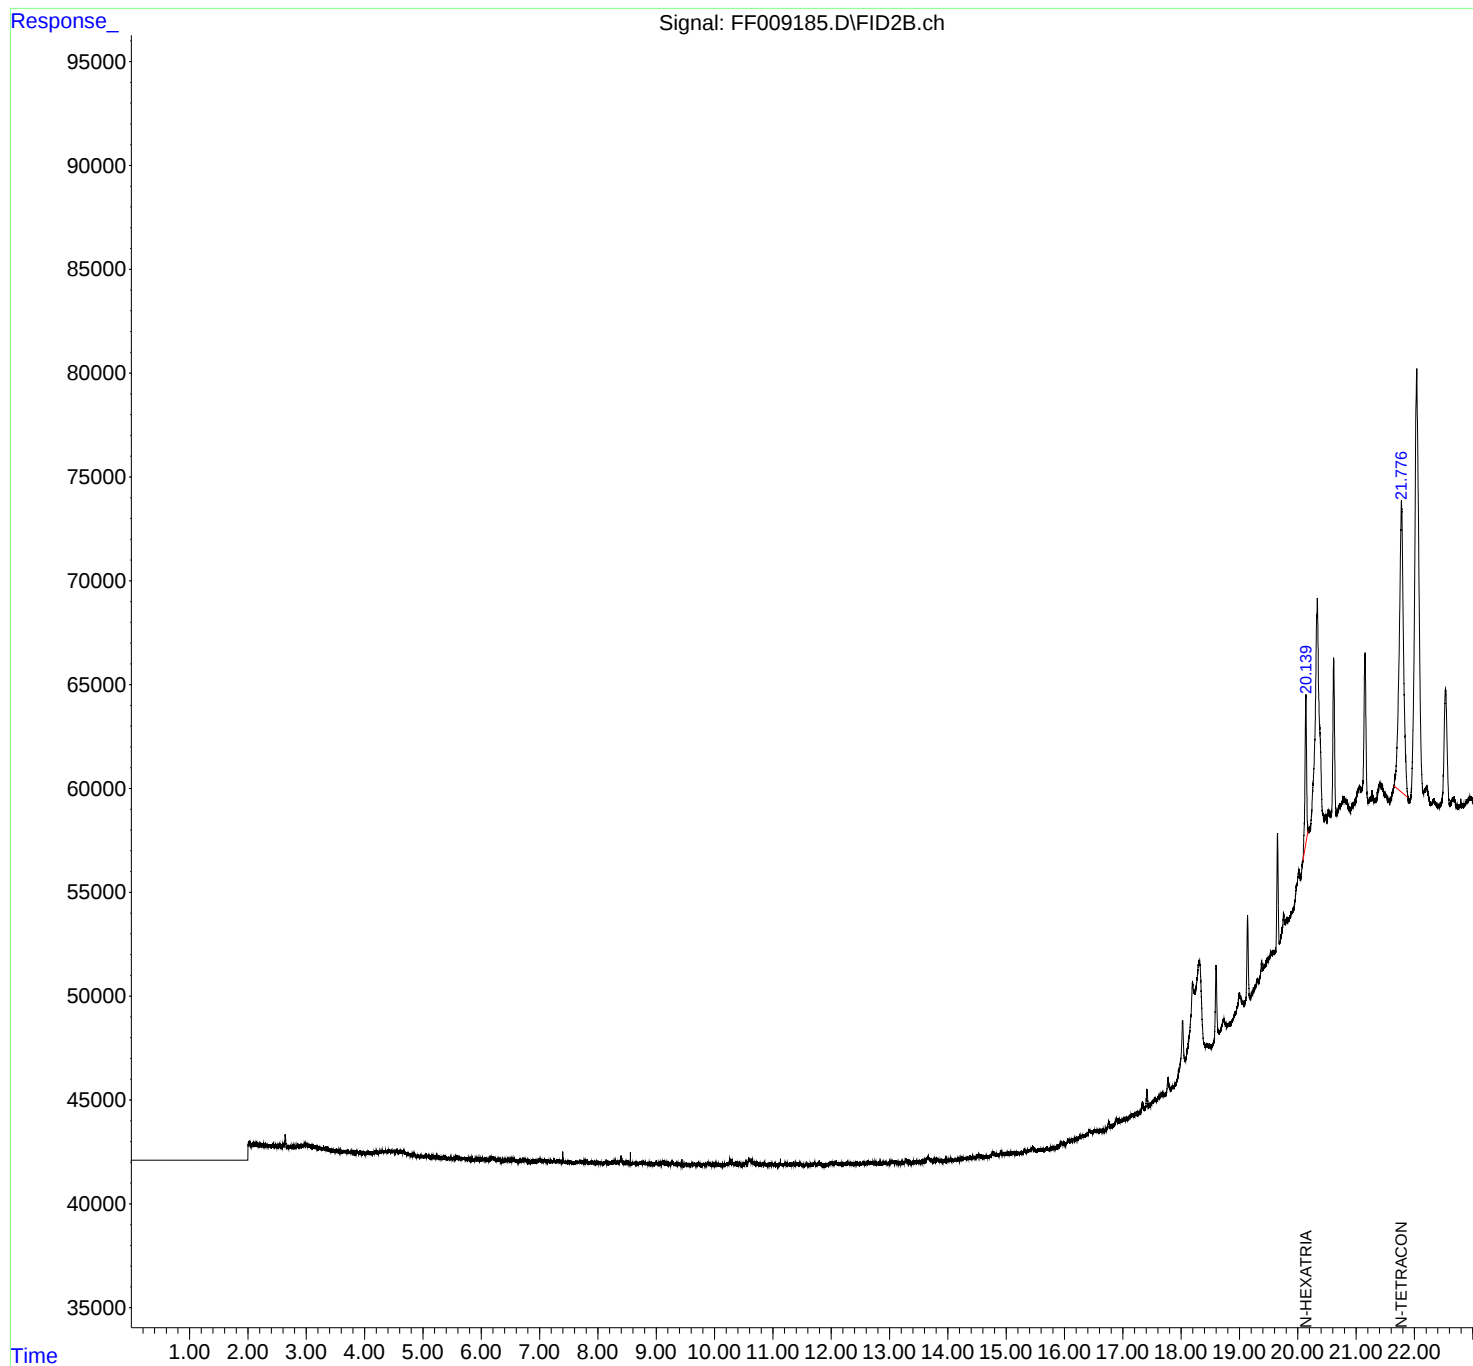


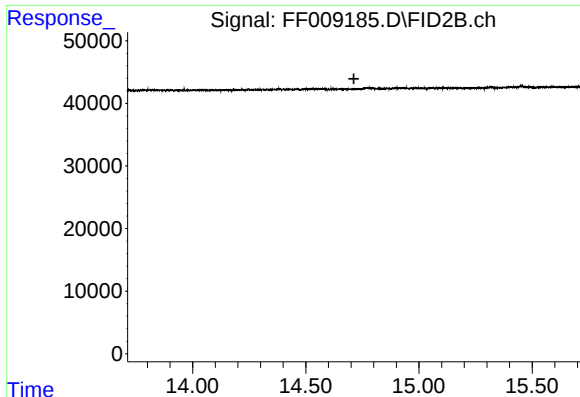

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.712 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

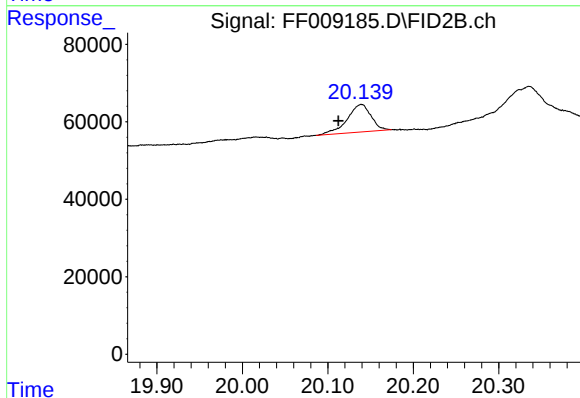

#16 N-HEXATRIACONTANE

R.T.: 20.139 min
Delta R.T.: 0.027 min
Response: 137643
Conc: 1.55 ug/ml

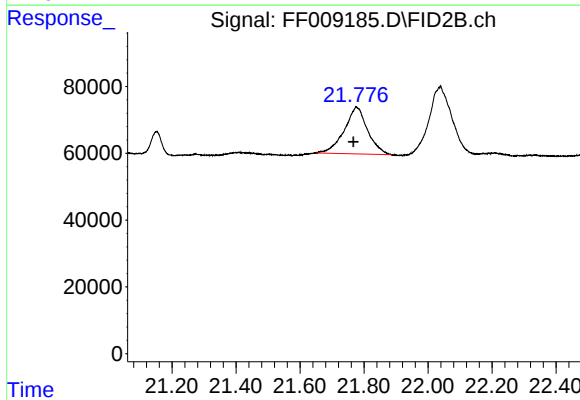

#18 N-TETRACONTANE

R.T.: 21.776 min
Delta R.T.: 0.009 min
Response: 708134
Conc: 8.72 ug/ml