

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102621\
Data File : FF009191.D
Signal(s) : FID2B.ch
Acq On : 26 Oct 2021 14:50
Operator : AJ\MA
Sample : M4325-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 27 01:27:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.707	2338113	21.322 ug/ml
Target Compounds			
11) N-HEXACOSANE	15.929	102383	0.846 ug/ml
12) N-OCTACOSANE	16.877	94556	0.808 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102621\
Data File : FF009191.D
Signal(s) : FID2B.ch
Acq On : 26 Oct 2021 14:50
Operator : AJ\MA
Sample : M4325-01
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 27 01:27:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

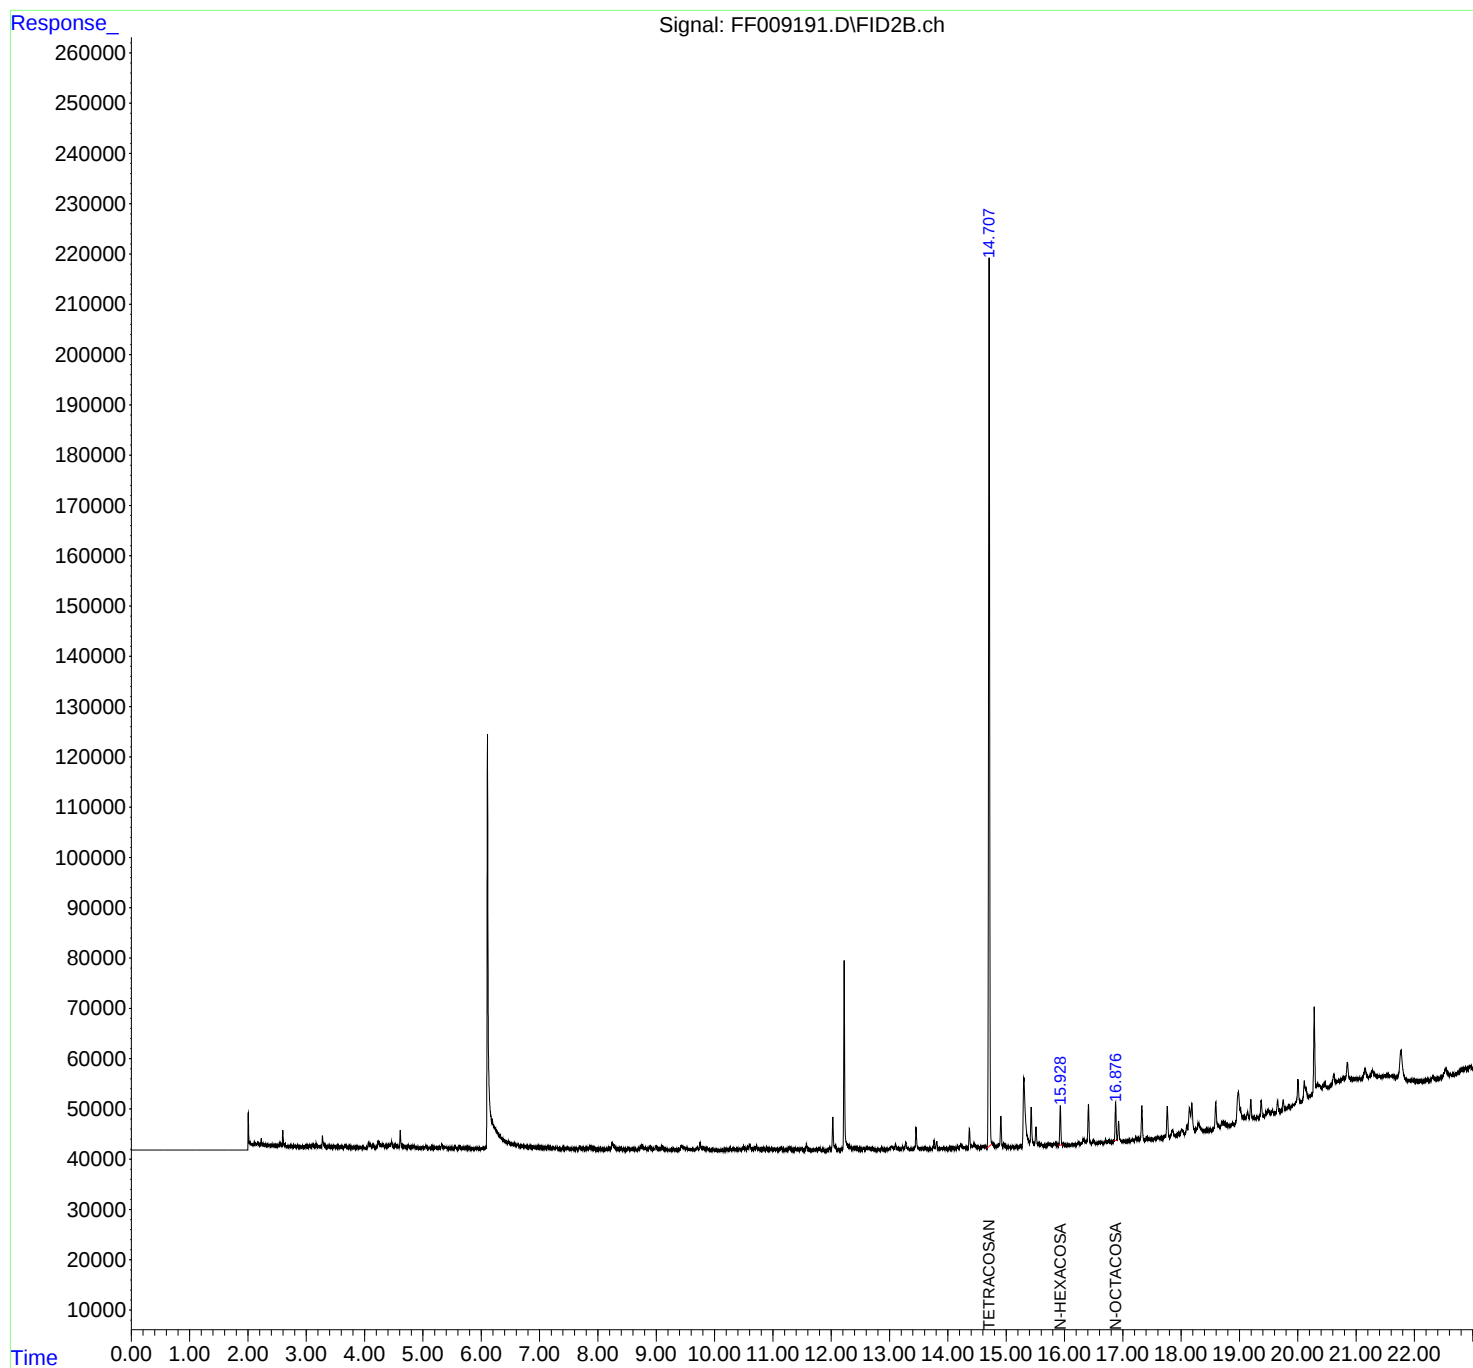


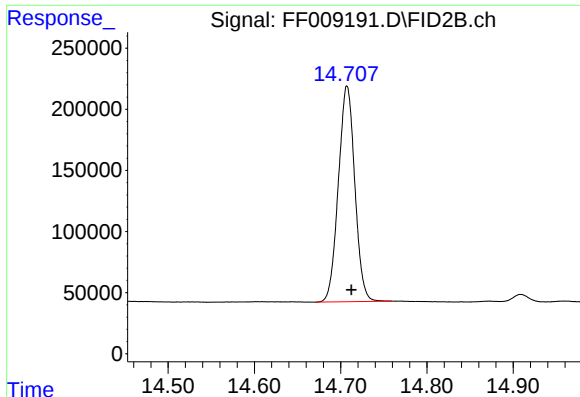

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.707 min
Delta R.T.: -0.005 min
Response: 2338113
Conc: 21.32 ug/ml

Instrument :
FID_F
ClientSampleId :

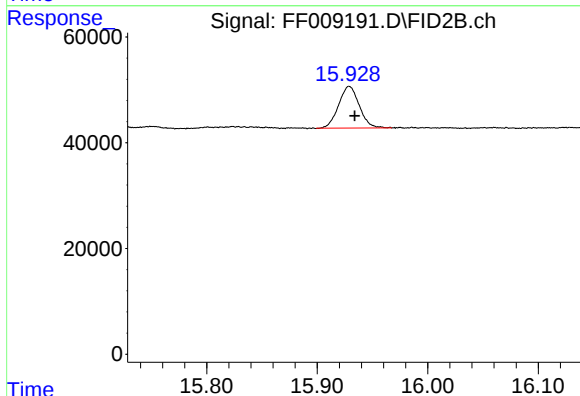

#11 N-HEXACOSANE

R.T.: 15.929 min
Delta R.T.: -0.005 min
Response: 102383
Conc: 0.85 ug/ml

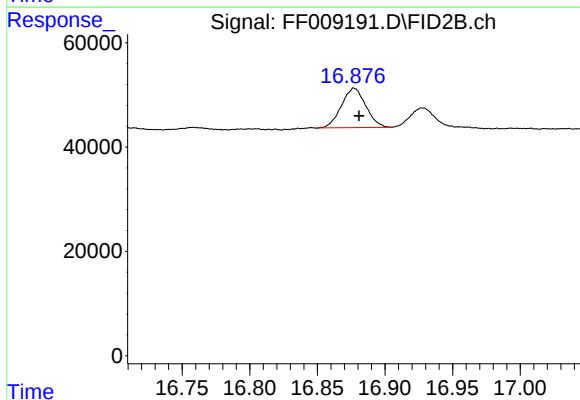

#12 N-OCTACOSANE

R.T.: 16.877 min
Delta R.T.: -0.004 min
Response: 94556
Conc: 0.81 ug/ml