

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102621\
Data File : FF009195.D
Signal(s) : FID2B.ch
Acq On : 26 Oct 2021 17:14
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 27 01:28:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.706	1808966	16.497 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.139	149331	1.680 ug/ml
18) N-TETRACONTANE	21.777	249254	3.068 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102621\
Data File : FF009195.D
Signal(s) : FID2B.ch
Acq On : 26 Oct 2021 17:14
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 27 01:28:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

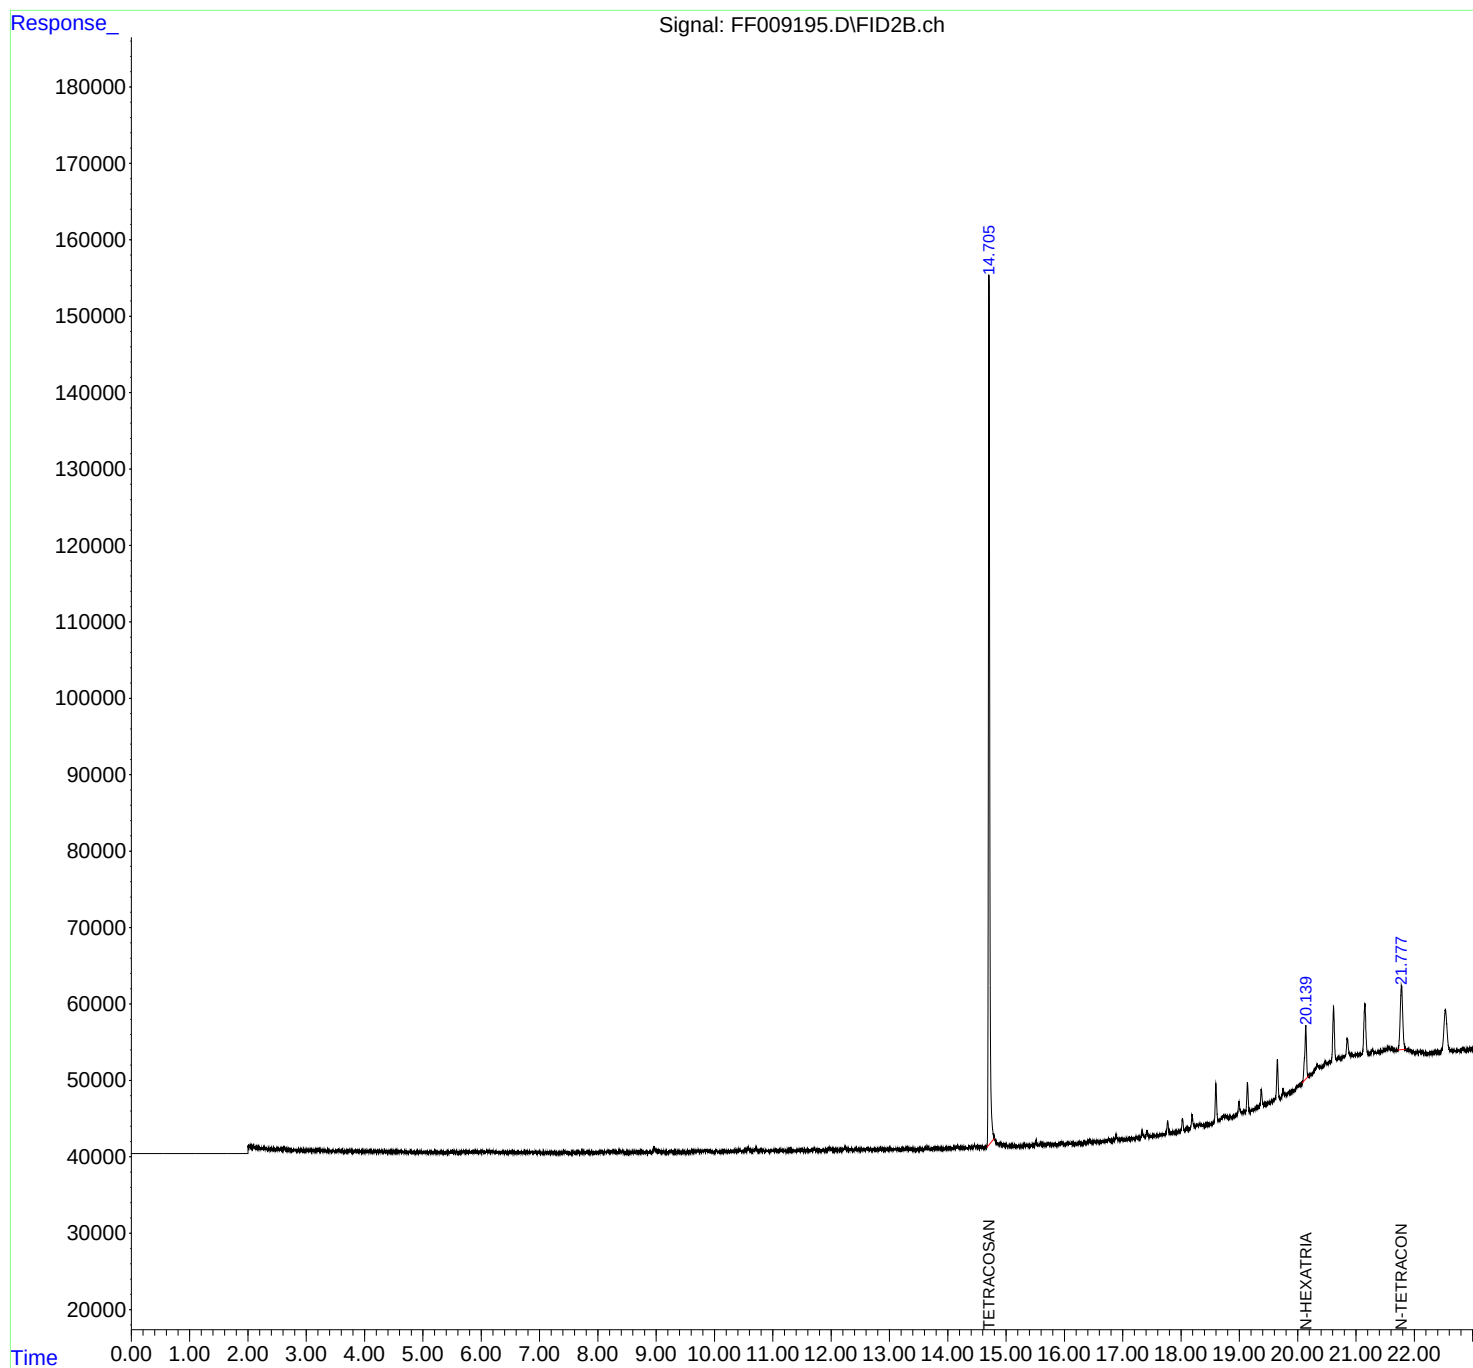


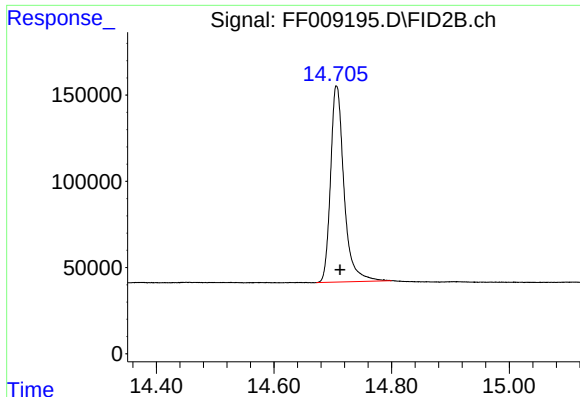

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.706 min
Delta R.T.: -0.006 min
Response: 1808966
Conc: 16.50 ug/ml

Instrument :
FID_F
ClientSampleId :

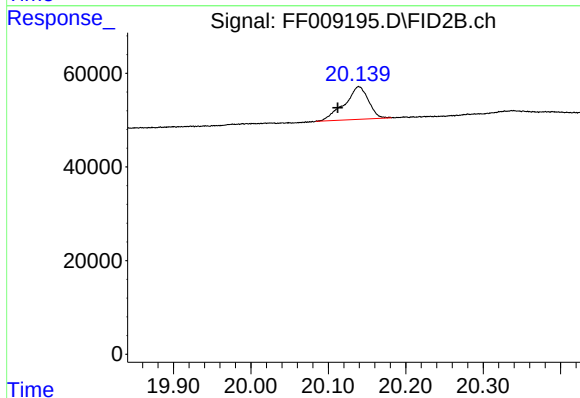

#16 N-HEXATRIACONTANE

R.T.: 20.139 min
Delta R.T.: 0.027 min
Response: 149331
Conc: 1.68 ug/ml

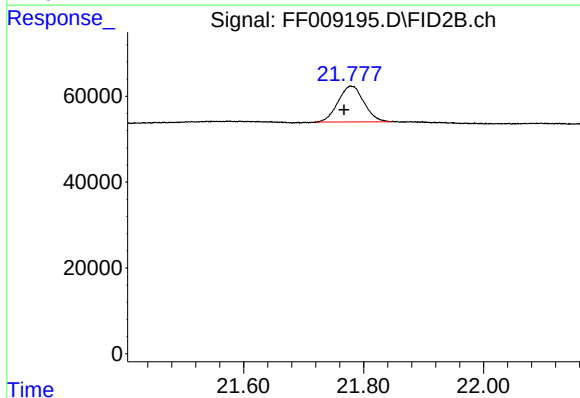

#18 N-TETRACONTANE

R.T.: 21.777 min
Delta R.T.: 0.010 min
Response: 249254
Conc: 3.07 ug/ml