

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102621\
Data File : FF009188.D
Signal(s) : FID2B.ch
Acq On : 26 Oct 2021 12:28
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 27 01:27:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.479	2110507	16.613 ug/ml
12) N-OCTACOSANE	16.878	2110505	18.029 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102621\
Data File : FF009188.D
Signal(s) : FID2B.ch
Acq On : 26 Oct 2021 12:28
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 27 01:27:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

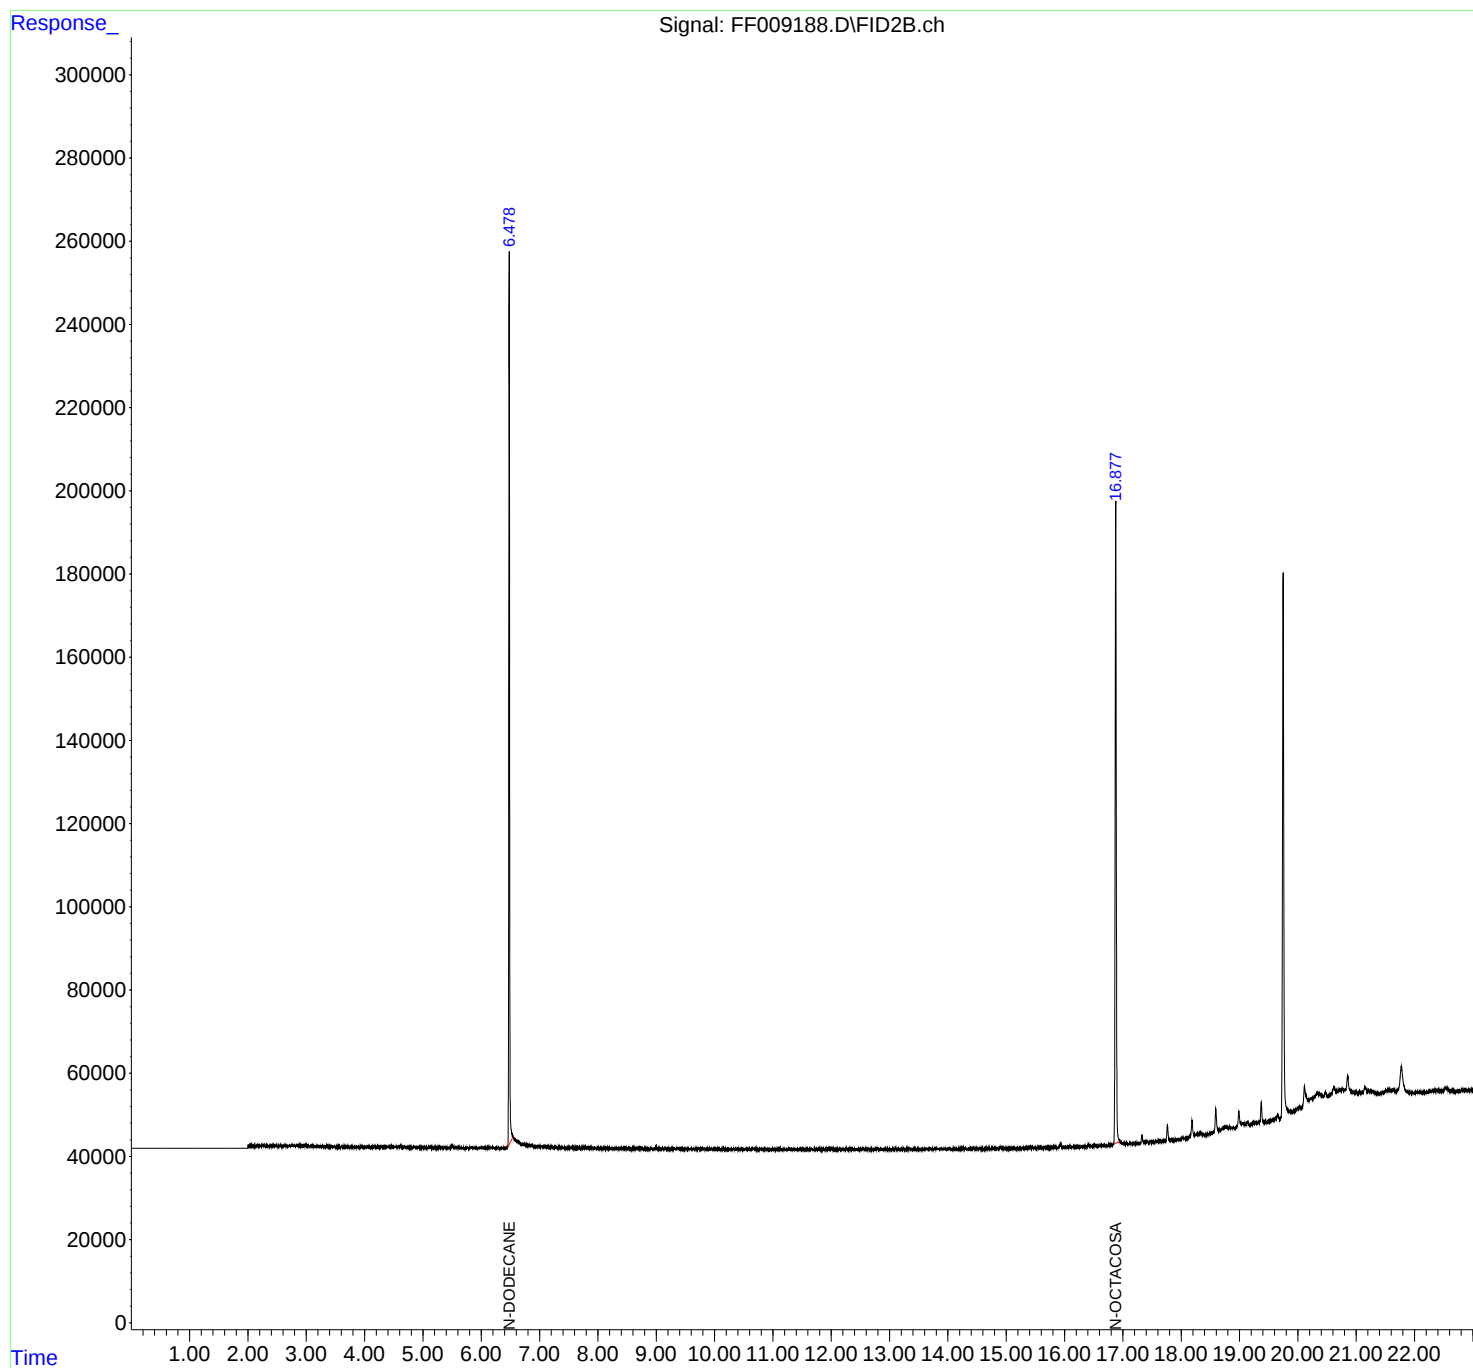


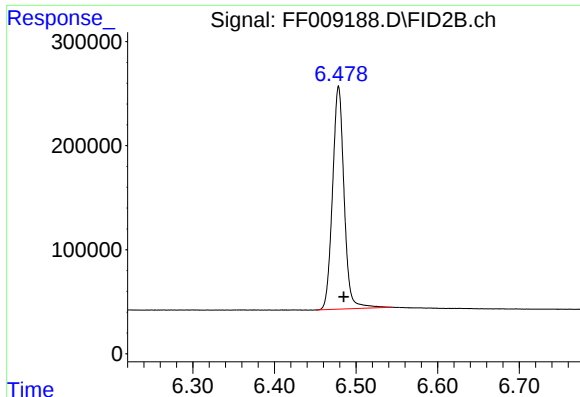

#3 N-DODECANE


R.T.: 6.479 min
Delta R.T.: -0.006 min
Response: 2110507
Conc: 16.61 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

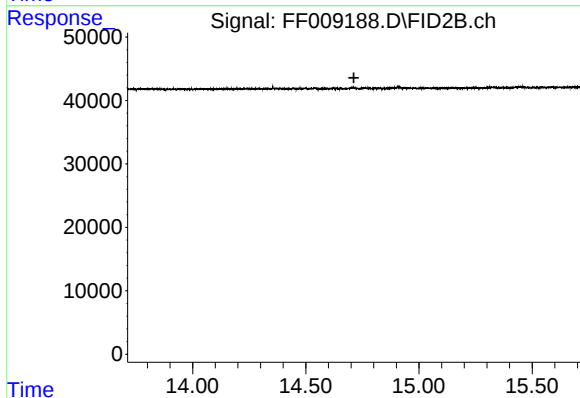

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.712 min
Response: 0
Conc: N.D.

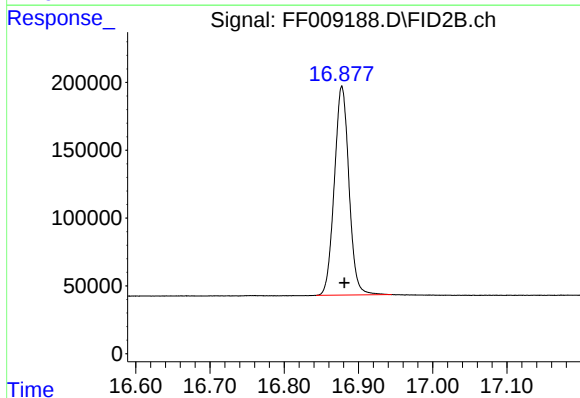

#12 N-OCTACOSANE

R.T.: 16.878 min
Delta R.T.: -0.003 min
Response: 2110505
Conc: 18.03 ug/ml