

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102623\
Data File : FF013627.D
Signal(s) : FID2B.ch
Acq On : 26 Oct 2023 10:02
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 27 01:01:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101623.M
Quant Title :
QLast Update : Mon Oct 16 12:53:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
8)	N-DOCOSANE	14.061	65359	0.497 ug/ml
10)	N-TETRACOSANE	15.167	76243	0.578 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102623\
Data File : FF013627.D
Signal(s) : FID2B.ch
Acq On : 26 Oct 2023 10:02
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 27 01:01:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101623.M
Quant Title :
QLast Update : Mon Oct 16 12:53:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

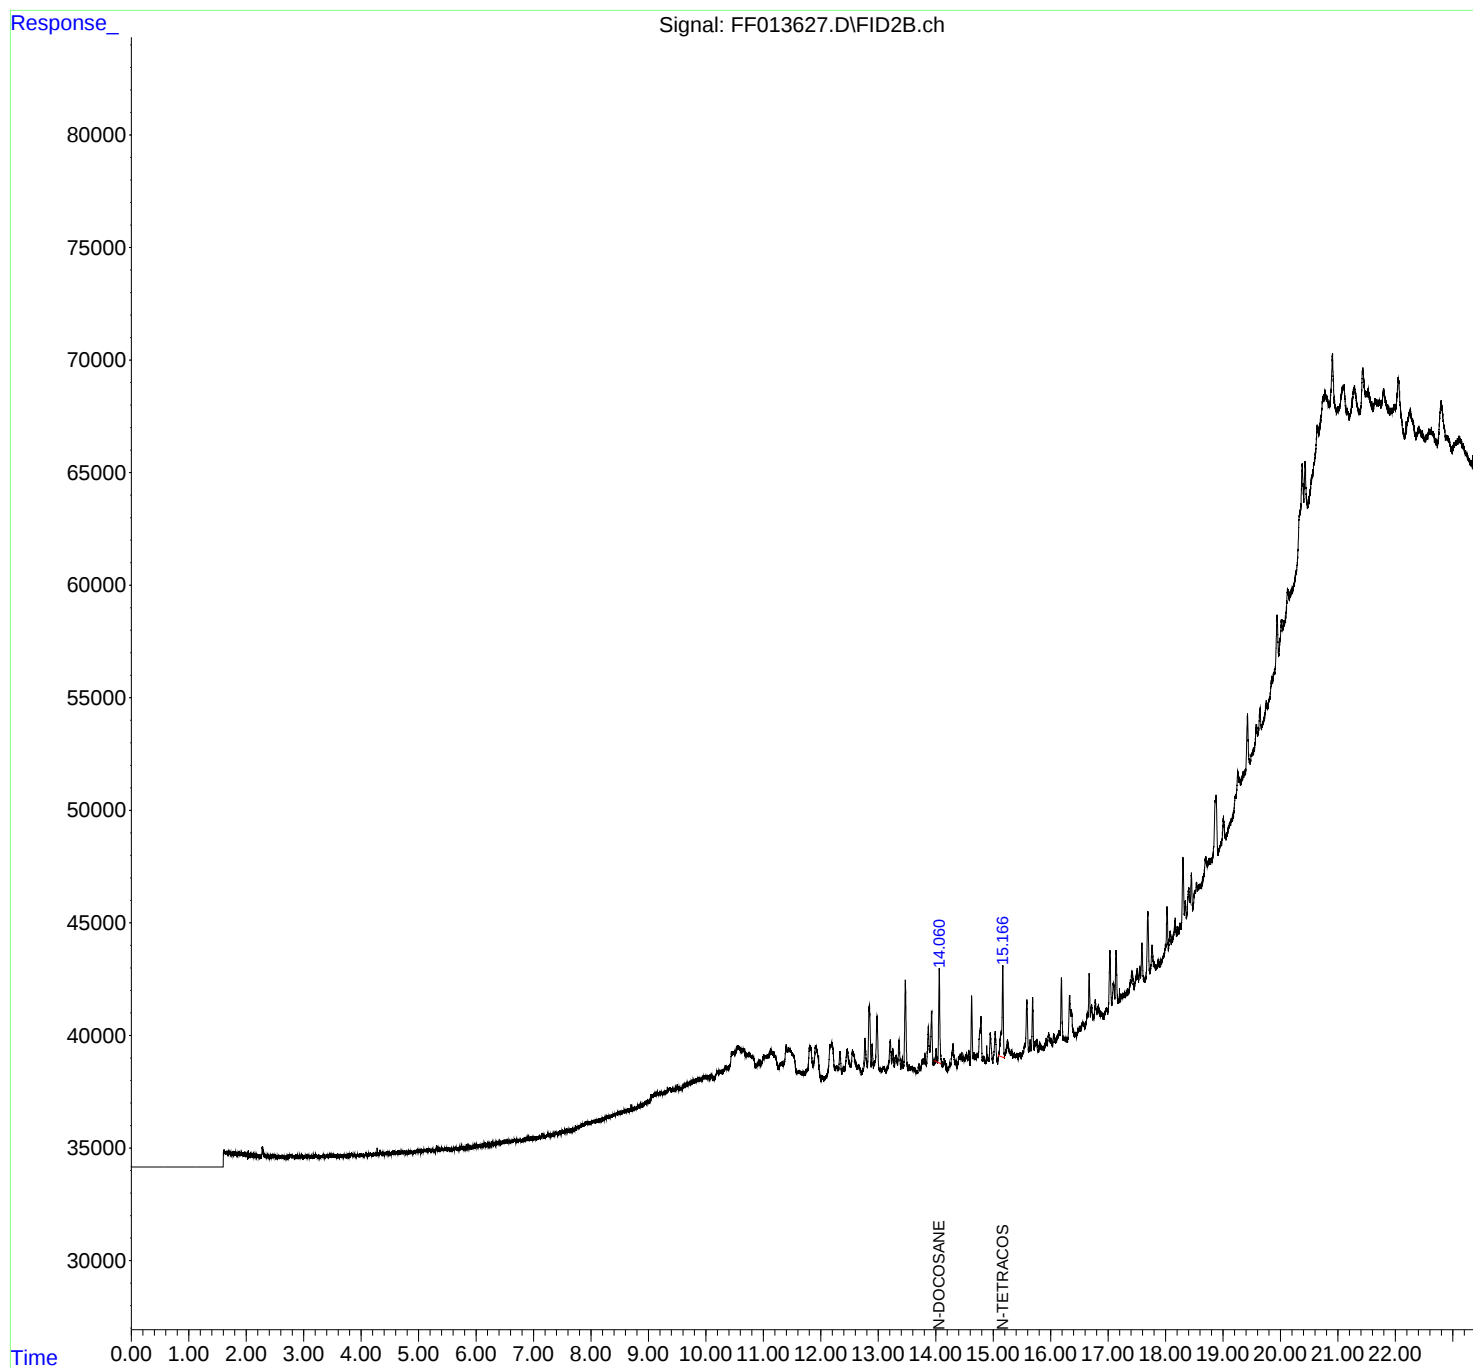


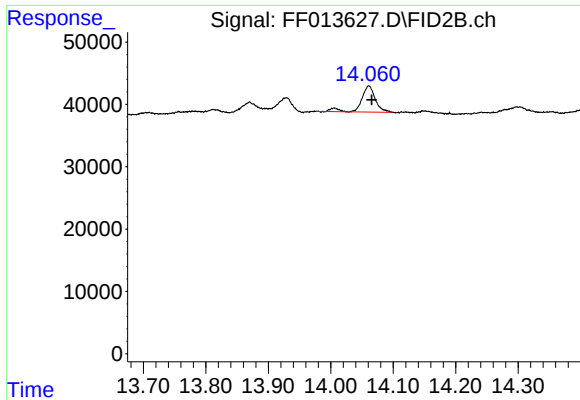

#8 N-DOCOSANE


R.T.: 14.061 min
Delta R.T.: -0.005 min
Response: 65359
Conc: 0.50 ug/ml

Instrument :
FID_F
ClientSampleId :

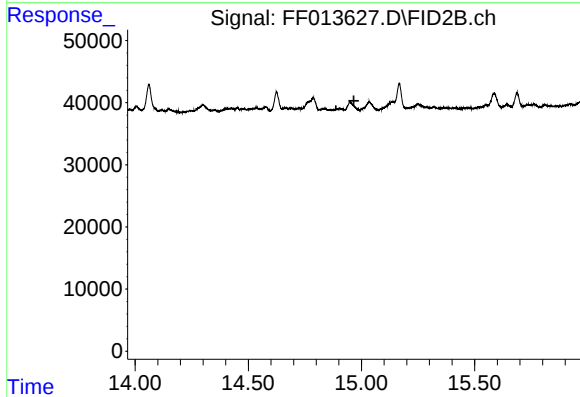

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.966 min
Response: 0
Conc: N.D.

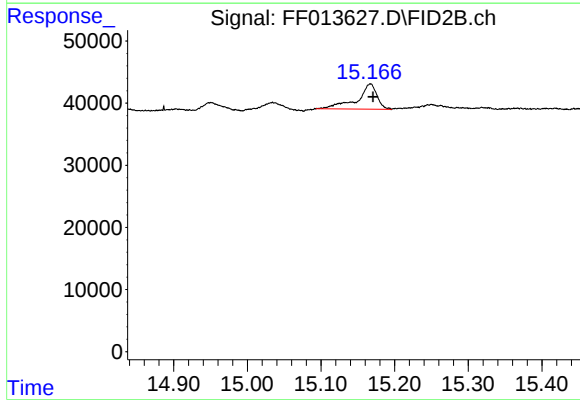

#10 N-TETRACOSANE

R.T.: 15.167 min
Delta R.T.: -0.003 min
Response: 76243
Conc: 0.58 ug/ml