

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102623\
Data File : FF013628.D
Signal(s) : FID2B.ch
Acq On : 26 Oct 2023 12:54
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 27 01:01:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101623.M
Quant Title :
QLast Update : Mon Oct 16 12:53:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.966	2091859	16.730 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.859	59550	0.483 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102623\
Data File : FF013628.D
Signal(s) : FID2B.ch
Acq On : 26 Oct 2023 12:54
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 27 01:01:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101623.M
Quant Title :
QLast Update : Mon Oct 16 12:53:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

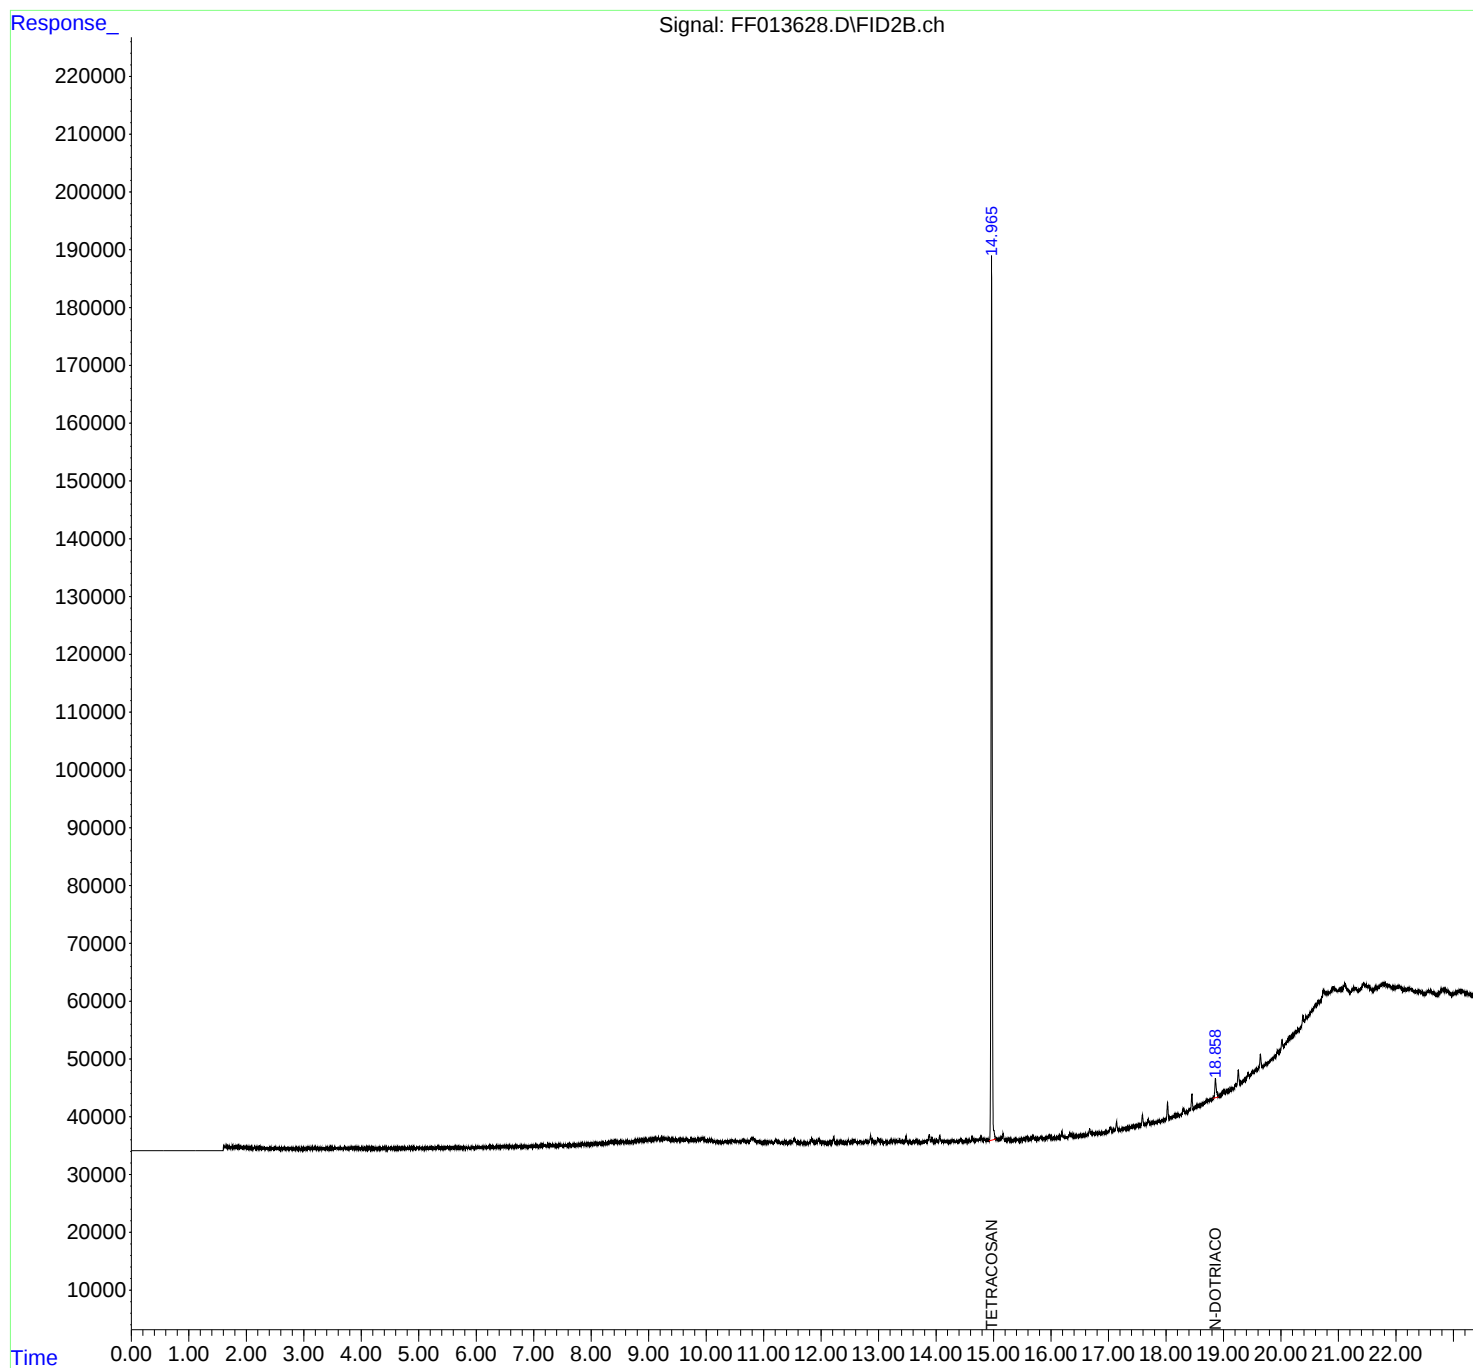


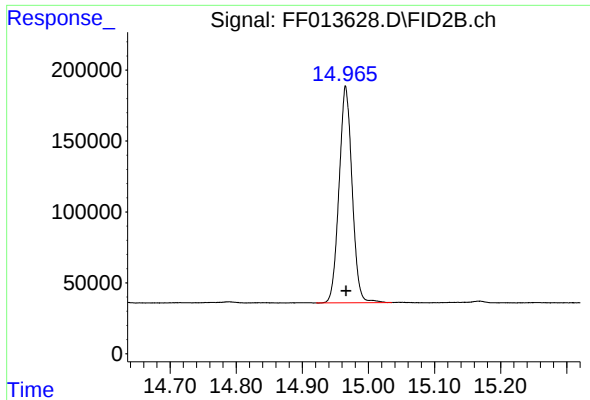

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.966 min
Delta R.T.: 0.000 min
Response: 2091859
Conc: 16.73 ug/ml

Instrument :
FID_F
ClientSampleId :

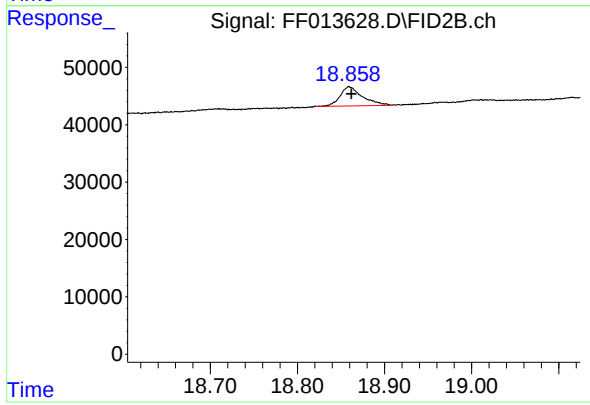

#14 N-DOTRIACONTANE

R.T.: 18.859 min
Delta R.T.: -0.003 min
Response: 59550
Conc: 0.48 ug/ml