

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102623\
Data File : FF013633.D
Signal(s) : FID2B.ch
Acq On : 26 Oct 2023 16:10
Operator : YP\AJ
Sample : 05050-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 27 01:05:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101623.M
Quant Title :
QLast Update : Mon Oct 16 12:53:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.967	1573891	12.587 ug/ml
Target Compounds			
4) N-TETRADECANE	8.471	89041	0.708 ug/ml
12) N-OCTACOSANE	17.190	62393	0.488 ug/ml
14) N-DOTRIACONTANE	18.858	76782	0.623 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102623\
Data File : FF013633.D
Signal(s) : FID2B.ch
Acq On : 26 Oct 2023 16:10
Operator : YP\AJ
Sample : 05050-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 27 01:05:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101623.M
Quant Title :
QLast Update : Mon Oct 16 12:53:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

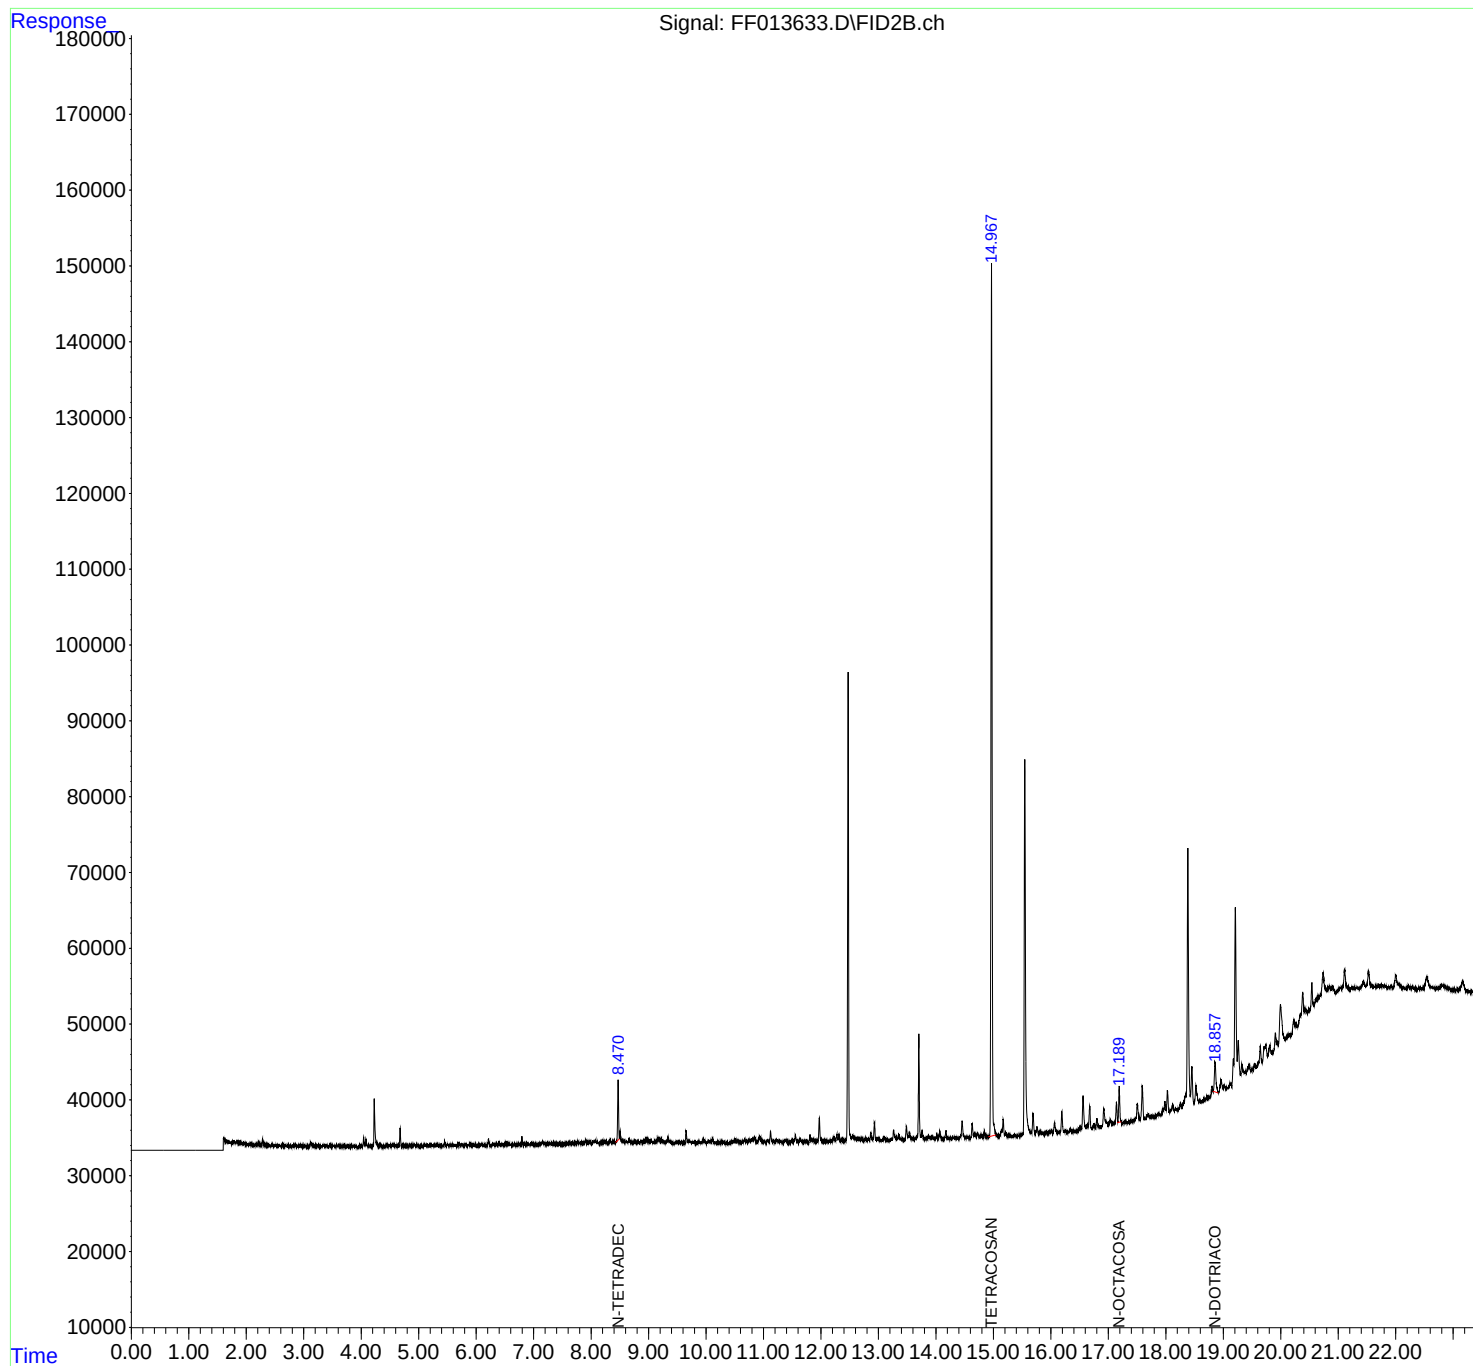


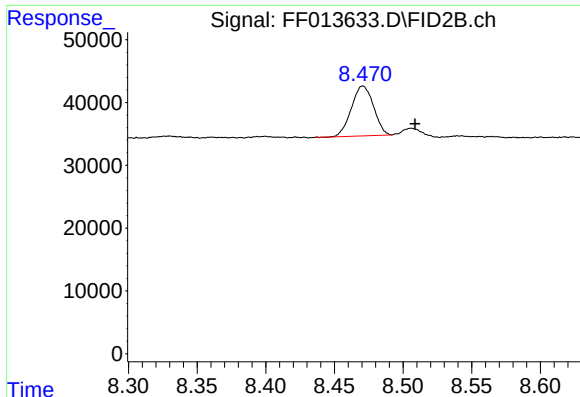

#4 N-TETRADECANE


R.T.: 8.471 min
Delta R.T.: -0.038 min
Response: 89041
Conc: 0.71 ug/ml

Instrument :
FID_F
ClientSampleId :

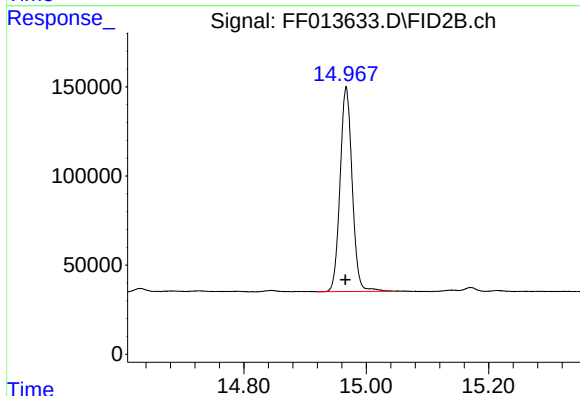


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.967 min
Delta R.T.: 0.000 min
Response: 1573891
Conc: 12.59 ug/ml

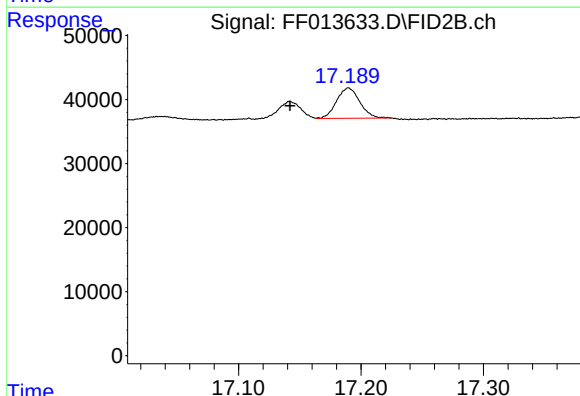

#12 N-OCTACOSANE

R.T.: 17.190 min
Delta R.T.: 0.048 min
Response: 62393
Conc: 0.49 ug/ml

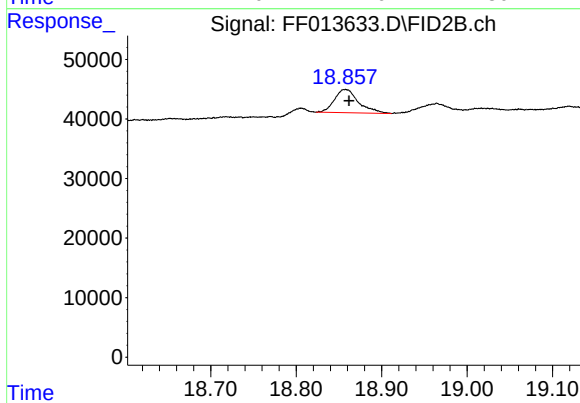

#14 N-DOTRIACONTANE

R.T.: 18.858 min
Delta R.T.: -0.005 min
Response: 76782
Conc: 0.62 ug/ml