

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102720\
Data File : FF007764.D
Signal(s) : FID2B.ch
Acq On : 27 Oct 2020 12:08
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 28 00:57:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
Quant Title :
QLast Update : Mon Oct 05 15:41:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.466	5859622	40.552 ug/ml
12)	N-OCTACOSANE	16.912	5278901	39.414 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102720\
Data File : FF007764.D
Signal(s) : FID2B.ch
Acq On : 27 Oct 2020 12:08
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Oct 28 00:57:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
Quant Title :
QLast Update : Mon Oct 05 15:41:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

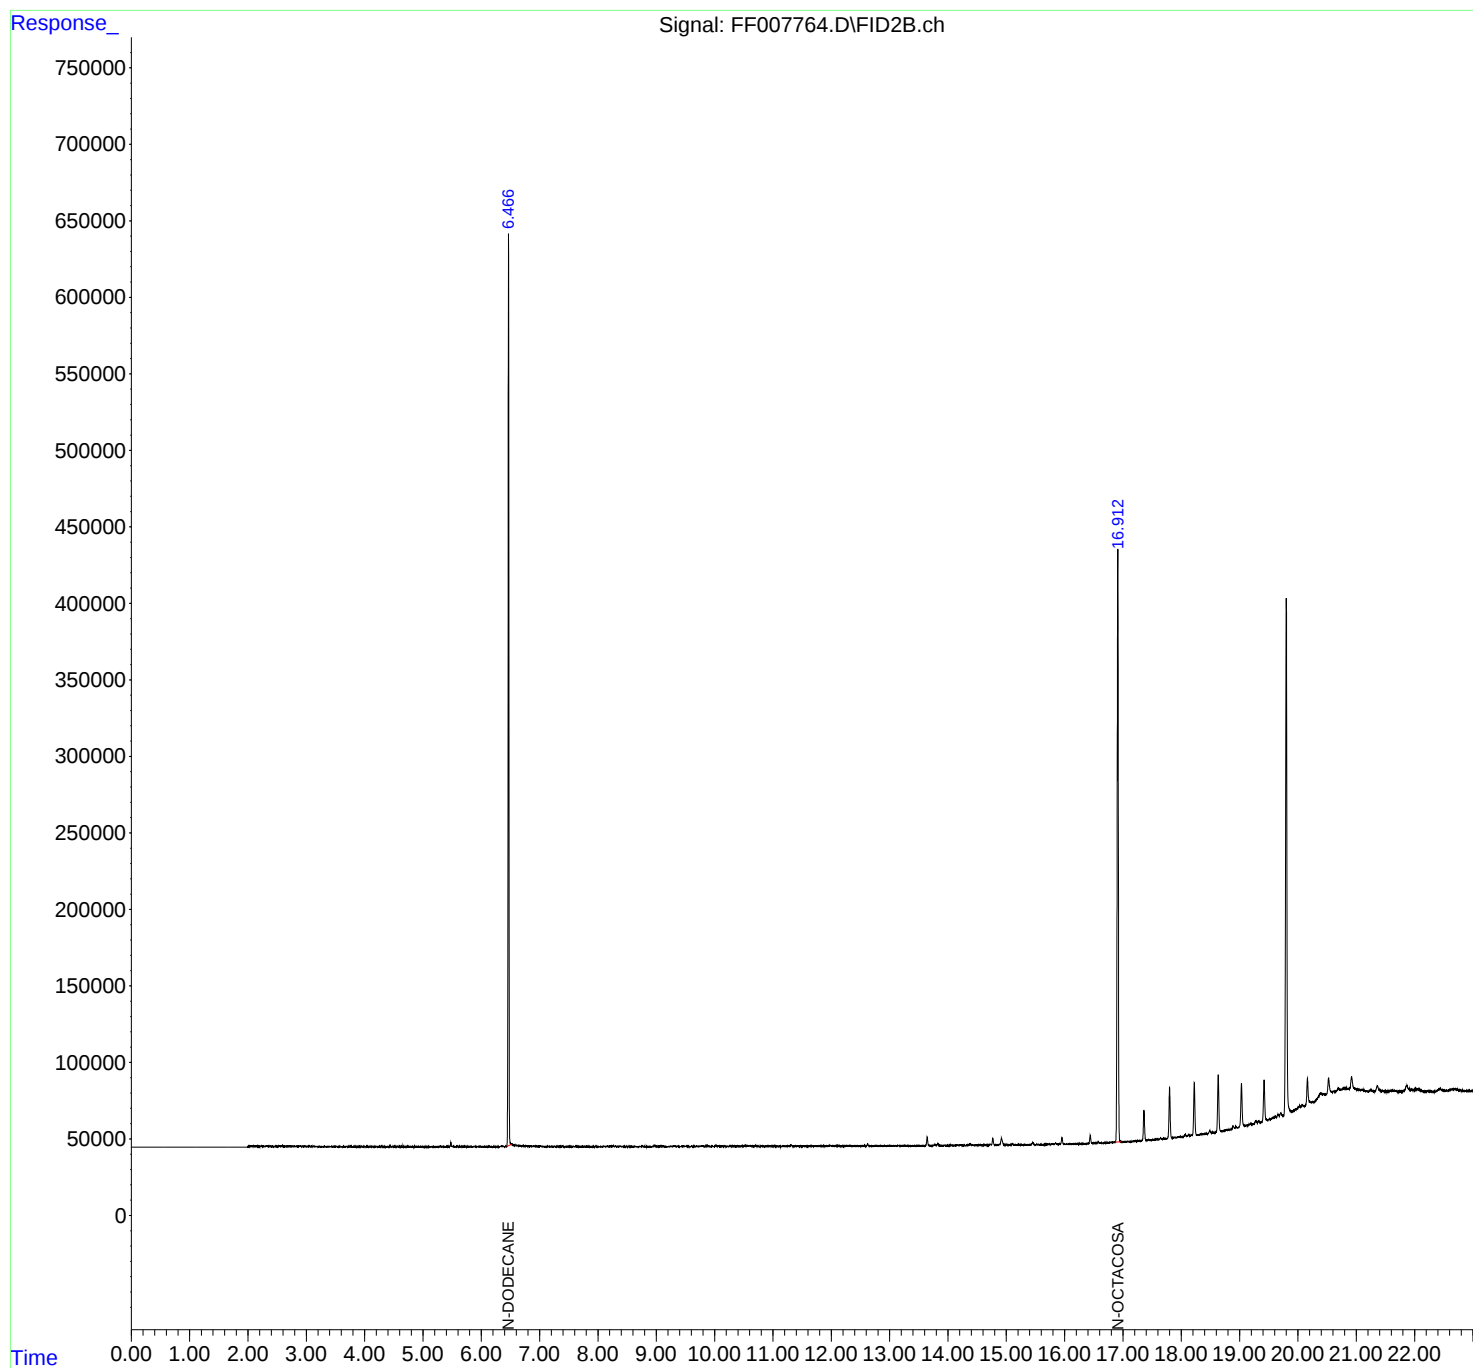


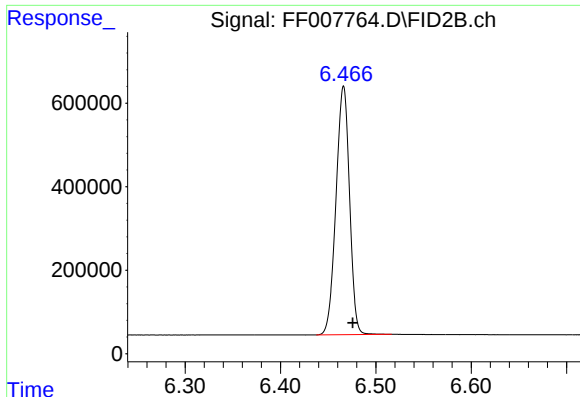

#3 N-DODECANE


R.T.: 6.466 min
Delta R.T.: -0.009 min
Response: 5859622
Conc: 40.55 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

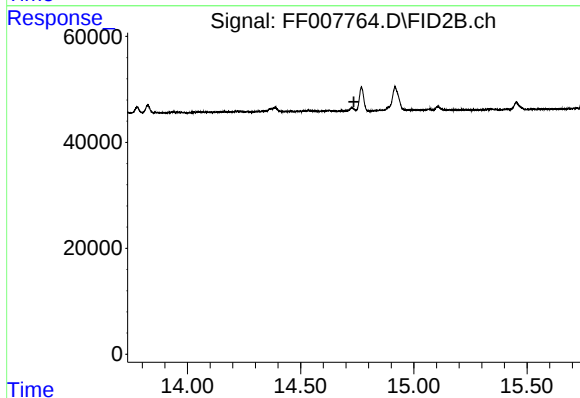

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.735 min
Response: 0
Conc: N.D.

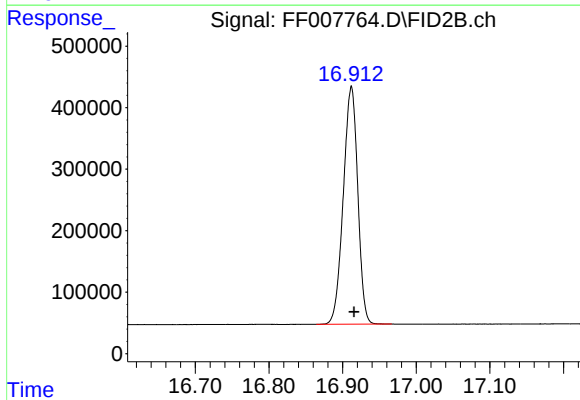

#12 N-OCTACOSANE

R.T.: 16.912 min
Delta R.T.: -0.004 min
Response: 5278901
Conc: 39.41 ug/ml