

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102721\
Data File : FF009210.D
Signal(s) : FID2B.ch
Acq On : 27 Oct 2021 21:25
Operator : AJ\MA
Sample : M4380-01 5X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 28 01:12:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.708	350005	3.192 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.927	128276	1.096 ug/ml
13) N-TRIACONTANE	17.760	141803	1.257 ug/ml
14) N-DOTRIACONTANE	18.594	124761	1.181 ug/ml
15) N-TETRATRIACONTANE	19.373	76603	0.784 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102721\
Data File : FF009210.D
Signal(s) : FID2B.ch
Acq On : 27 Oct 2021 21:25
Operator : AJ\MA
Sample : M4380-01 5X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 28 01:12:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

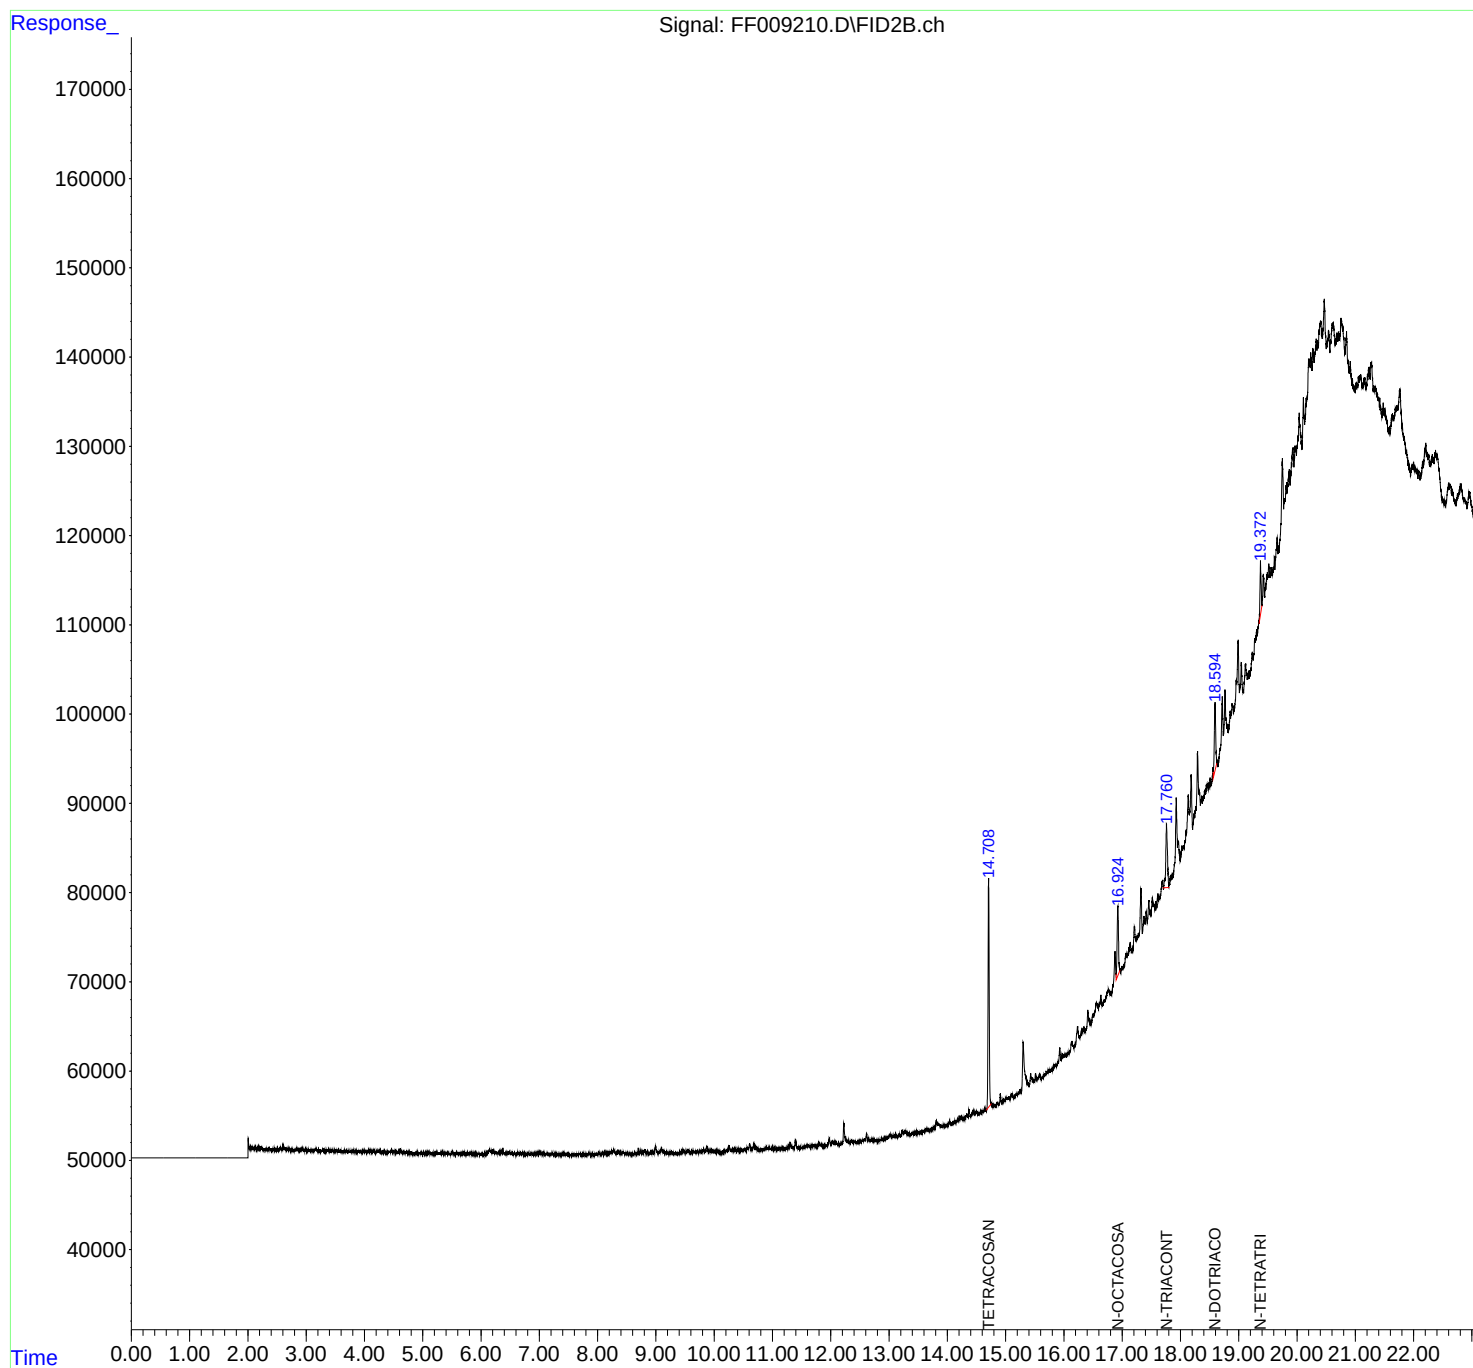

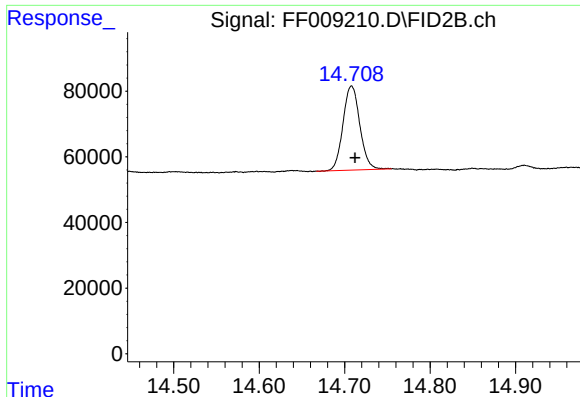


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.708 min
Delta R.T.: -0.004 min
Response: 350005
Conc: 3.19 ug/ml

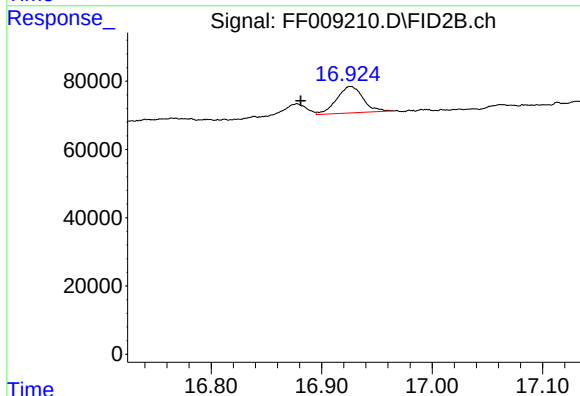


#12 N-OCTACOSANE

R.T.: 16.927 min
Delta R.T.: 0.046 min
Response: 128276
Conc: 1.10 ug/ml

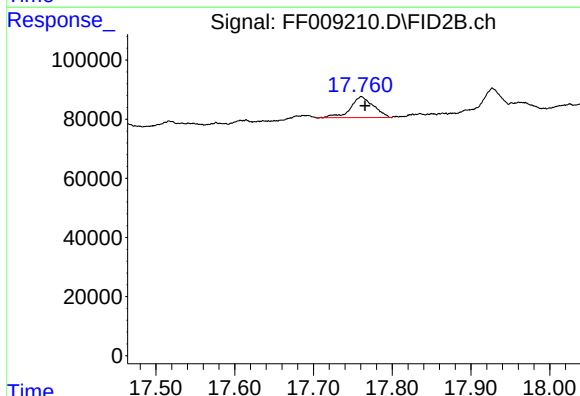


#13 N-TRIACONTANE

R.T.: 17.760 min
Delta R.T.: -0.005 min
Response: 141803
Conc: 1.26 ug/ml

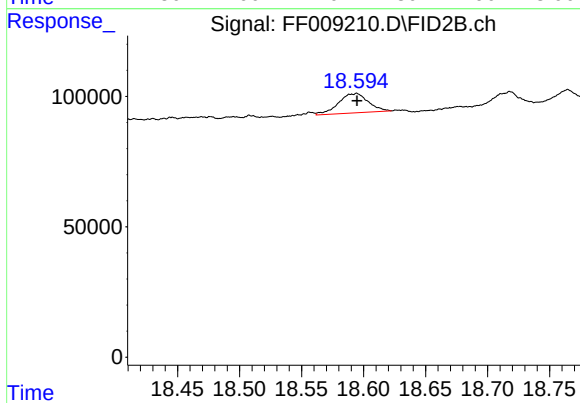

#14 N-DOTRIACONTANE

R.T.: 18.594 min
Delta R.T.: 0.000 min
Response: 124761
Conc: 1.18 ug/ml

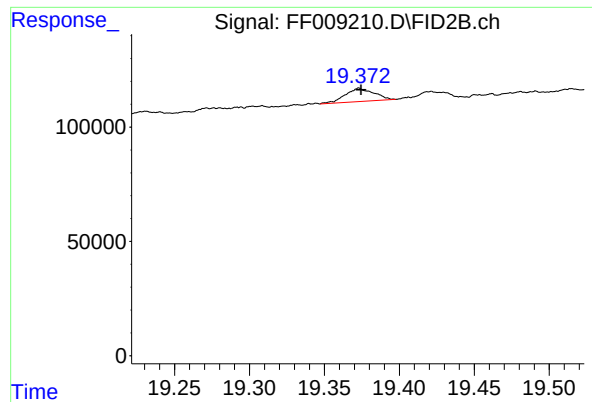

#15 N-TETRATRIACONTANE

R.T.:	19.373 min
Delta R.T.:	-0.001 min
Response:	76603
Conc:	0.78 ug/ml