

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102721\
 Data File : FF009199.D
 Signal(s) : FID2B.ch
 Acq On : 27 Oct 2021 10:26
 Operator : AJ\MA
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Oct 28 01:09:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
 Quant Title :
 QLast Update : Fri Oct 08 02:25:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.708	5061305	46.156 ug/ml
Target Compounds			
2) N-DECANE	4.464	6874899	54.243 ug/ml
3) N-DODECANE	6.482	6780803	53.375 ug/ml
4) N-TETRADECANE	8.273	6629150	52.871 ug/ml
5) N-HEXADECANE	9.871	6496131	51.167 ug/ml
6) N-OCTADECANE	11.310	6449050	50.026 ug/ml
7) N-EICOSANE	12.616	6283597	48.810 ug/ml
8) N-DOCOSANE	13.811	6021517	47.629 ug/ml
10) N-TETRACOSANE	14.912	5827424	46.553 ug/ml
11) N-HEXACOSANE	15.930	5593702	46.207 ug/ml
12) N-OCTACOSANE	16.877	5409963	46.214 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102721\
Data File : FF009199.D
Signal(s) : FID2B.ch
Acq On : 27 Oct 2021 10:26
Operator : AJ\MA
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Oct 28 01:09:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

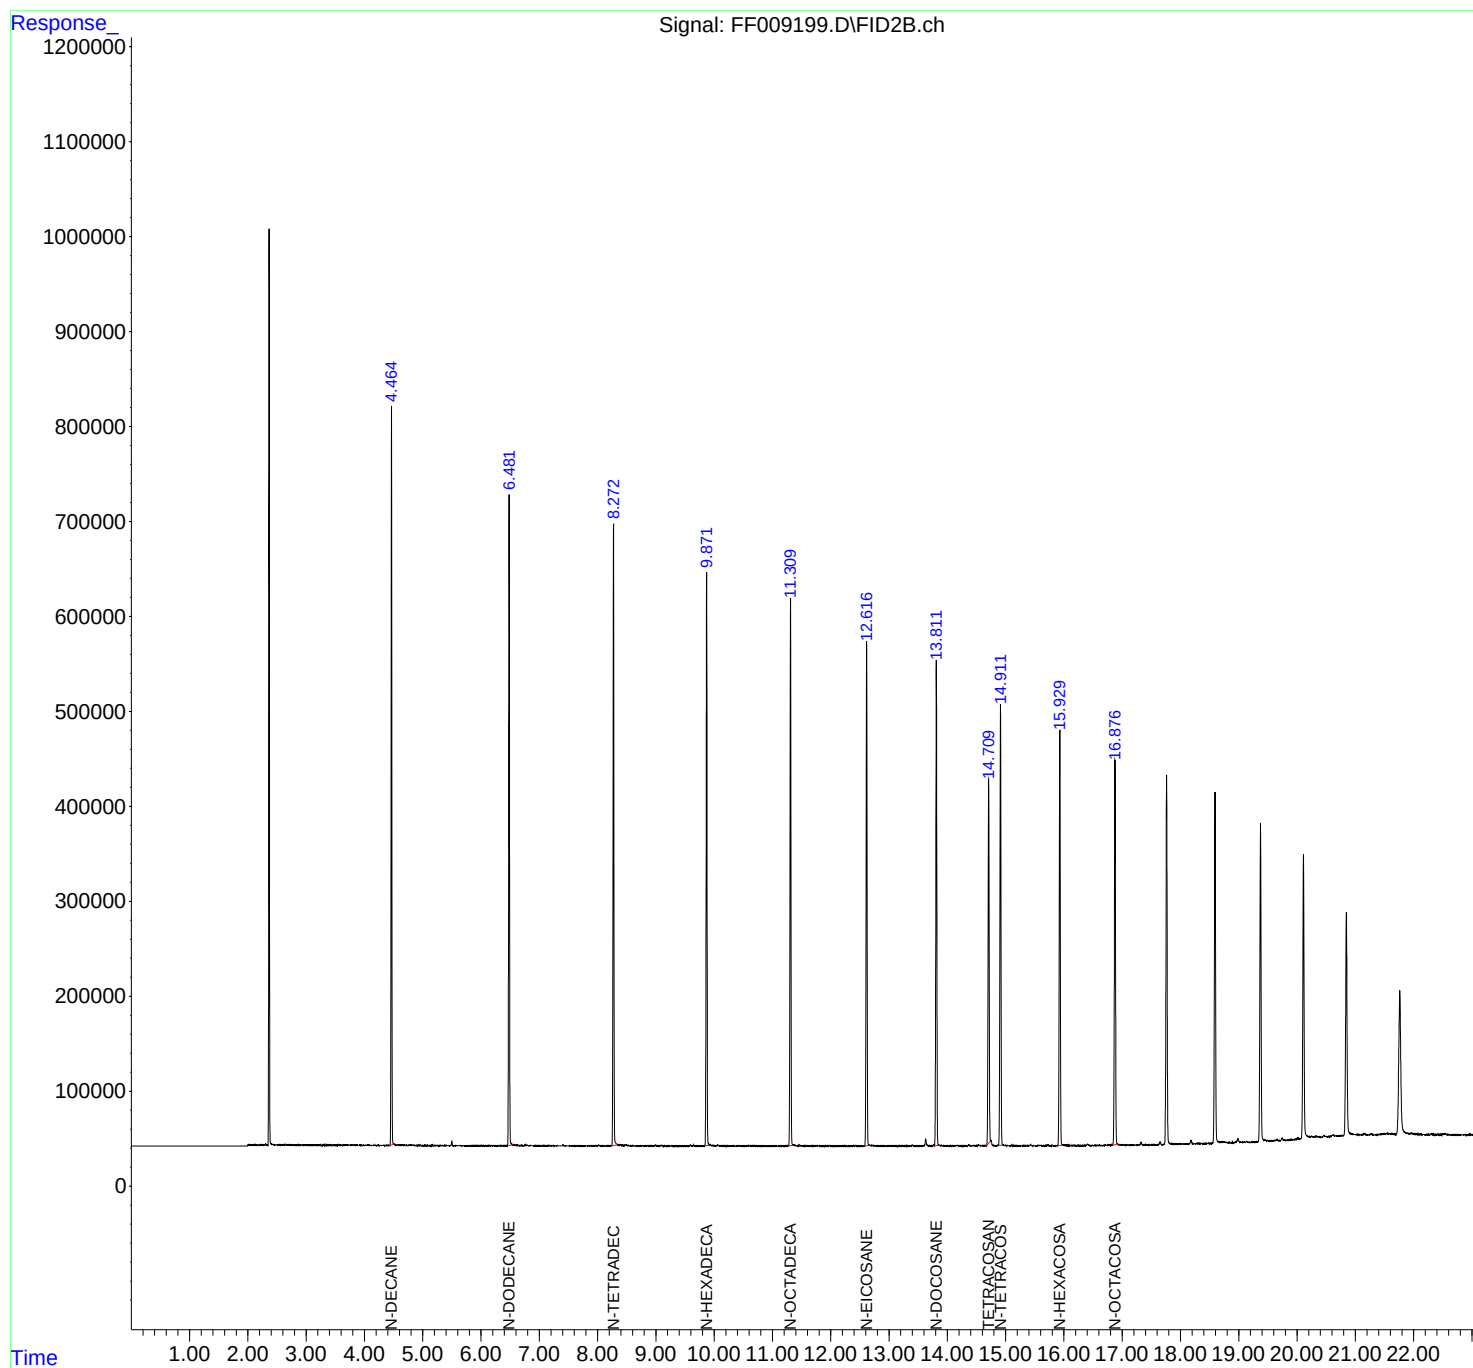

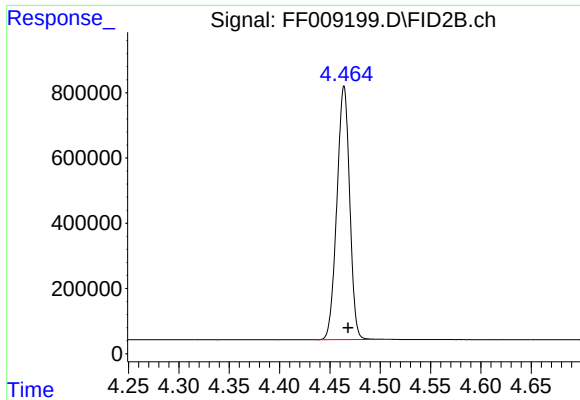


#2 N-DECANE

R.T.: 4.464 min
Delta R.T.: -0.004 min
Response: 6874899
Conc: 54.24 ug/ml

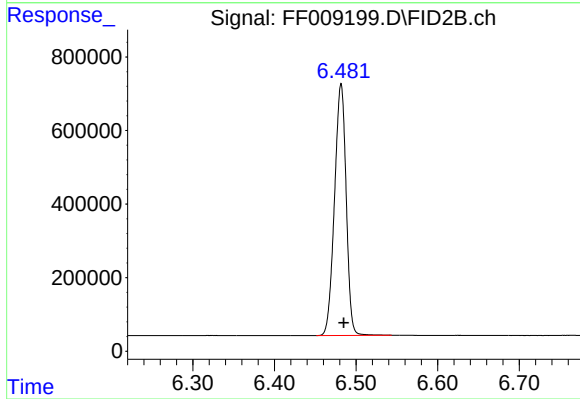


#3 N-DODECANE

R.T.: 6.482 min
Delta R.T.: -0.003 min
Response: 6780803
Conc: 53.37 ug/ml

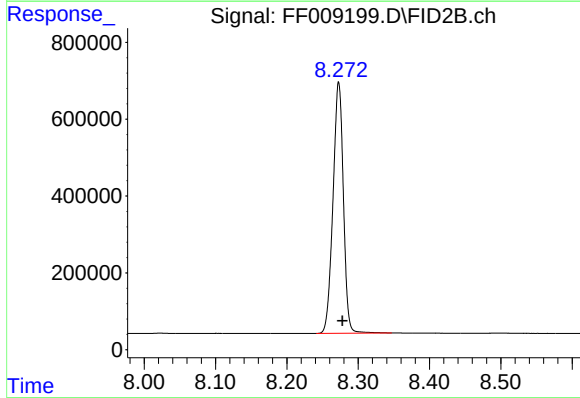


#4 N-TETRADECANE

R.T.: 8.273 min
Delta R.T.: -0.005 min
Response: 6629150
Conc: 52.87 ug/ml

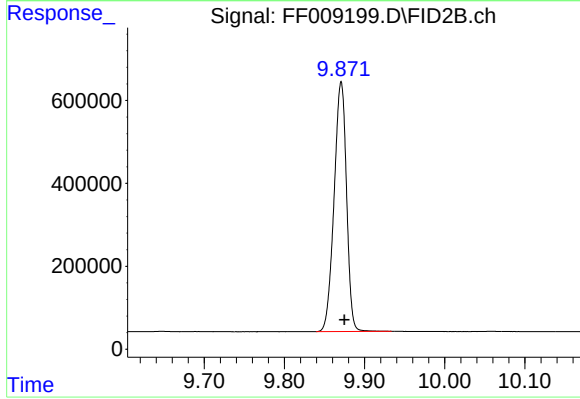


#5 N-HEXADECANE

R.T.: 9.871 min
Delta R.T.: -0.004 min
Response: 6496131
Conc: 51.17 ug/ml

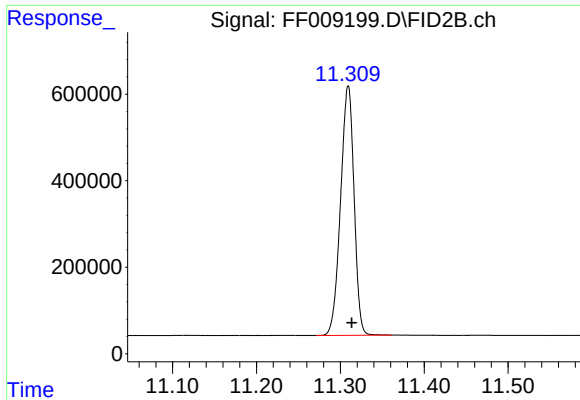


#6 N-OCTADECANE

R.T.: 11.310 min
Delta R.T.: -0.004 min
Response: 6449050
Conc: 50.03 ug/ml

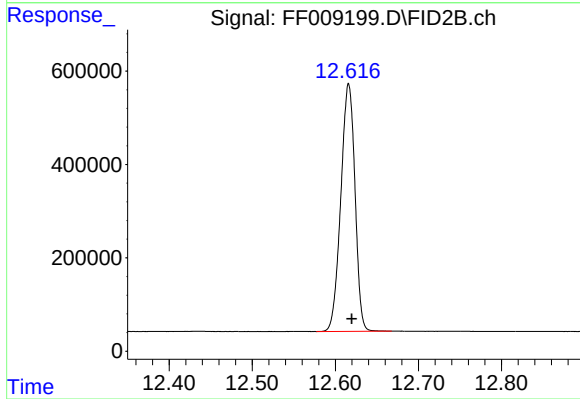


#7 N-EICOSANE

R.T.: 12.616 min
Delta R.T.: -0.004 min
Response: 6283597
Conc: 48.81 ug/ml

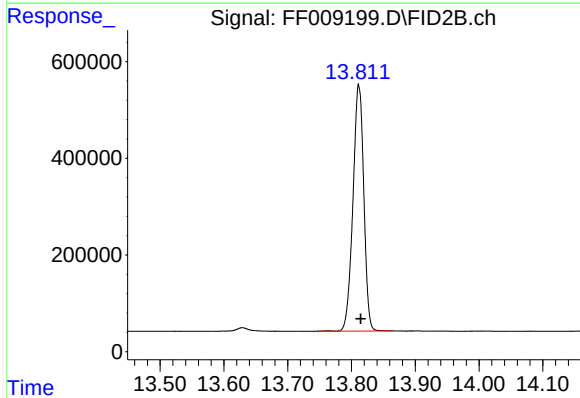


#8 N-DOCOSANE

R.T.: 13.811 min
Delta R.T.: -0.003 min
Response: 6021517
Conc: 47.63 ug/ml

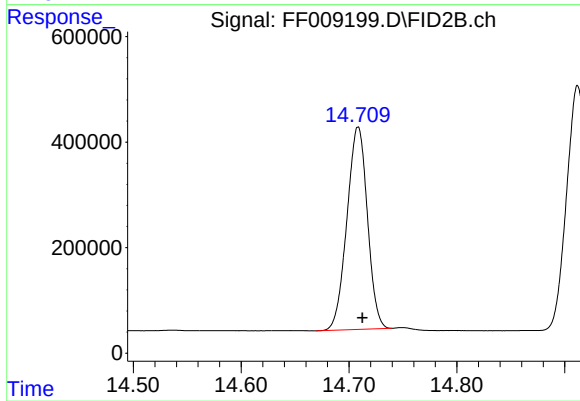


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.708 min
Delta R.T.: -0.004 min
Response: 5061305
Conc: 46.16 ug/ml

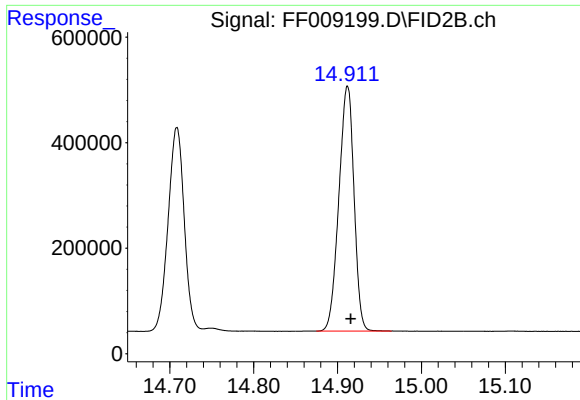


#10 N-TETRACOSANE

R.T.: 14.912 min
Delta R.T.: -0.004 min
Response: 5827424
Conc: 46.55 ug/ml

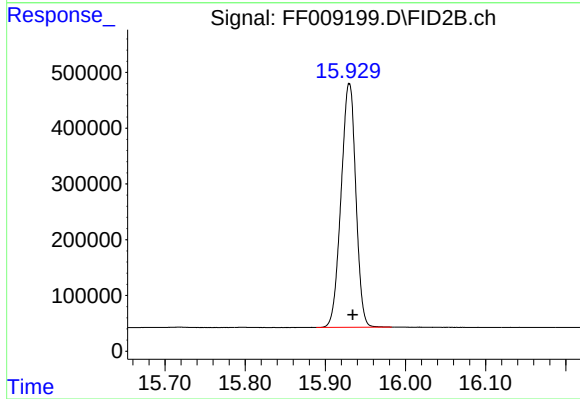

#11 N-HEXACOSANE

R.T.: 15.930 min
Delta R.T.: -0.004 min
Response: 5593702
Conc: 46.21 ug/ml

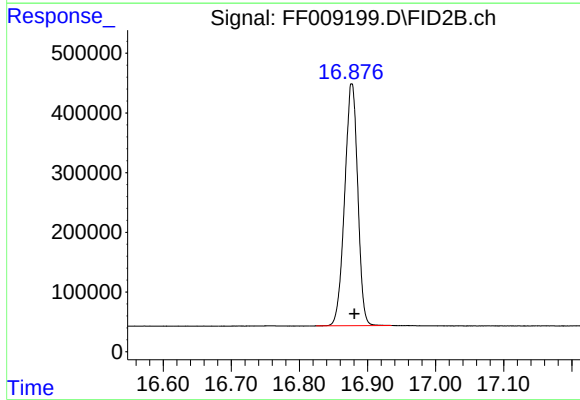

#12 N-OCTACOSANE

R.T.: 16.877 min
Delta R.T.: -0.004 min
Response: 5409963
Conc: 46.21 ug/ml