

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF102820\  
Data File : FF007774.D  
Signal(s) : FID2B.ch  
Acq On : 28 Oct 2020 11:11  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Oct 29 01:26:44 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF100220.M  
Quant Title :  
QLast Update : Mon Oct 05 15:41:23 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

|                             | Compound                 | R.T.   | Response | Conc Units   |
|-----------------------------|--------------------------|--------|----------|--------------|
| -----                       |                          |        |          |              |
| System Monitoring Compounds |                          |        |          |              |
| 9) S                        | TETRACOSANE-d50 (SURR... | 14.726 | 2073503  | 16.476 ug/ml |
|                             |                          |        |          |              |
| Target Compounds            |                          |        |          |              |
| 10)                         | N-TETRACOSANE            | 14.911 | 190752   | 1.322 ug/ml  |
| -----                       |                          |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF102820\  
Data File : FF007774.D  
Signal(s) : FID2B.ch  
Acq On : 28 Oct 2020 11:11  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Oct 29 01:26:44 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF100220.M  
Quant Title :  
QLast Update : Mon Oct 05 15:41:23 2020  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

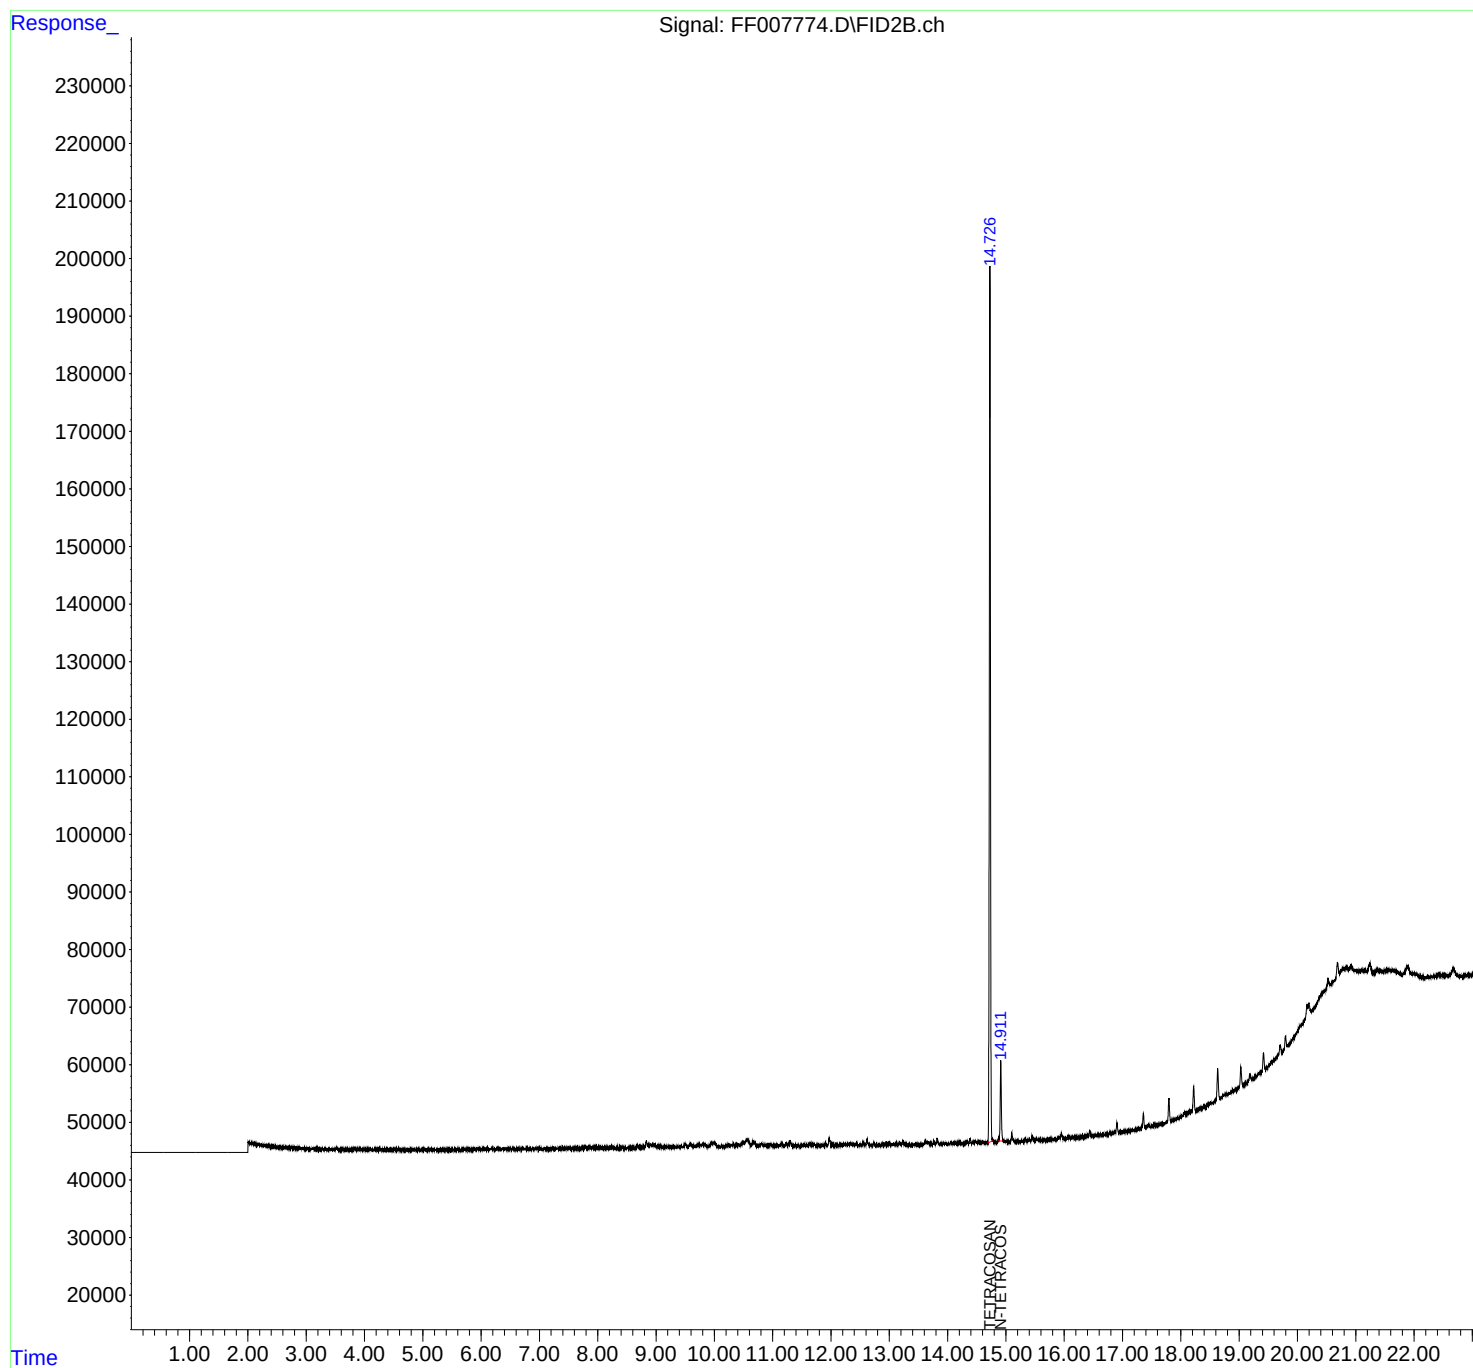

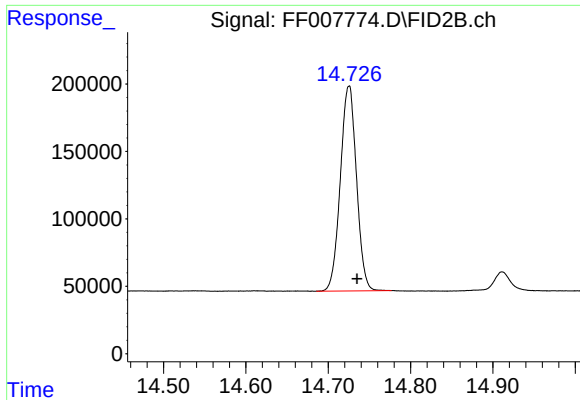

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.726 min  
Delta R.T.: -0.009 min  
Response: 2073503  
Conc: 16.48 ug/ml

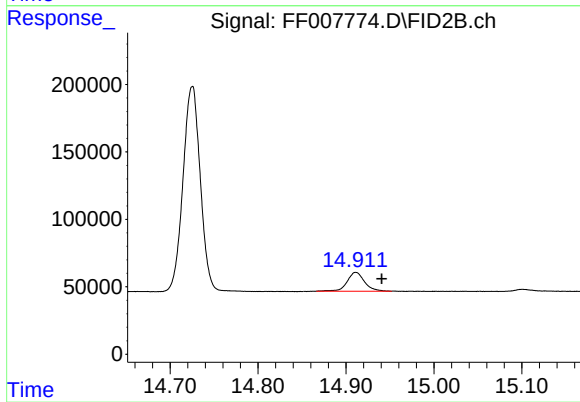

#10 N-TETRACOSANE

R.T.: 14.911 min  
Delta R.T.: -0.030 min  
Response: 190752  
Conc: 1.32 ug/ml