

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102820\
 Data File : FF007783.D
 Signal(s) : FID2B.ch
 Acq On : 28 Oct 2020 16:23
 Operator : DD\AJ
 Sample : PB132671BS
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Oct 29 01:29:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
 Quant Title :
 QLast Update : Mon Oct 05 15:41:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.729	2489535	19.782 ug/ml
Target Compounds			
2) N-DECANE	4.445	3293860	23.222 ug/ml
3) N-DODECANE	6.470	3288332	22.757 ug/ml
4) N-TETRADECANE	8.267	3245461	22.260 ug/ml
5) N-HEXADECANE	9.870	3162570	21.154 ug/ml
6) N-OCTADECANE	11.315	3103099	20.597 ug/ml
7) N-EICOSANE	12.627	3057382	20.565 ug/ml
8) N-DOCOSANE	13.828	2947218	20.205 ug/ml
10) N-TETRACOSANE	14.934	2865393	19.864 ug/ml
11) N-HEXACOSANE	15.958	2729458	19.648 ug/ml
12) N-OCTACOSANE	16.910	2694433	20.117 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102820\
Data File : FF007783.D
Signal(s) : FID2B.ch
Acq On : 28 Oct 2020 16:23
Operator : DD\AJ
Sample : PB132671BS
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Oct 29 01:29:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
Quant Title :
QLast Update : Mon Oct 05 15:41:23 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

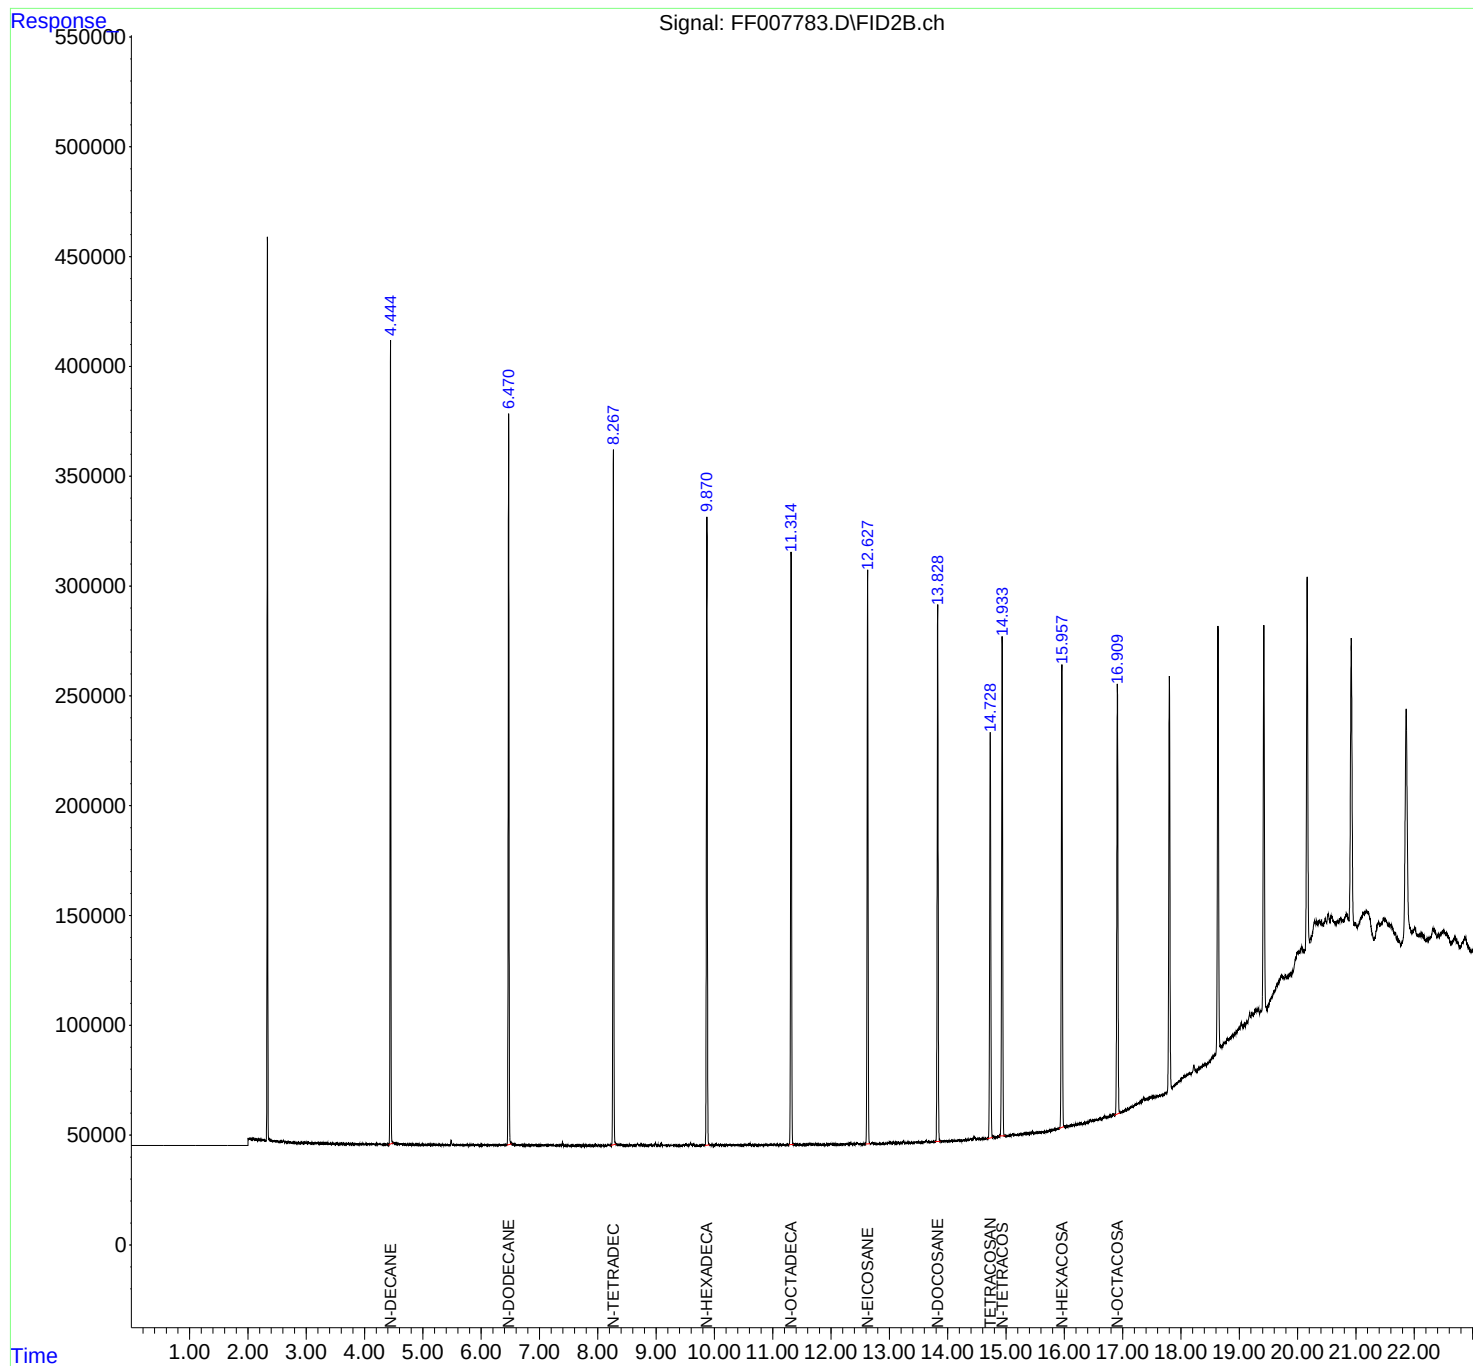

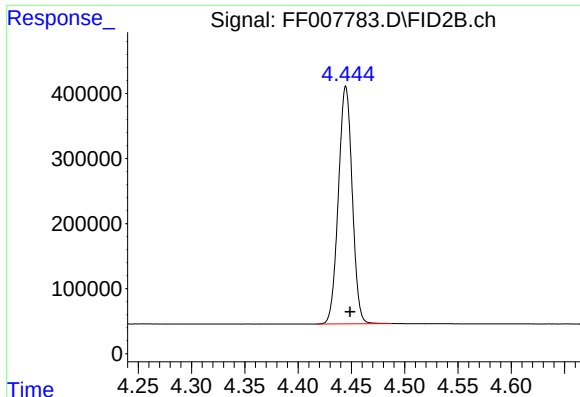


#2 N-DECANE

R.T.: 4.445 min
Delta R.T.: -0.004 min
Response: 3293860
Conc: 23.22 ug/ml

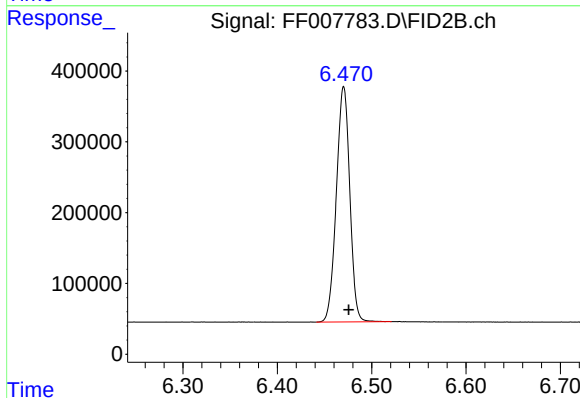


#3 N-DODECANE

R.T.: 6.470 min
Delta R.T.: -0.005 min
Response: 3288332
Conc: 22.76 ug/ml

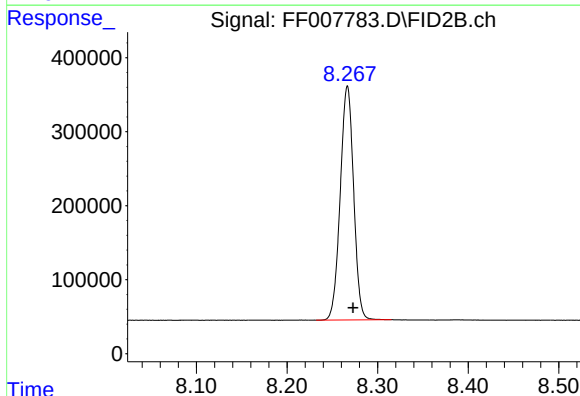


#4 N-TETRADECANE

R.T.: 8.267 min
Delta R.T.: -0.006 min
Response: 3245461
Conc: 22.26 ug/ml

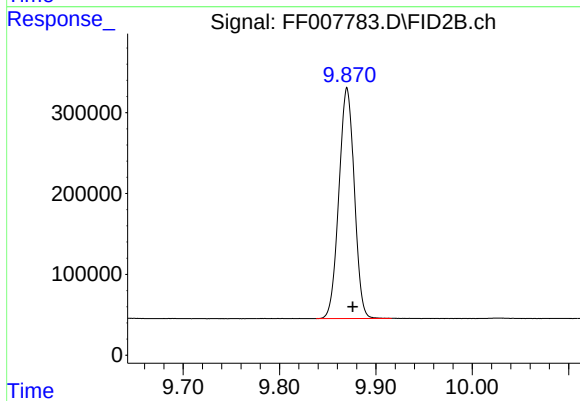


#5 N-HEXADECANE

R.T.: 9.870 min
Delta R.T.: -0.006 min
Response: 3162570
Conc: 21.15 ug/ml

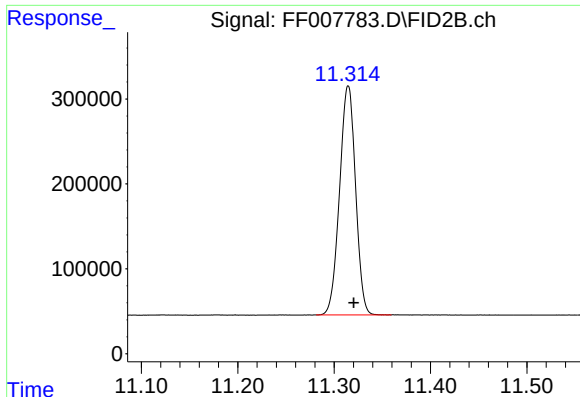


#6 N-OCTADECANE

R.T.: 11.315 min
Delta R.T.: -0.006 min
Response: 3103099
Conc: 20.60 ug/ml

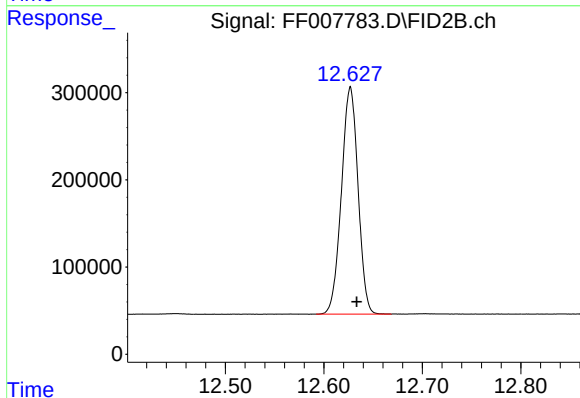


#7 N-EICOSANE

R.T.: 12.627 min
Delta R.T.: -0.006 min
Response: 3057382
Conc: 20.56 ug/ml

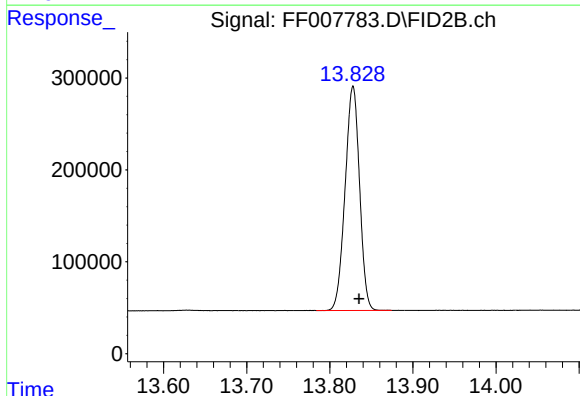


#8 N-DOCOSANE

R.T.: 13.828 min
Delta R.T.: -0.007 min
Response: 2947218
Conc: 20.20 ug/ml

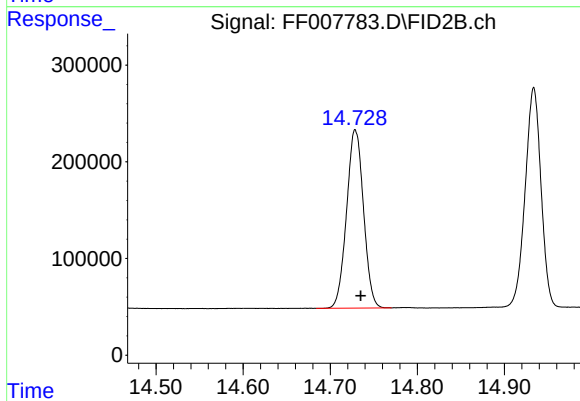


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.729 min
Delta R.T.: -0.006 min
Response: 2489535
Conc: 19.78 ug/ml

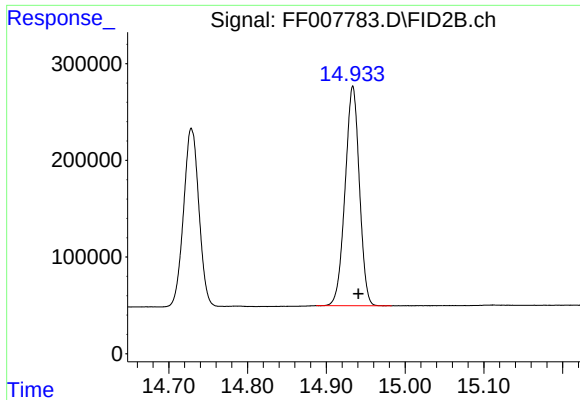


#10 N-TETRACOSANE

R.T.: 14.934 min
Delta R.T.: -0.007 min
Response: 2865393
Conc: 19.86 ug/ml

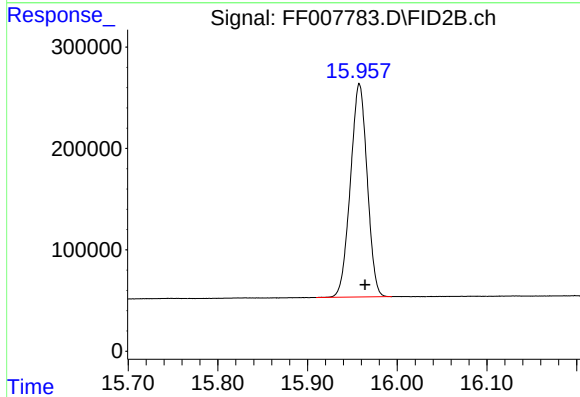

#11 N-HEXACOSANE

R.T.: 15.958 min
Delta R.T.: -0.006 min
Response: 2729458
Conc: 19.65 ug/ml

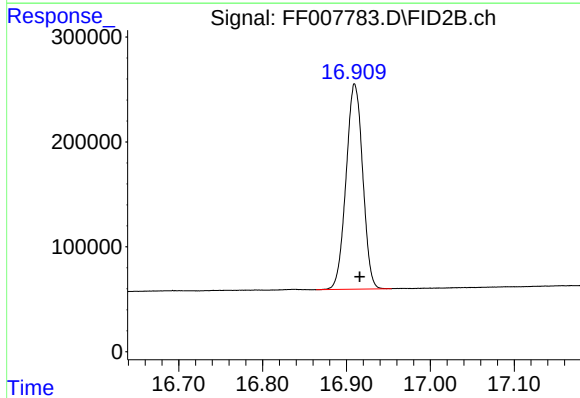

#12 N-OCTACOSANE

R.T.: 16.910 min
Delta R.T.: -0.006 min
Response: 2694433
Conc: 20.12 ug/ml