

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102920\
Data File : FF007791.D
Signal(s) : FID2B.ch
Acq On : 29 Oct 2020 10:45
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 30 02:43:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
Quant Title :
QLast Update : Mon Oct 05 15:41:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.467	6515166	45.089 ug/ml
12)	N-OCTACOSANE	16.913	6106446	45.592 ug/ml
13)	N-TRIACONTANE	17.800	663504	5.131 ug/ml
14)	N-DOTRIACONTANE	18.636	817789	6.797 ug/ml
15)	N-TETRATRIACONTANE	19.422	604324	5.751 ug/ml
16)	N-HEXATRIACONTANE	20.167	407032	4.266 ug/ml
17)	N-OCTATRIACONTANE	20.924	229639	2.779 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102920\
Data File : FF007791.D
Signal(s) : FID2B.ch
Acq On : 29 Oct 2020 10:45
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 30 02:43:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
Quant Title :
QLast Update : Mon Oct 05 15:41:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

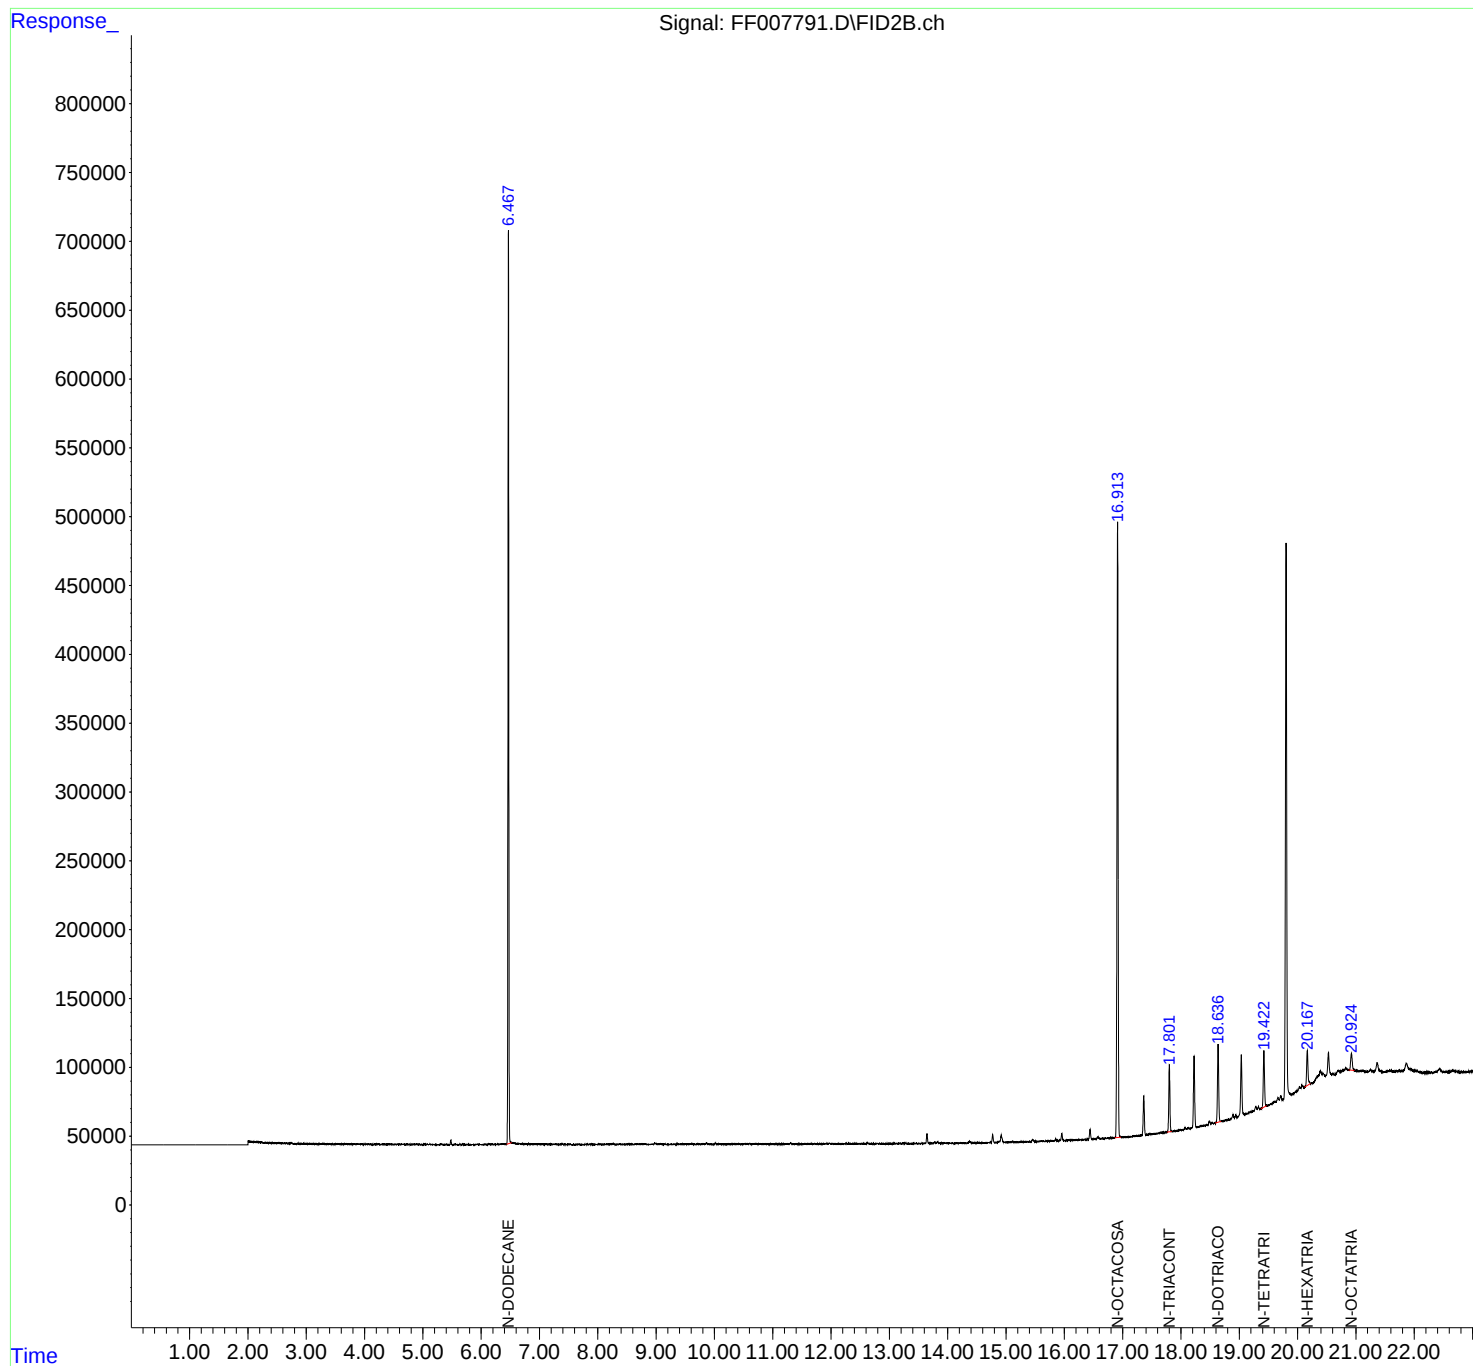


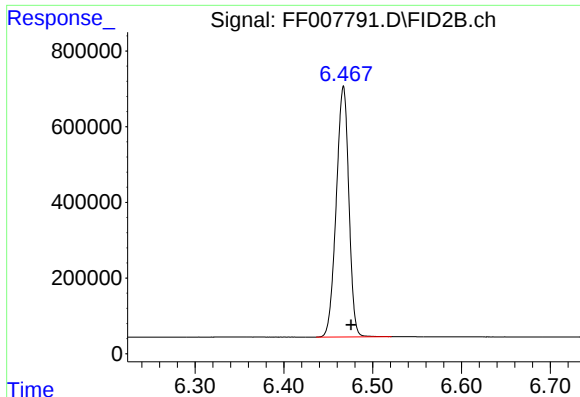

#3 N-DODECANE


R.T.: 6.467 min
Delta R.T.: -0.009 min
Response: 6515166
Conc: 45.09 ug/ml

Instrument :
FID_F
ClientSampleId :

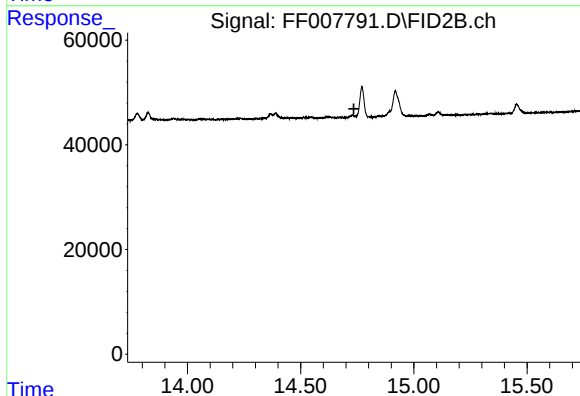


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.735 min
Response: 0
Conc: N.D.

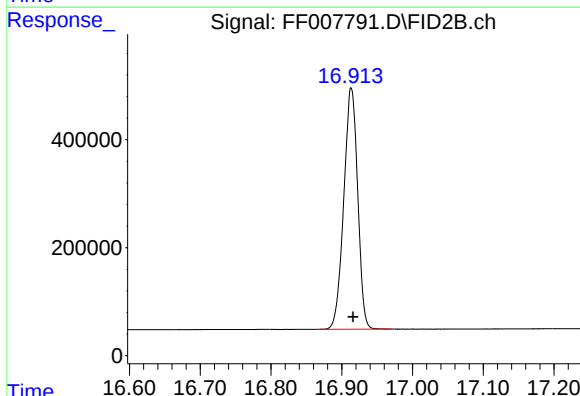


#12 N-OCTACOSANE

R.T.: 16.913 min
Delta R.T.: -0.003 min
Response: 6106446
Conc: 45.59 ug/ml

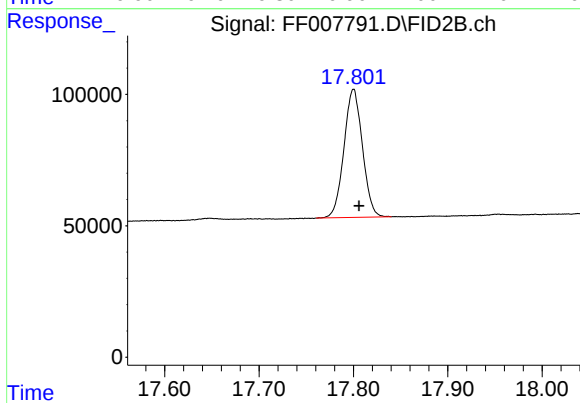

#13 N-TRIACONTANE


R.T.: 17.800 min
Delta R.T.: -0.006 min
Response: 663504
Conc: 5.13 ug/ml

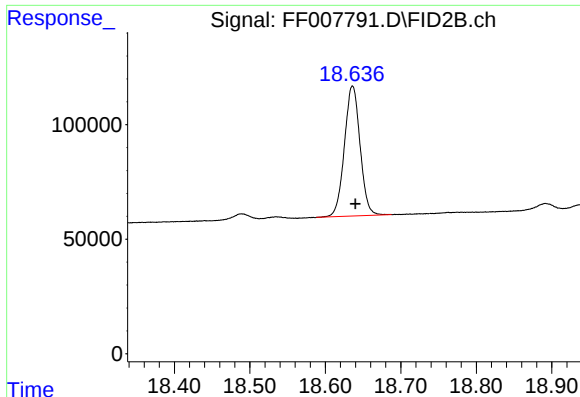

#14 N-DOTRIACONTANE


R.T.: 18.636 min
Delta R.T.: -0.004 min
Response: 817789
Conc: 6.80 ug/ml

Instrument :
FID_F
ClientSampleId :

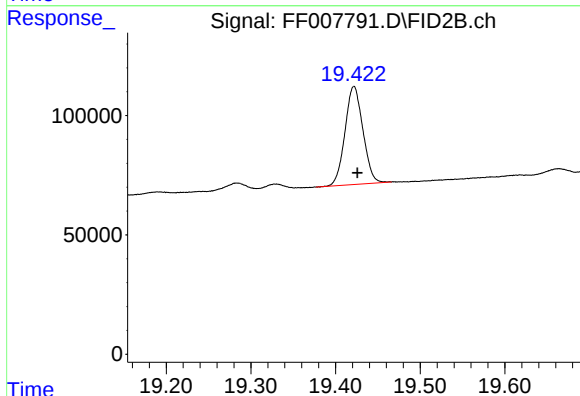


#15 N-TETRATRIACONTANE

R.T.: 19.422 min
Delta R.T.: -0.004 min
Response: 604324
Conc: 5.75 ug/ml

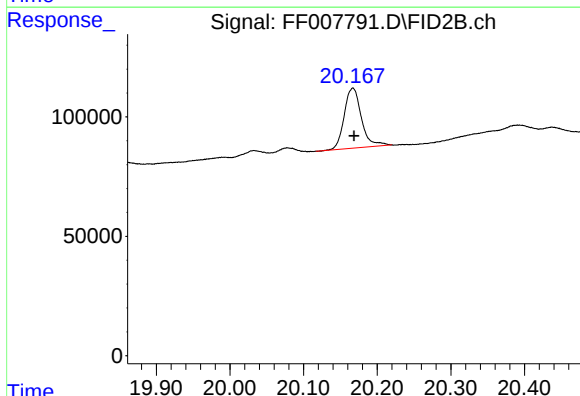

#16 N-HEXATRIACONTANE

R.T.: 20.167 min
Delta R.T.: -0.001 min
Response: 407032
Conc: 4.27 ug/ml

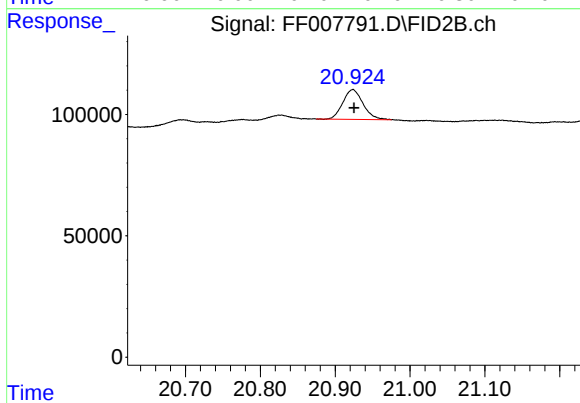

#17 N-OCTATRIACONTANE

R.T.: 20.924 min
Delta R.T.: -0.002 min
Response: 229639
Conc: 2.78 ug/ml