

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102920\
 Data File : FF007795.D
 Signal(s) : FID2B.ch
 Acq On : 29 Oct 2020 12:50
 Operator : DD\AJ
 Sample : PB132701BL
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 30 02:44:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
 Quant Title :
 QLast Update : Mon Oct 05 15:41:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.736	1917931	15.240 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.649	65038	0.541 ug/ml
15) N-TETRATRIACONTANE	19.429	158281	1.506 ug/ml
16) N-HEXATRIACONTANE	20.171	67007	0.702 ug/ml
17) N-OCTATRIACONTANE	20.994f	85511	1.035 ug/ml
18) N-TETRACONTANE	21.862	57855	0.663 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102920\
Data File : FF007795.D
Signal(s) : FID2B.ch
Acq On : 29 Oct 2020 12:50
Operator : DD\AJ
Sample : PB132701BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Oct 30 02:44:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
Quant Title :
QLast Update : Mon Oct 05 15:41:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

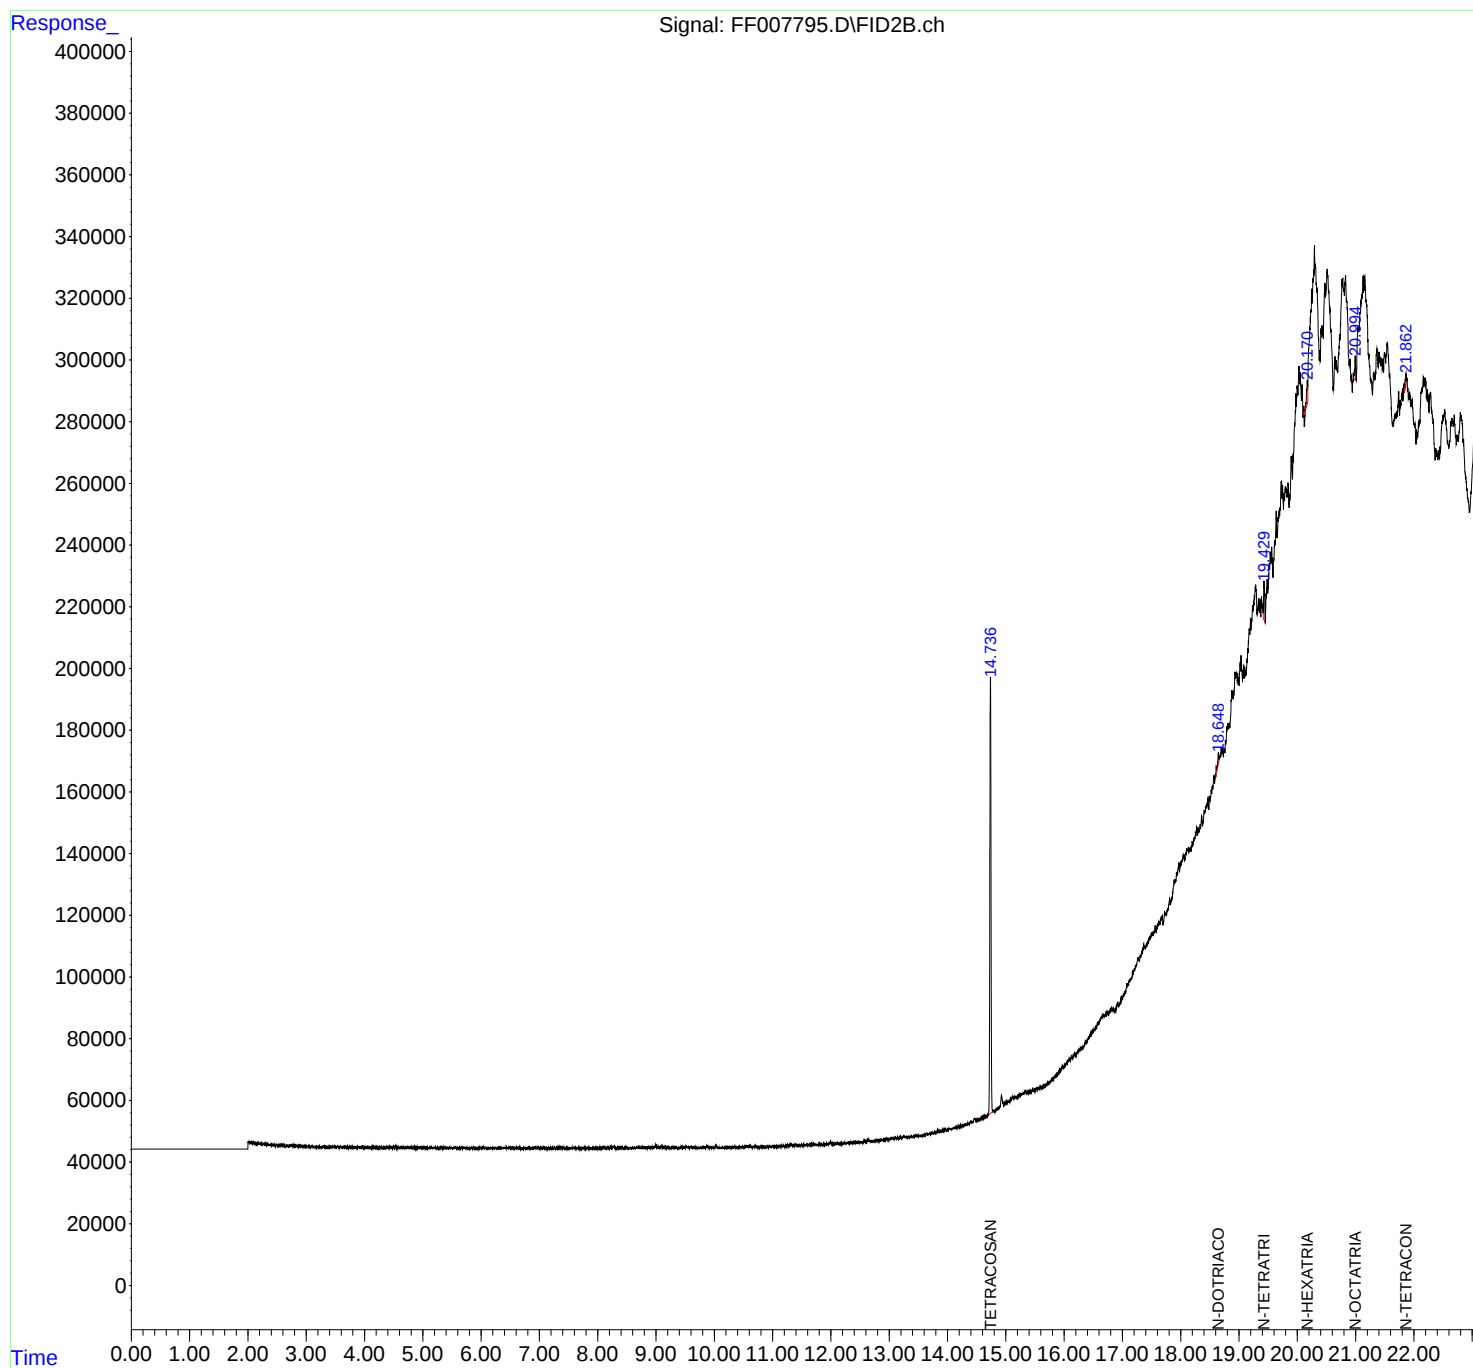


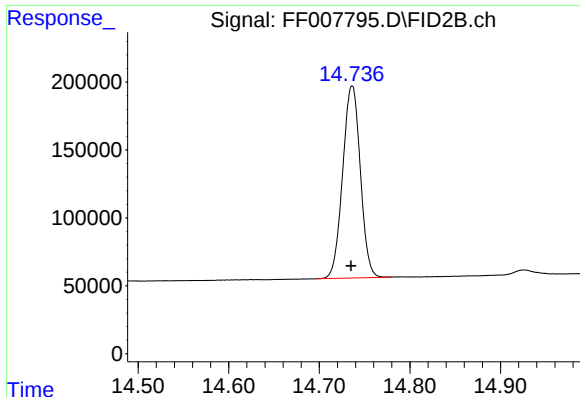

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.736 min
Delta R.T.: 0.001 min
Response: 1917931
Conc: 15.24 ug/ml

Instrument :
FID_F
ClientSampleId :

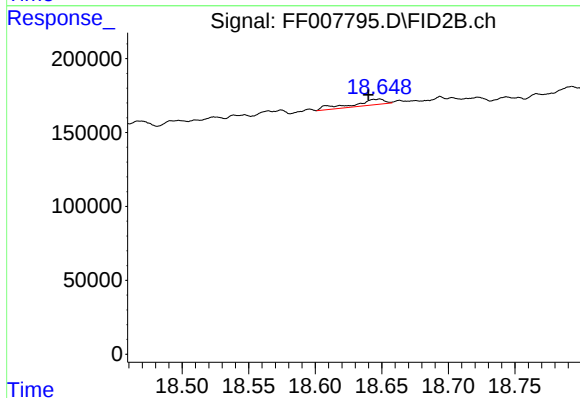


#14 N-DOTRIACONTANE

R.T.: 18.649 min
Delta R.T.: 0.009 min
Response: 65038
Conc: 0.54 ug/ml

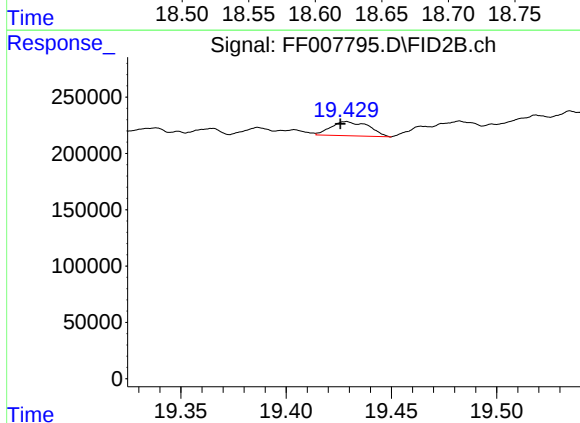


#15 N-TETRATRIACONTANE

R.T.: 19.429 min
Delta R.T.: 0.003 min
Response: 158281
Conc: 1.51 ug/ml

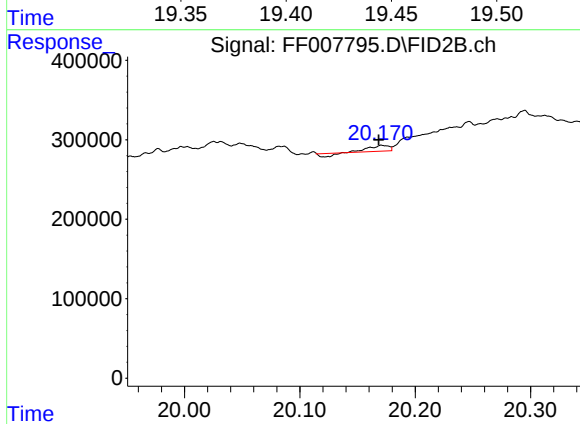

#16 N-HEXATRIACONTANE


R.T.: 20.171 min
Delta R.T.: 0.002 min
Response: 67007
Conc: 0.70 ug/ml

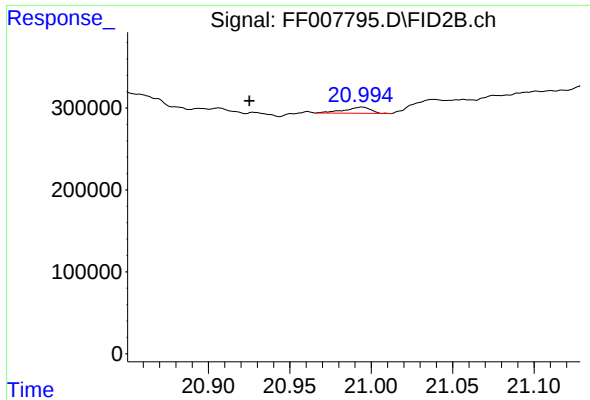

#17 N-OCTATRIACONTANE

R.T.: 20.994 min
Delta R.T.: 0.069 min
Response: 85511
Conc: 1.03 ug/ml

Instrument :
FID_F
ClientSampleId :

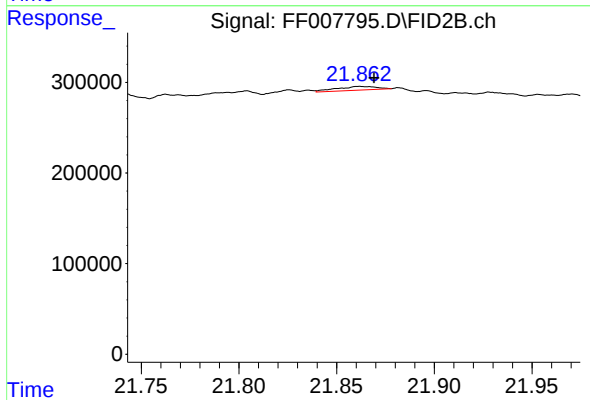

#18 N-TETRACONTANE

R.T.: 21.862 min
Delta R.T.: -0.008 min
Response: 57855
Conc: 0.66 ug/ml