

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102920\
 Data File : FF007799.D
 Signal(s) : FID2B.ch
 Acq On : 29 Oct 2020 14:54
 Operator : DD\AJ
 Sample : L4217-07 2X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 30 02:46:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
 Quant Title :
 QLast Update : Mon Oct 05 15:41:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.738	942370	7.488 ug/ml
Target Compounds			
1) N-OCTANE	2.336	65711	0.473 ug/ml
4) N-TETRADECANE	8.270	98521	0.676 ug/ml
8) N-DOCOSANE	13.836	63825	0.438 ug/ml
10) N-TETRACOSANE	14.938	204110	1.415 ug/ml
11) N-HEXACOSANE	15.968	121847	0.877 ug/ml
12) N-OCTACOSANE	16.923	330559	2.468 ug/ml
13) N-TRIACONTANE	17.813	548936	4.245 ug/ml
14) N-DOTRIACONTANE	18.648	576058	4.788 ug/ml
15) N-TETRATRIACONTANE	19.443	303222	2.886 ug/ml
16) N-HEXATRIACONTANE	20.180	321284	3.367 ug/ml
17) N-OCTATRIACONTANE	20.937	128349	1.553 ug/ml
18) N-TETRACONTANE	21.840	465304	5.331 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102920\
Data File : FF007799.D
Signal(s) : FID2B.ch
Acq On : 29 Oct 2020 14:54
Operator : DD\AJ
Sample : L4217-07 2X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 30 02:46:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
Quant Title :
QLast Update : Mon Oct 05 15:41:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

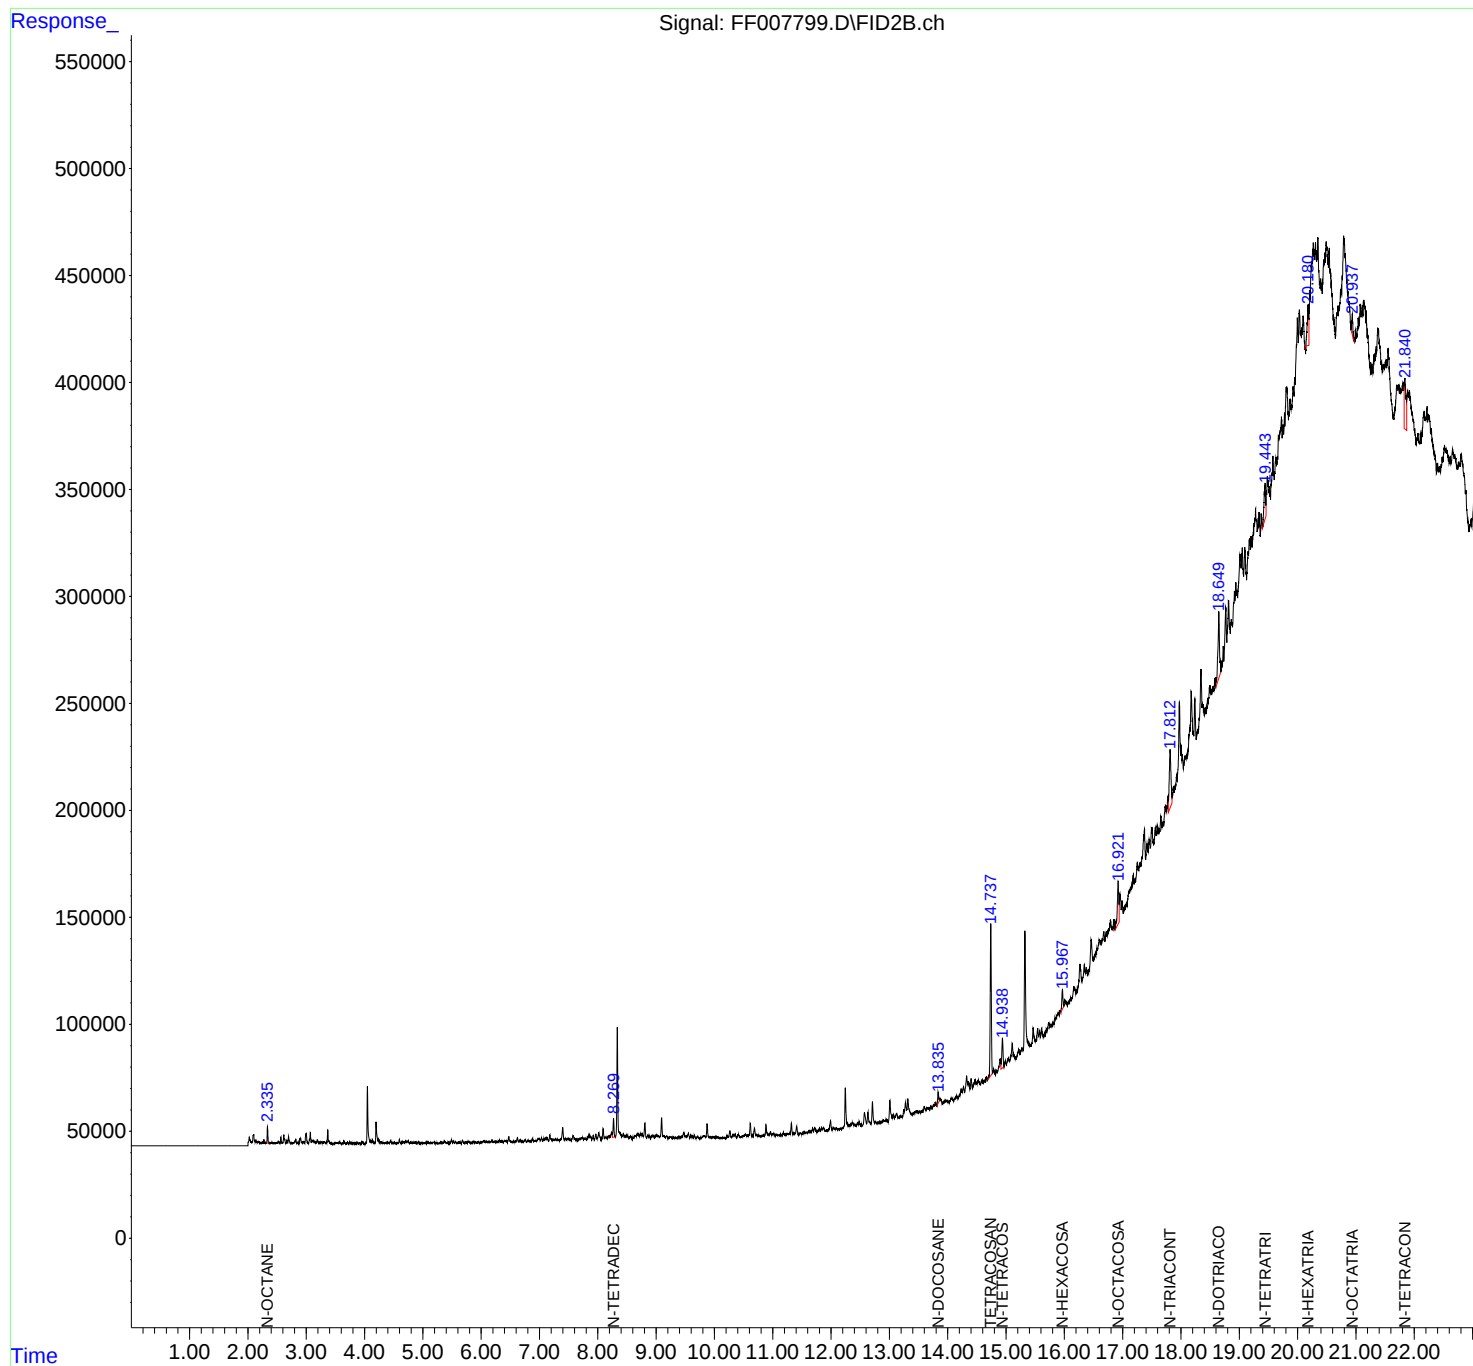


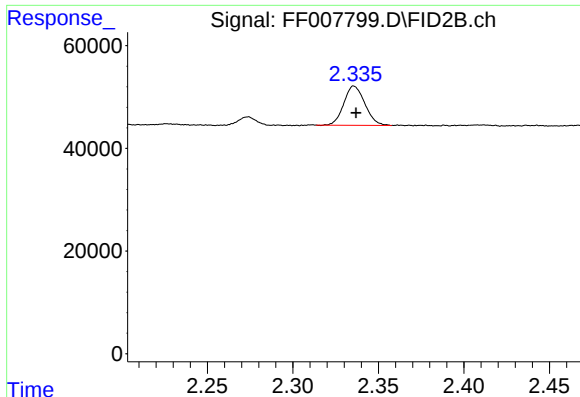

#1 N-OCTANE


R.T.: 2.336 min
Delta R.T.: -0.001 min
Response: 65711
Conc: 0.47 ug/ml

Instrument :
FID_F
ClientSampleId :

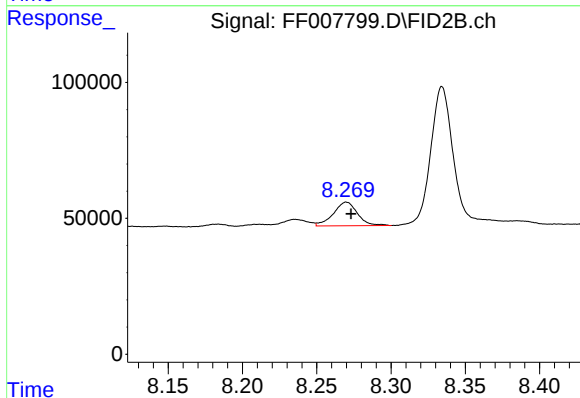


#4 N-TETRADECANE

R.T.: 8.270 min
Delta R.T.: -0.003 min
Response: 98521
Conc: 0.68 ug/ml

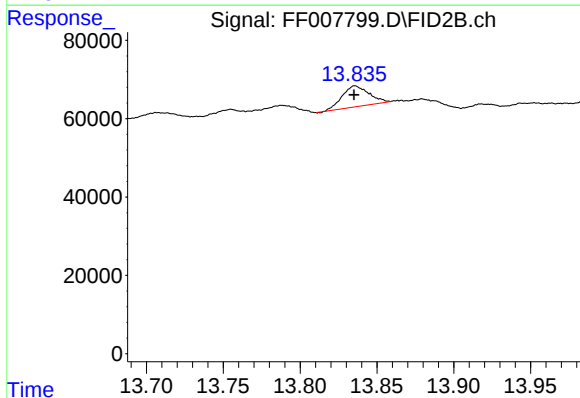


#8 N-DOCOSANE

R.T.: 13.836 min
Delta R.T.: 0.000 min
Response: 63825
Conc: 0.44 ug/ml

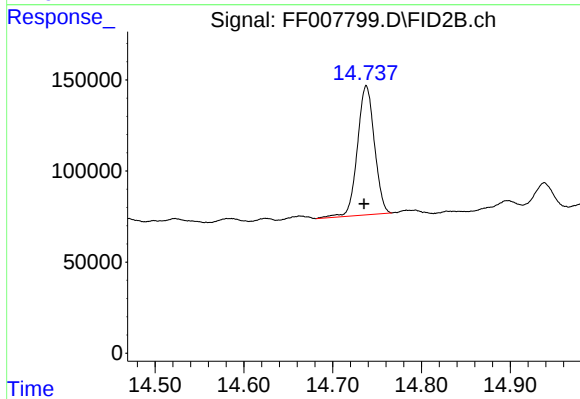

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.738 min
Delta R.T.: 0.003 min
Response: 942370
Conc: 7.49 ug/ml

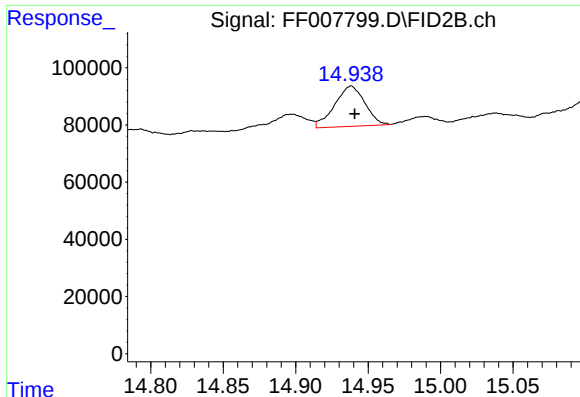

#10 N-TETRACOSANE


R.T.: 14.938 min
Delta R.T.: -0.002 min
Response: 204110
Conc: 1.41 ug/ml

Instrument :
FID_F
ClientSampleId :

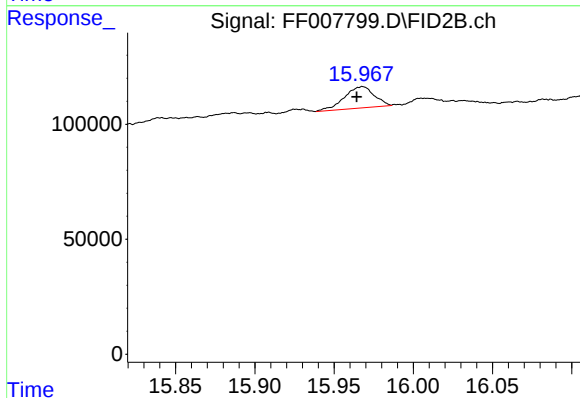


#11 N-HEXACOSANE

R.T.: 15.968 min
Delta R.T.: 0.004 min
Response: 121847
Conc: 0.88 ug/ml

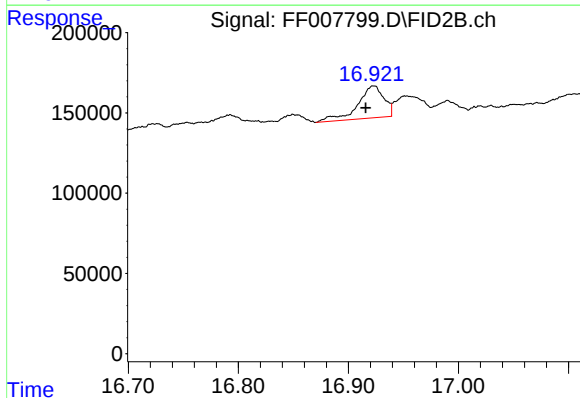


#12 N-OCTACOSANE

R.T.: 16.923 min
Delta R.T.: 0.007 min
Response: 330559
Conc: 2.47 ug/ml

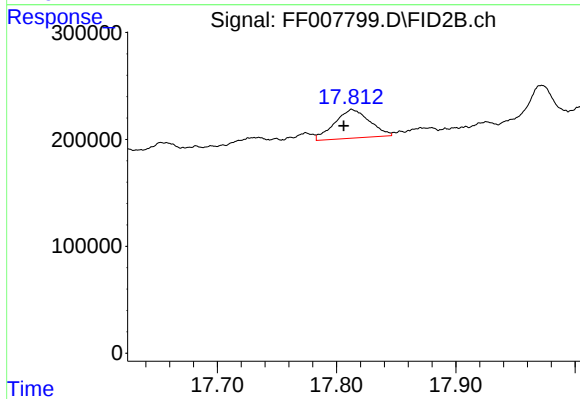

#13 N-TRIACONTANE


R.T.: 17.813 min
Delta R.T.: 0.007 min
Response: 548936
Conc: 4.25 ug/ml

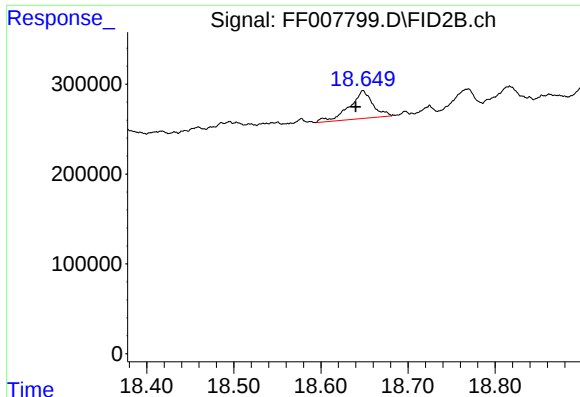

#14 N-DOTRIACONTANE


R.T.: 18.648 min
Delta R.T.: 0.009 min
Response: 576058
Conc: 4.79 ug/ml

Instrument :
FID_F
ClientSampleId :

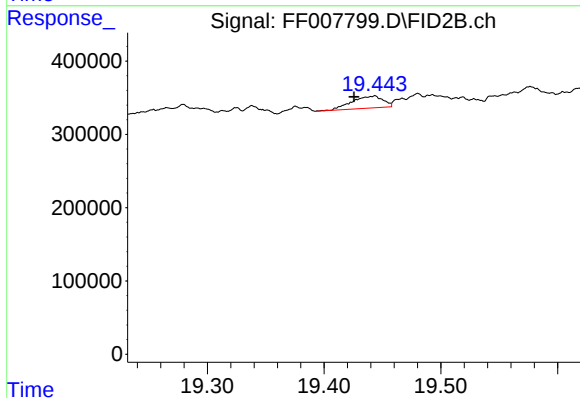


#15 N-TETRATRIACONTANE

R.T.: 19.443 min
Delta R.T.: 0.018 min
Response: 303222
Conc: 2.89 ug/ml

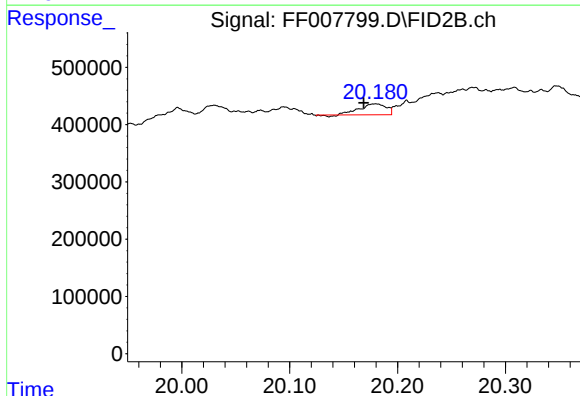


#16 N-HEXATRIACONTANE

R.T.: 20.180 min
Delta R.T.: 0.011 min
Response: 321284
Conc: 3.37 ug/ml

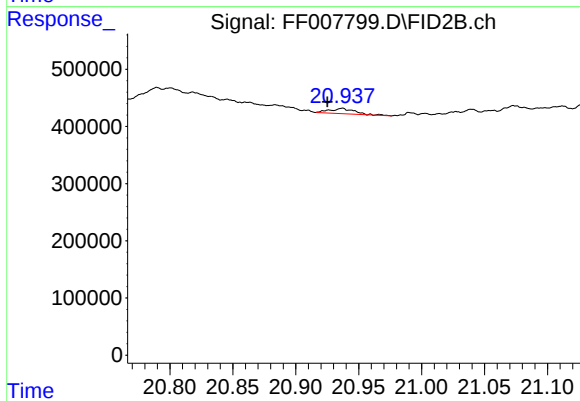

#17 N-OCTATRIACONTANE

R.T.: 20.937 min
Delta R.T.: 0.012 min
Response: 128349
Conc: 1.55 ug/ml

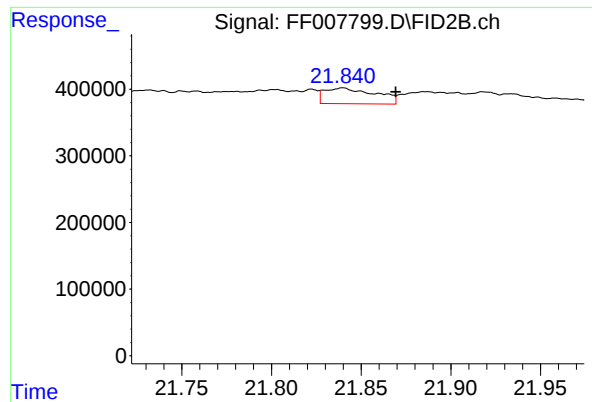

#18 N-TETRACONTANE

R.T.: 21.840 min
Delta R.T.: -0.029 min
Response: 465304
Conc: 5.33 ug/ml

Instrument :
FID_F
ClientSampleId :