

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102920\
 Data File : FF007800.D
 Signal(s) : FID2B.ch
 Acq On : 29 Oct 2020 15:25
 Operator : DD\AJ
 Sample : L4227-07 10X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Oct 30 02:46:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
 Quant Title :
 QLast Update : Mon Oct 05 15:41:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.737	137923	1.096 ug/ml
Target Compounds			
3) N-DODECANE	6.473	108333	0.750 ug/ml
4) N-TETRADECANE	8.270	111800	0.767 ug/ml
5) N-HEXADECANE	9.874	108312	0.724 ug/ml
6) N-OCTADECANE	11.319	85963	0.571 ug/ml
10) N-TETRACOSANE	14.935	152410	1.057 ug/ml
13) N-TRIACONTANE	17.810	94435	0.730 ug/ml
14) N-DOTRIACONTANE	18.644	207135	1.722 ug/ml
15) N-TETRATRIACONTANE	19.442	103087	0.981 ug/ml
16) N-HEXATRIACONTANE	20.217	579496	6.074 ug/ml
18) N-TETRACONTANE	21.868	640899	7.342 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102920\
Data File : FF007800.D
Signal(s) : FID2B.ch
Acq On : 29 Oct 2020 15:25
Operator : DD\AJ
Sample : L4227-07 10X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 30 02:46:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
Quant Title :
QLast Update : Mon Oct 05 15:41:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

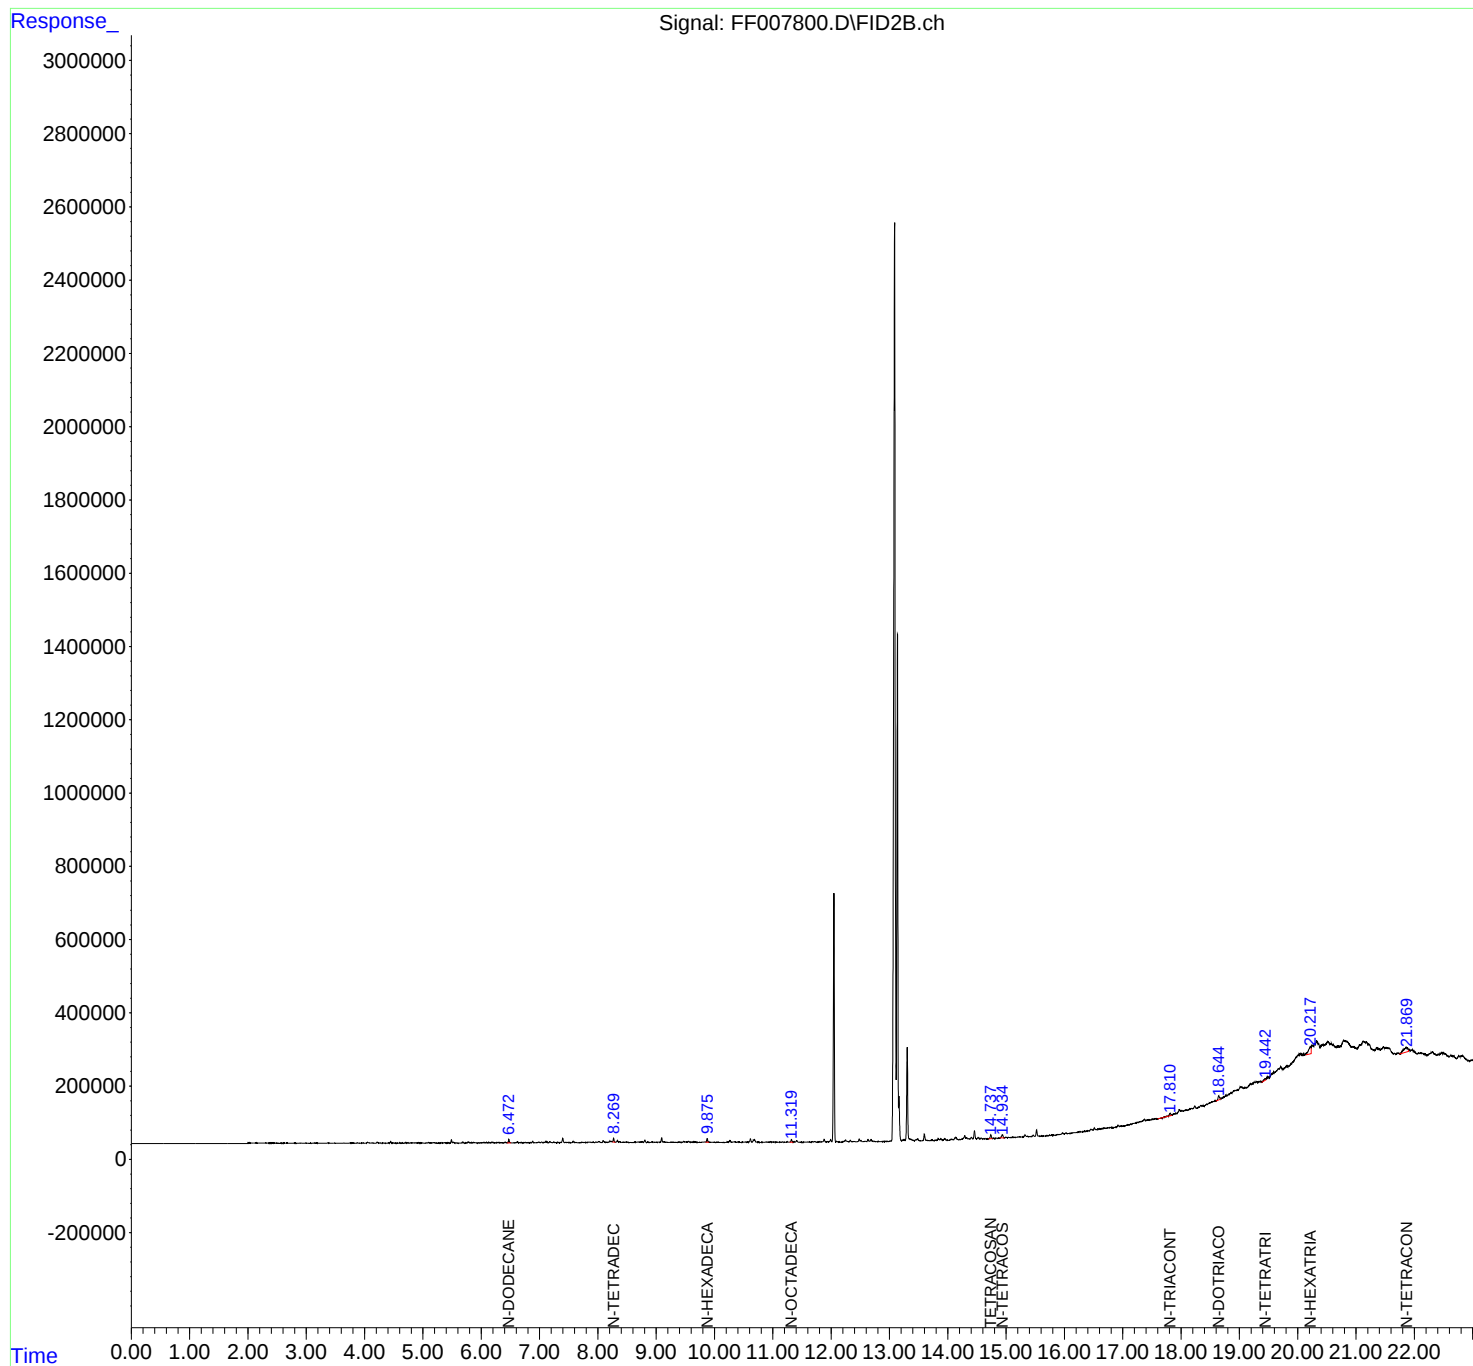


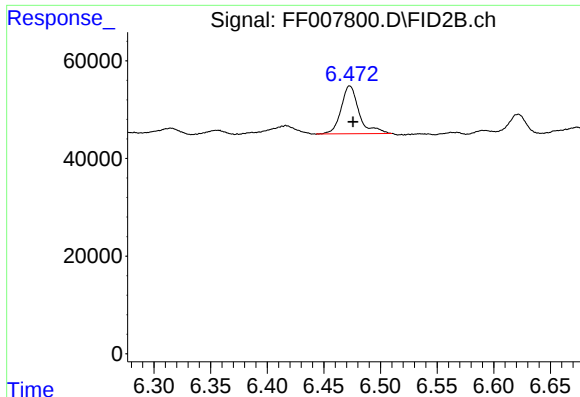

#3 N-DODECANE


R.T.: 6.473 min
Delta R.T.: -0.003 min
Response: 108333
Conc: 0.75 ug/ml

Instrument :
FID_F
ClientSampleId :

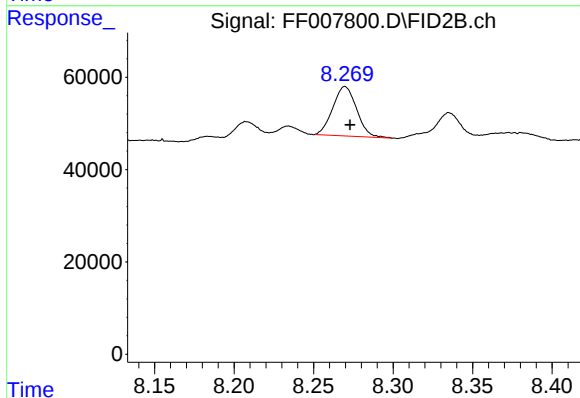


#4 N-TETRADECANE

R.T.: 8.270 min
Delta R.T.: -0.003 min
Response: 111800
Conc: 0.77 ug/ml

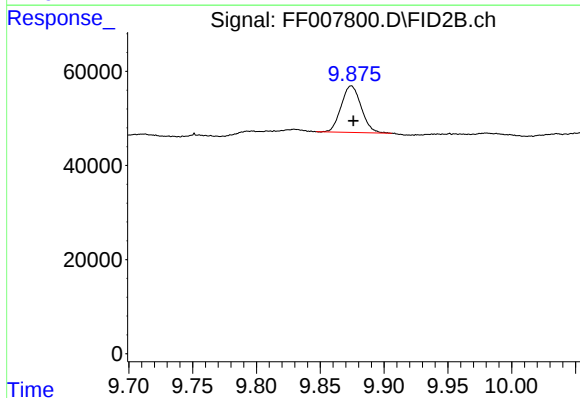


#5 N-HEXADECANE

R.T.: 9.874 min
Delta R.T.: -0.002 min
Response: 108312
Conc: 0.72 ug/ml

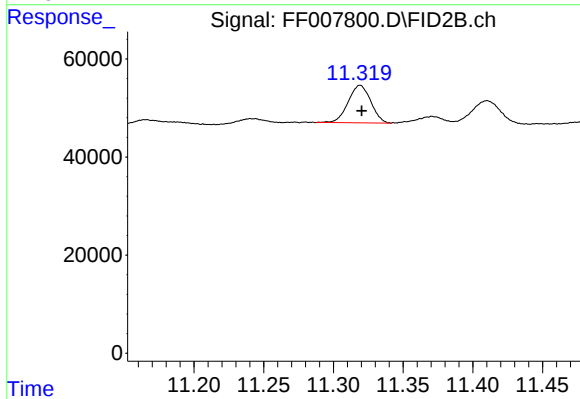

#6 N-OCTADECANE


R.T.: 11.319 min
Delta R.T.: -0.001 min
Response: 85963
Conc: 0.57 ug/ml

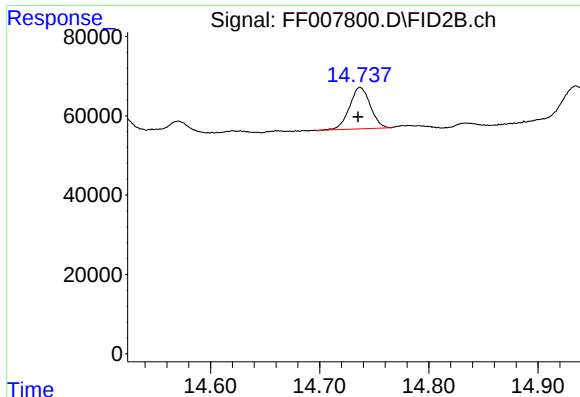

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.737 min
Delta R.T.: 0.002 min
Response: 137923
Conc: 1.10 ug/ml

Instrument :
FID_F
ClientSampleId :

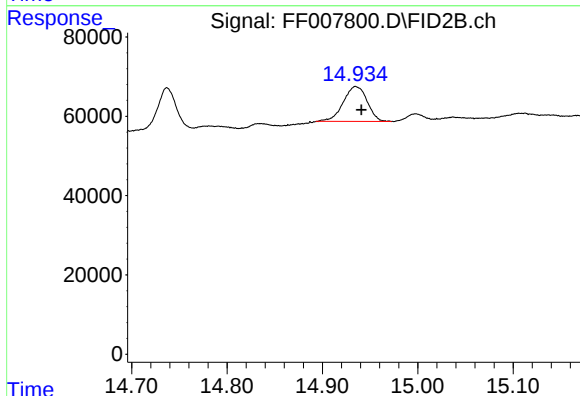


#10 N-TETRACOSANE

R.T.: 14.935 min
Delta R.T.: -0.006 min
Response: 152410
Conc: 1.06 ug/ml

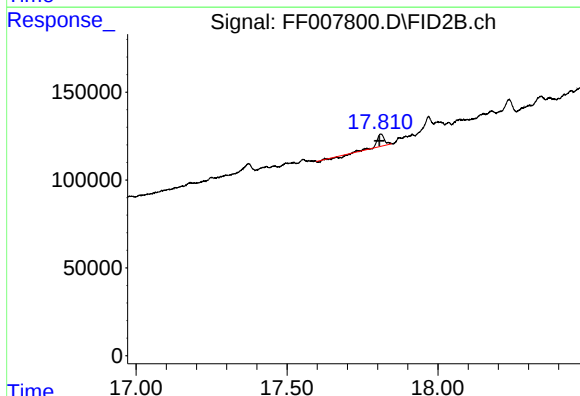


#13 N-TRIACONTANE

R.T.: 17.810 min
Delta R.T.: 0.004 min
Response: 94435
Conc: 0.73 ug/ml

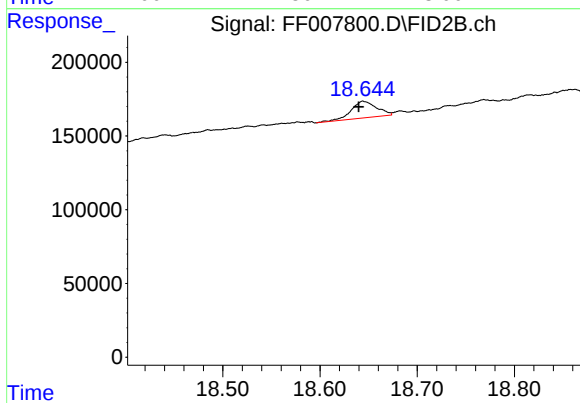

#14 N-DOTRIACONTANE

R.T.: 18.644 min
Delta R.T.: 0.005 min
Response: 207135
Conc: 1.72 ug/ml

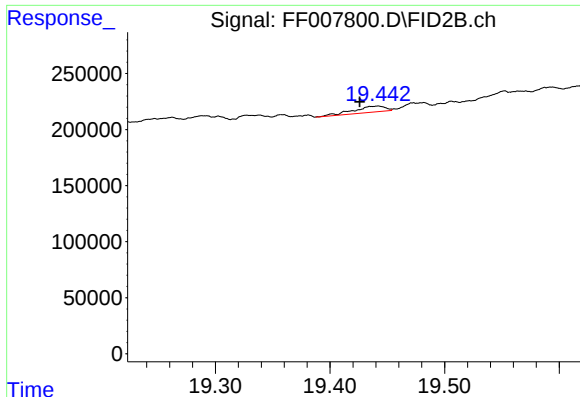

#15 N-TETRATRIACONTANE


R.T.: 19.442 min

Delta R.T.: 0.016 min

Response: 103087

Conc: 0.98 ug/ml

Instrument :
FID_F
ClientSampleId :

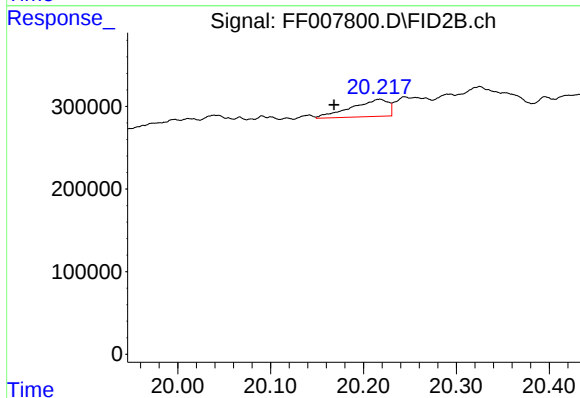


#16 N-HEXATRIACONTANE

R.T.: 20.217 min

Delta R.T.: 0.049 min

Response: 579496

Conc: 6.07 ug/ml

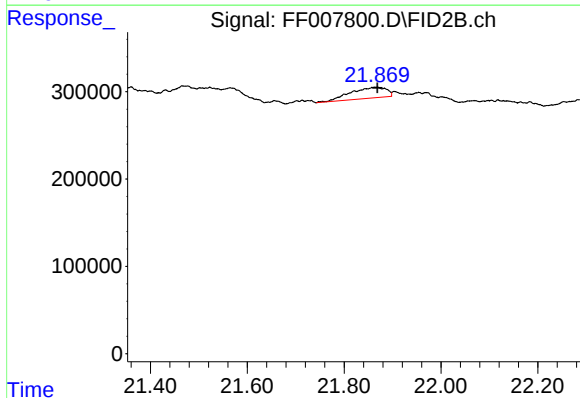

#18 N-TETRACONTANE

R.T.: 21.868 min

Delta R.T.: 0.000 min

Response: 640899

Conc: 7.34 ug/ml