

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF102920\  
 Data File : FF007805.D  
 Signal(s) : FID2B.ch  
 Acq On : 29 Oct 2020 18:49  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 52 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Oct 30 02:47:34 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF100220.M  
 Quant Title :  
 QLast Update : Mon Oct 05 15:41:23 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.739 | 1962487  | 15.594 ug/ml |
| Target Compounds              |        |          |              |
| 14) N-DOTRIACONTANE           | 18.645 | 48864    | 0.406 ug/ml  |
| 16) N-HEXATRIACONTANE         | 20.206 | 477681   | 5.007 ug/ml  |
| 18) N-TETRACONTANE            | 21.872 | 236471   | 2.709 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF102920\  
Data File : FF007805.D  
Signal(s) : FID2B.ch  
Acq On : 29 Oct 2020 18:49  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampled :

Integration File: autoint1.e  
Quant Time: Oct 30 02:47:34 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF100220.M  
Quant Title :  
QLast Update : Mon Oct 05 15:41:23 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

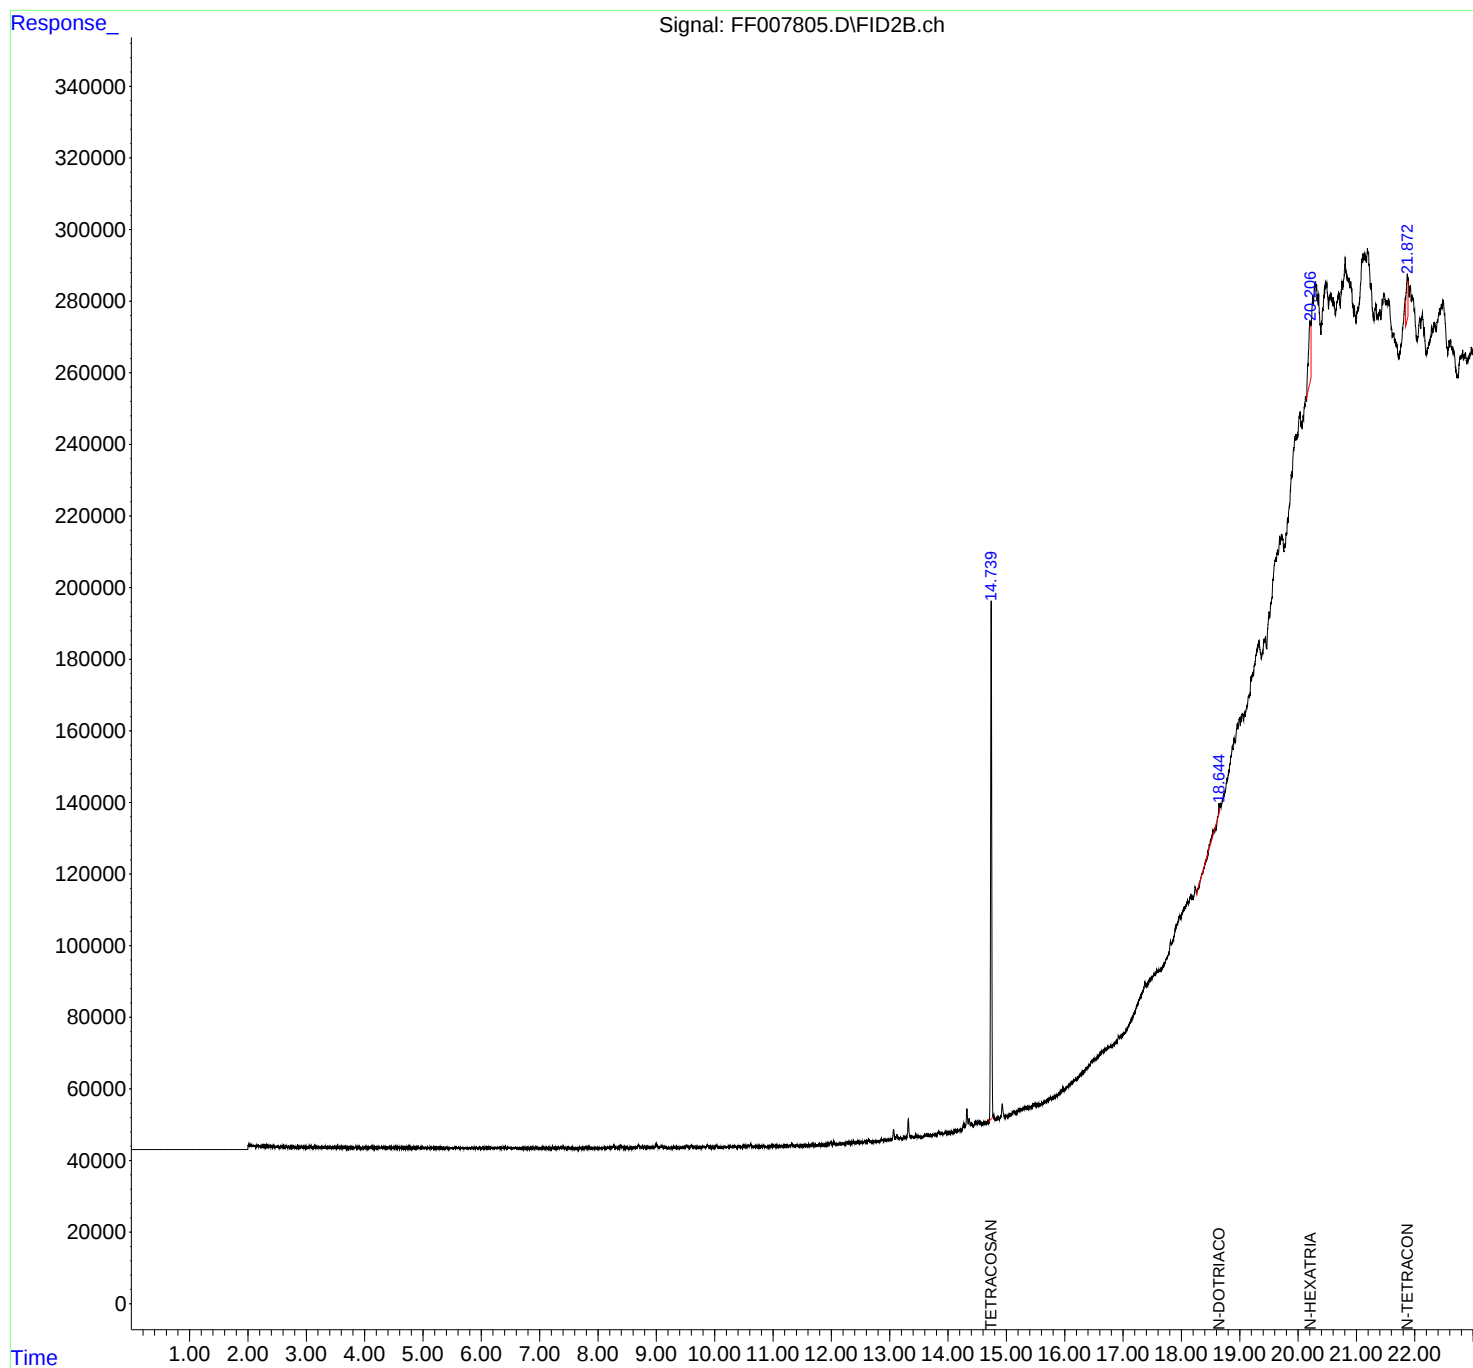


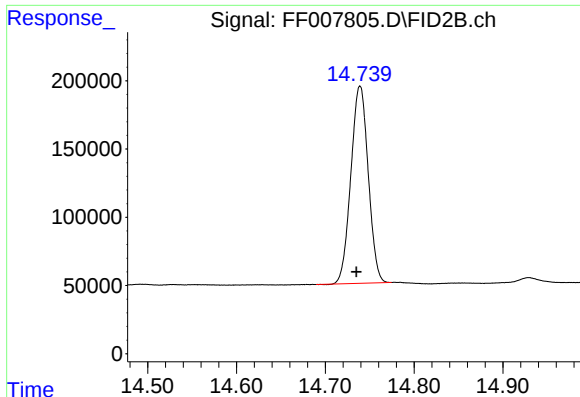

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.739 min  
Delta R.T.: 0.004 min  
Response: 1962487  
Conc: 15.59 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

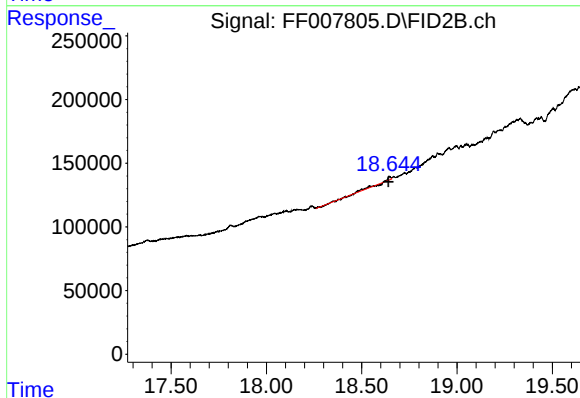


#14 N-DOTRIACONTANE

R.T.: 18.645 min  
Delta R.T.: 0.006 min  
Response: 48864  
Conc: 0.41 ug/ml

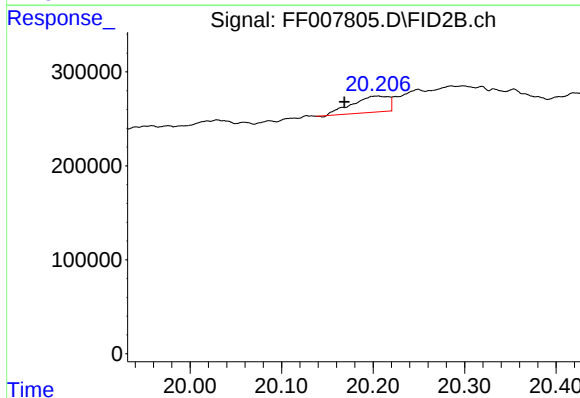

#16 N-HEXATRIACONTANE

R.T.: 20.206 min  
Delta R.T.: 0.037 min  
Response: 477681  
Conc: 5.01 ug/ml

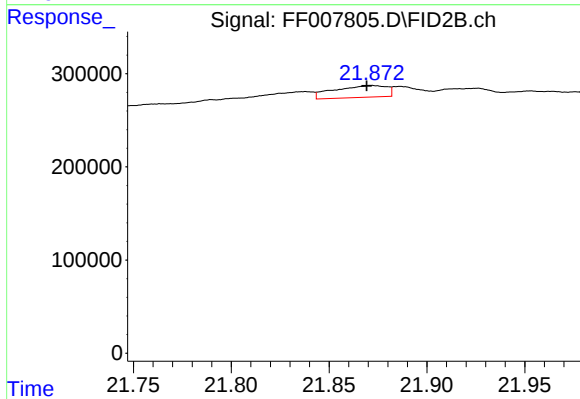

#18 N-TETRACONTANE

R.T.: 21.872 min  
Delta R.T.: 0.003 min  
Response: 236471  
Conc: 2.71 ug/ml