

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102920\
 Data File : FF007794.D
 Signal(s) : FID2B.ch
 Acq On : 29 Oct 2020 12:19
 Operator : DD\AJ
 Sample : L4219-17MSD 2X
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CL-01-102320MSD

Integration File: autoint1.e
 Quant Time: Oct 30 02:44:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
 Quant Title :
 QLast Update : Mon Oct 05 15:41:23 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.735	1035765	8.230 ug/ml
Target Compounds			
2) N-DECANE	4.445	1247242	8.793 ug/ml
3) N-DODECANE	6.471	1285128	8.894 ug/ml
4) N-TETRADECANE	8.269	1418695	9.731 ug/ml
5) N-HEXADECANE	9.872	1156386	7.735 ug/ml
6) N-OCTADECANE	11.317	1151137	7.641 ug/ml
7) N-EICOSANE	12.630	1240292	8.343 ug/ml
8) N-DOCOSANE	13.832	1178612	8.080 ug/ml
10) N-TETRACOSANE	14.939	1379210	9.561 ug/ml
11) N-HEXACOSANE	15.966	1210632	8.715 ug/ml
12) N-OCTACOSANE	16.922	1324135	9.886 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102920\
Data File : FF007794.D
Signal(s) : FID2B.ch
Acq On : 29 Oct 2020 12:19
Operator : DD\AJ
Sample : L4219-17MSD 2X
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CL-01-102320MSD

Integration File: autoint1.e
Quant Time: Oct 30 02:44:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100220.M
Quant Title :
QLast Update : Mon Oct 05 15:41:23 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

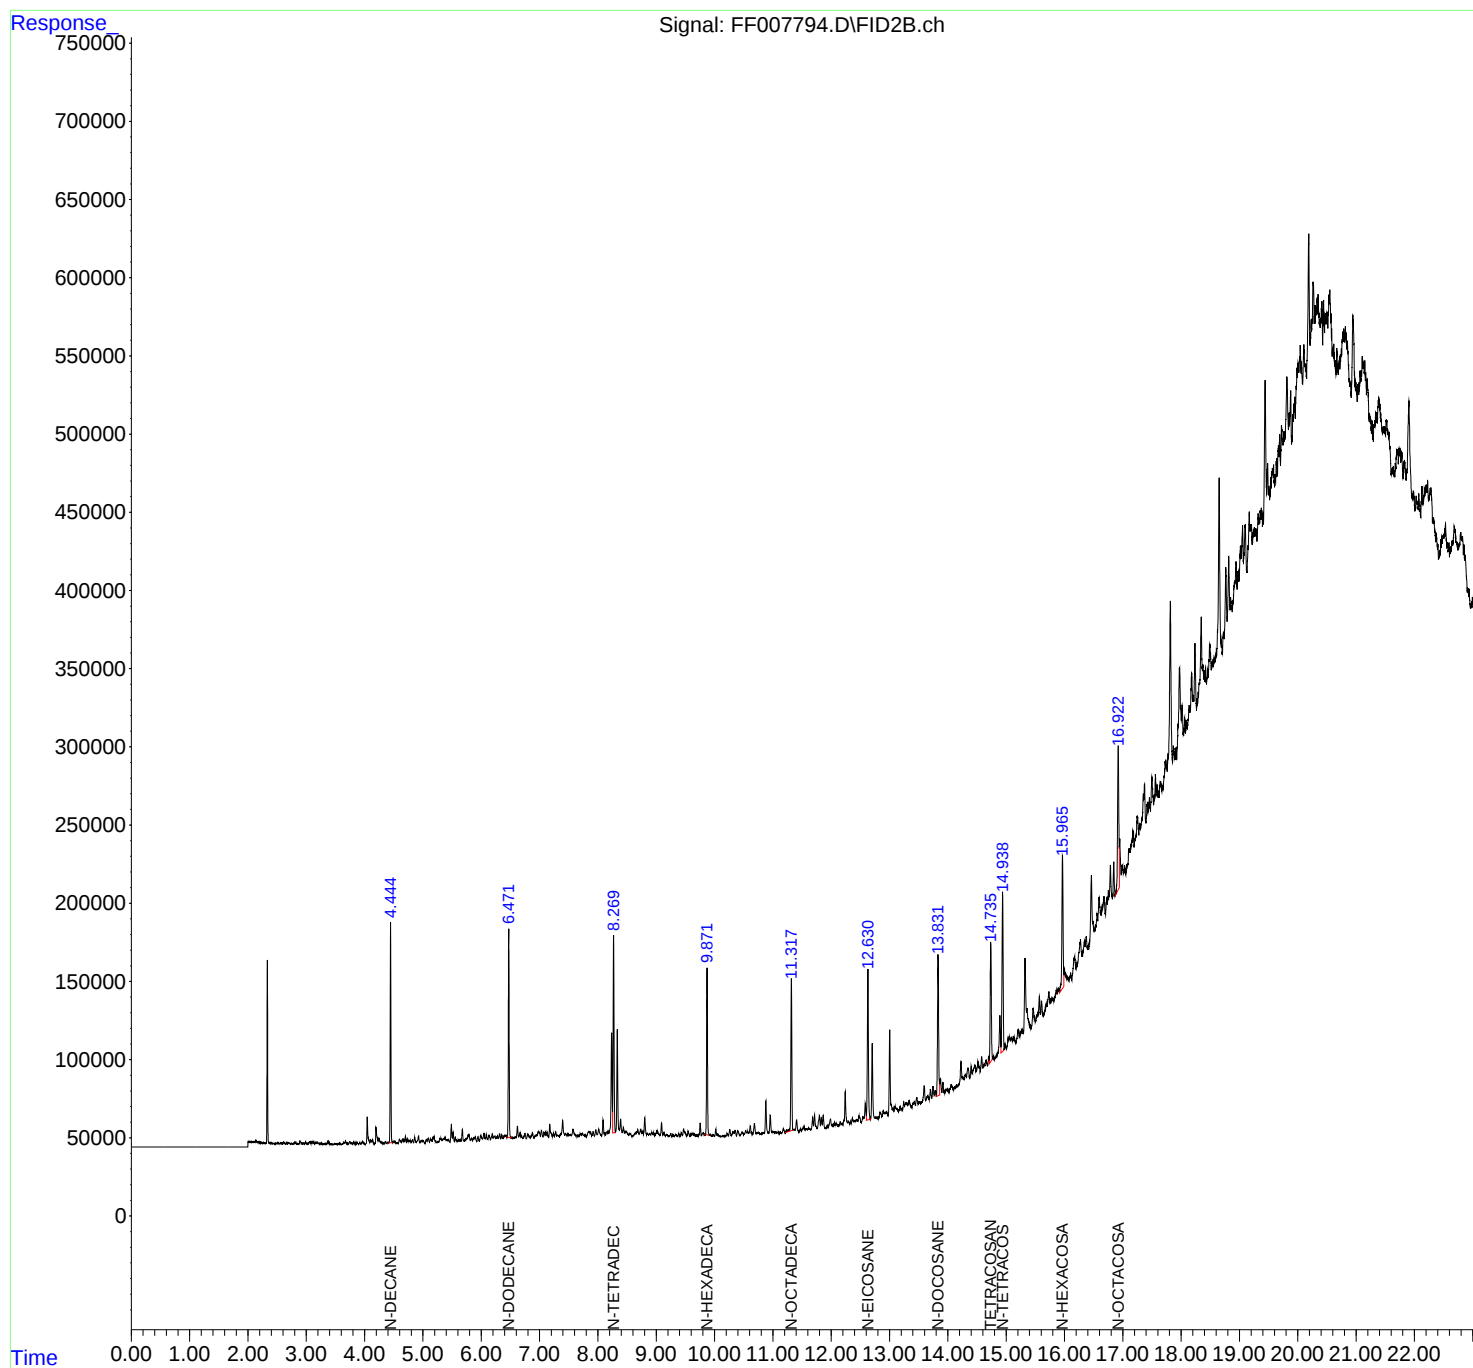


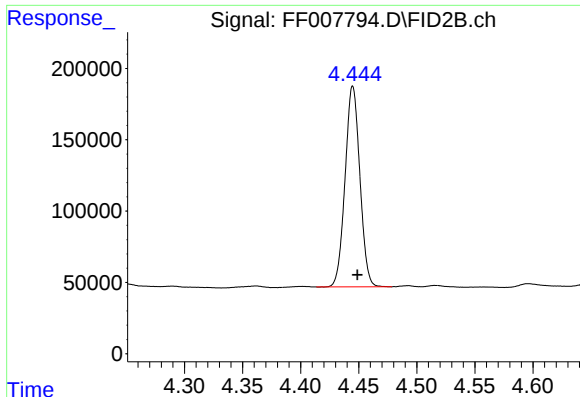

#2 N-DECANE


R.T.: 4.445 min
Delta R.T.: -0.004 min
Response: 1247242
Conc: 8.79 ug/ml

Instrument :
FID_F
ClientSampleId :
CL-01-102320MSD

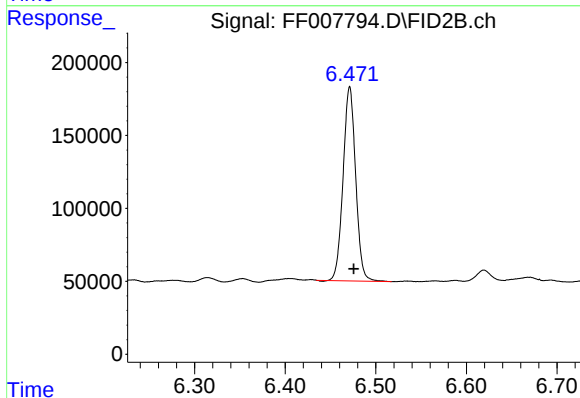


#3 N-DODECANE

R.T.: 6.471 min
Delta R.T.: -0.004 min
Response: 1285128
Conc: 8.89 ug/ml

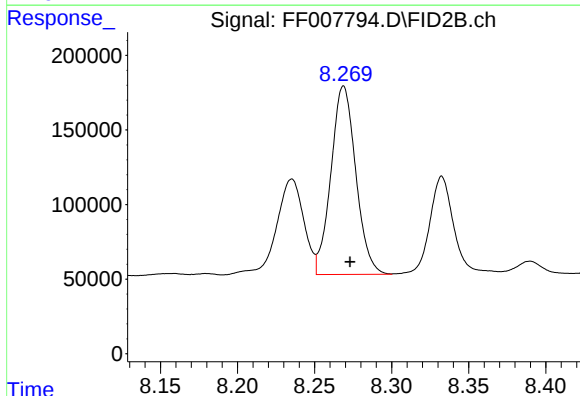


#4 N-TETRADECANE

R.T.: 8.269 min
Delta R.T.: -0.004 min
Response: 1418695
Conc: 9.73 ug/ml

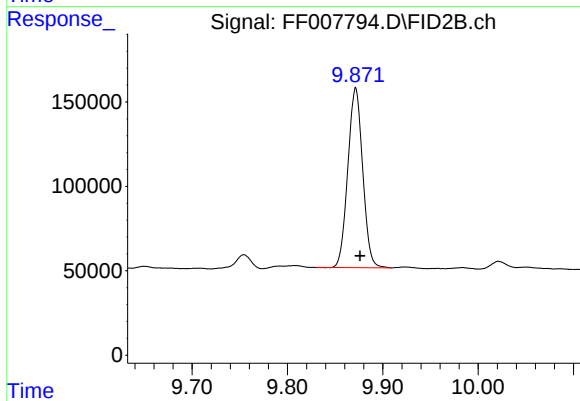

#5 N-HEXADECANE


R.T.: 9.872 min
Delta R.T.: -0.004 min
Response: 1156386
Conc: 7.73 ug/ml

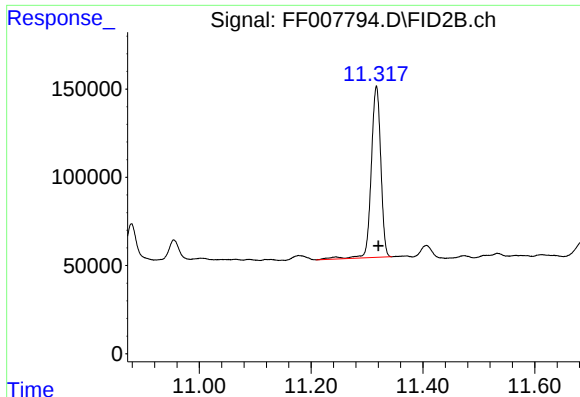

#6 N-OCTADECANE


R.T.: 11.317 min
Delta R.T.: -0.003 min
Response: 1151137
Conc: 7.64 ug/ml

Instrument :
FID_F
ClientSampleId :
CL-01-102320MSD

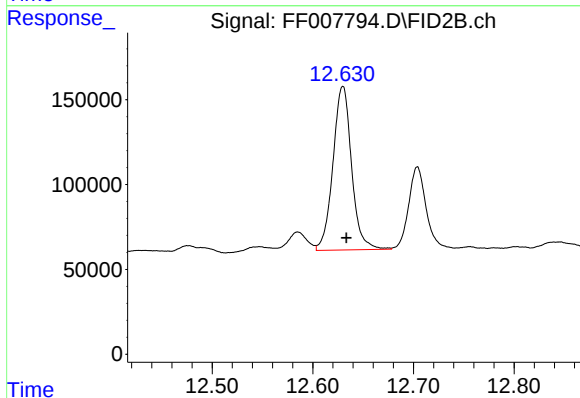


#7 N-EICOSANE

R.T.: 12.630 min
Delta R.T.: -0.003 min
Response: 1240292
Conc: 8.34 ug/ml

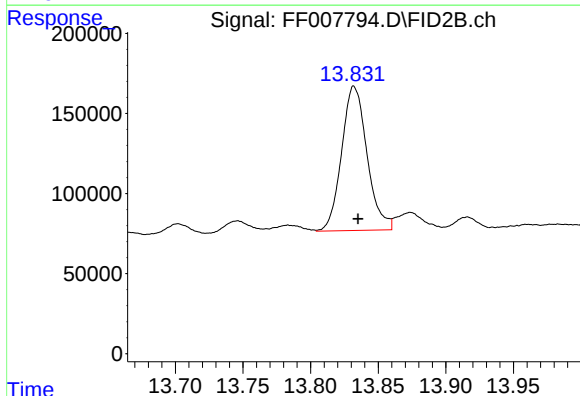


#8 N-DOCOSANE

R.T.: 13.832 min
Delta R.T.: -0.003 min
Response: 1178612
Conc: 8.08 ug/ml

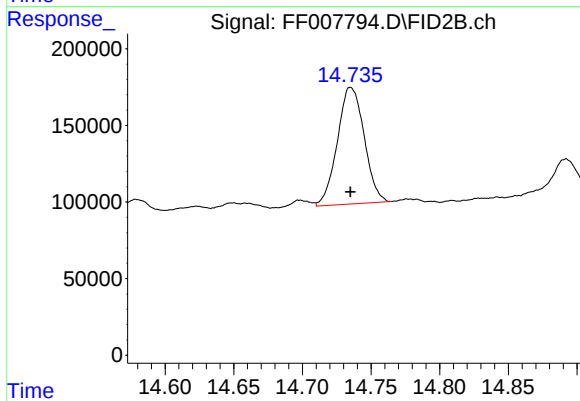

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.735 min
Delta R.T.: 0.000 min
Response: 1035765
Conc: 8.23 ug/ml

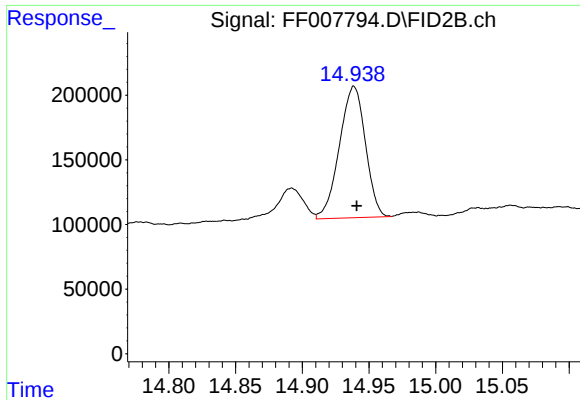

#10 N-TETRACOSANE


R.T.: 14.939 min
Delta R.T.: -0.002 min
Response: 1379210
Conc: 9.56 ug/ml

Instrument :
FID_F
ClientSampleId :
CL-01-102320MSD

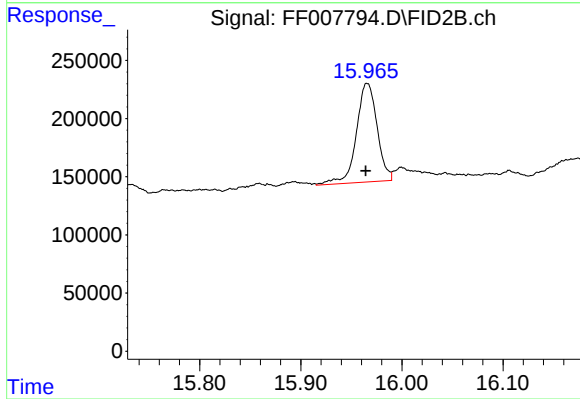

#11 N-HEXACOSANE

R.T.: 15.966 min
Delta R.T.: 0.002 min
Response: 1210632
Conc: 8.71 ug/ml

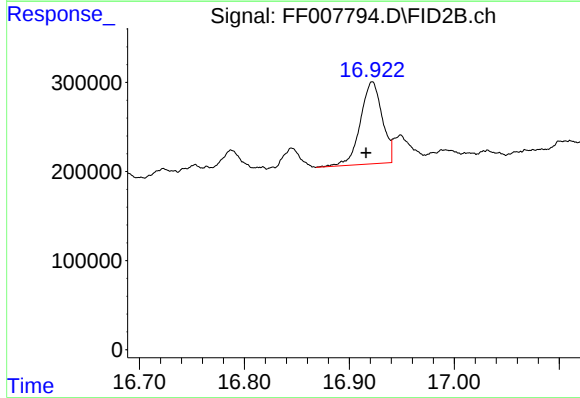

#12 N-OCTACOSANE

R.T.: 16.922 min
Delta R.T.: 0.006 min
Response: 1324135
Conc: 9.89 ug/ml