

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102921\
Data File : FF009216.D
Signal(s) : FID2B.ch
Acq On : 29 Oct 2021 14:03
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 29 23:01:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.481	3425673	26.965 ug/ml
12)	N-OCTACOSANE	16.880	3243637	27.708 ug/ml
13)	N-TRIACONTANE	17.764	168662	1.495 ug/ml
14)	N-DOTRIACONTANE	18.594	220985	2.093 ug/ml
15)	N-TETRATRIACONTANE	19.375	179458	1.836 ug/ml
16)	N-HEXATRIACONTANE	20.112	134974	1.518 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102921\
Data File : FF009216.D
Signal(s) : FID2B.ch
Acq On : 29 Oct 2021 14:03
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 29 23:01:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

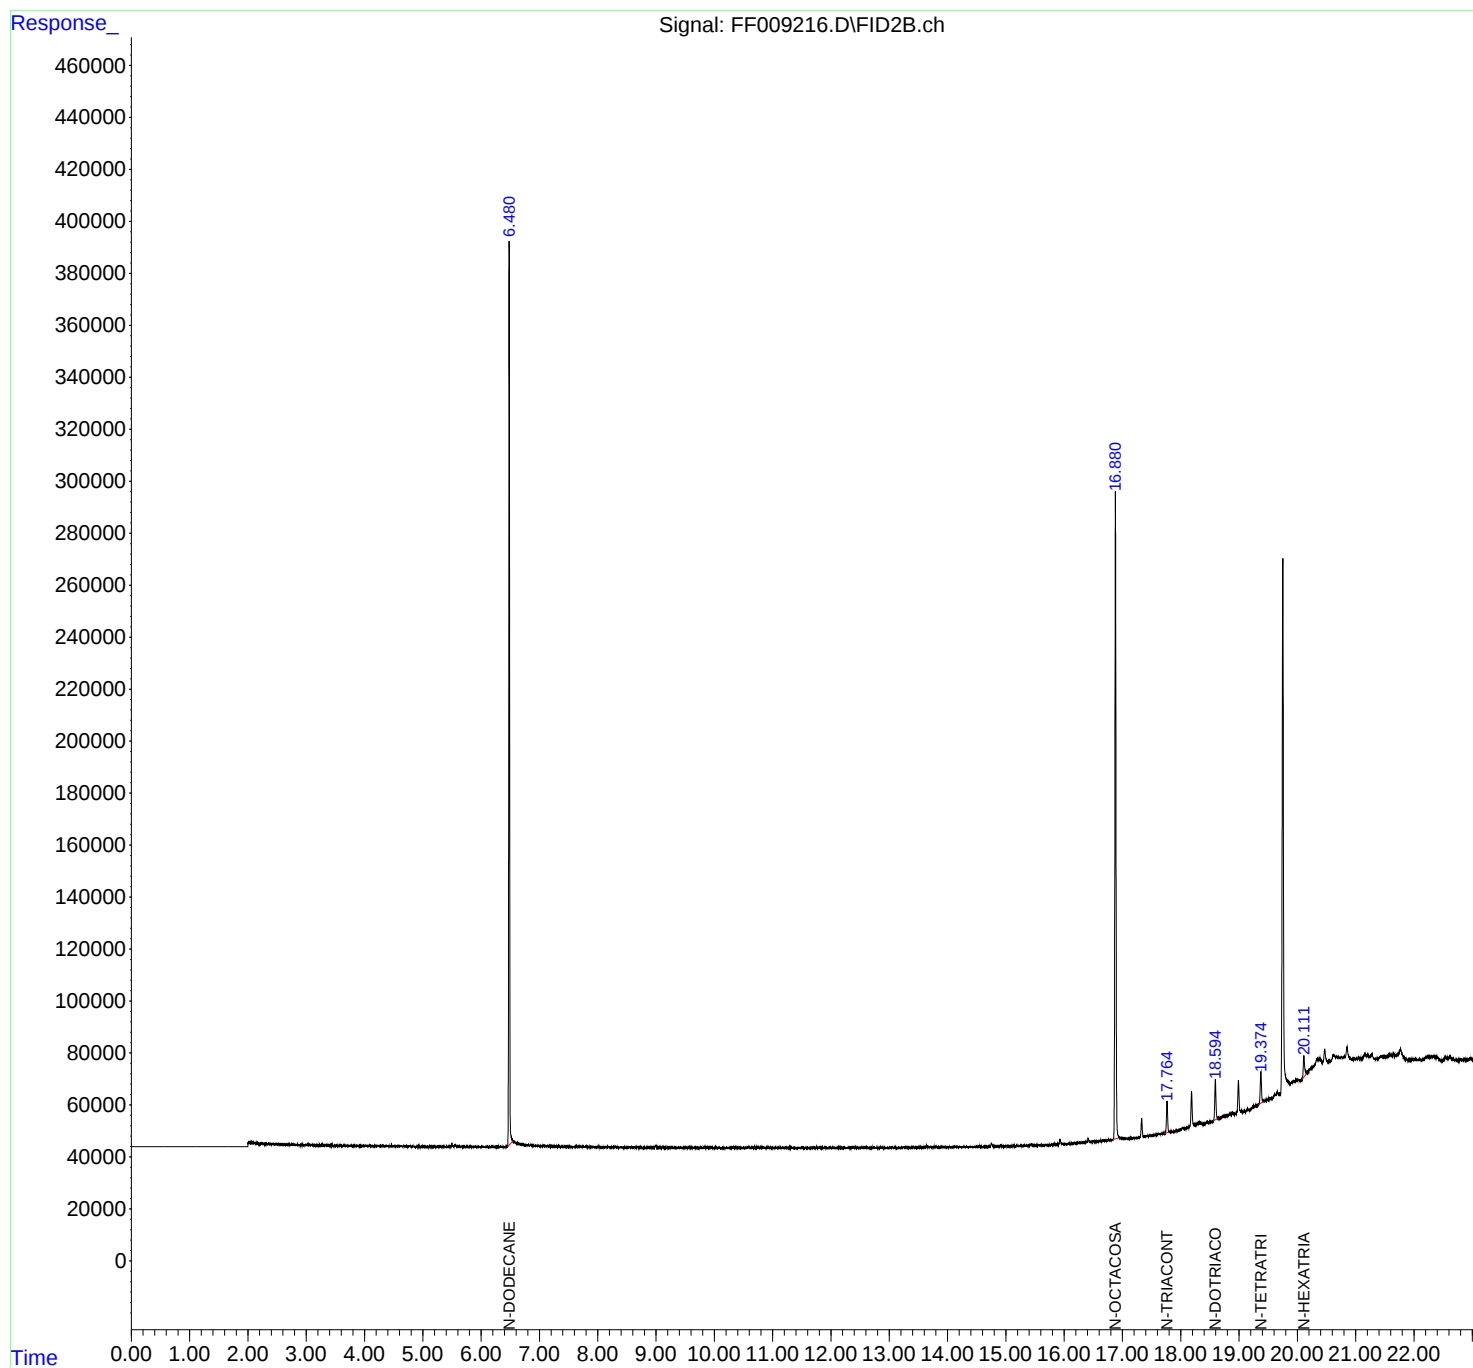


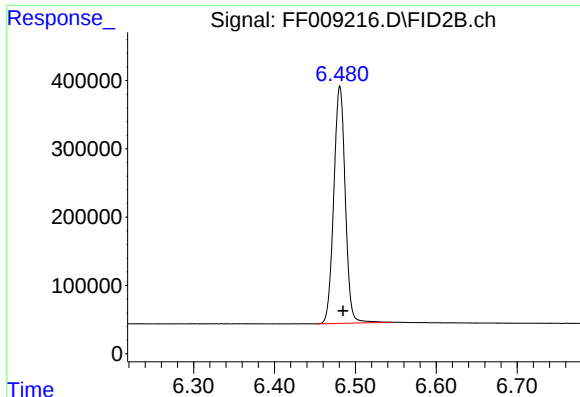

#3 N-DODECANE


R.T.: 6.481 min
Delta R.T.: -0.004 min
Response: 3425673
Conc: 26.97 ug/ml

Instrument :
FID_F
ClientSampleId :

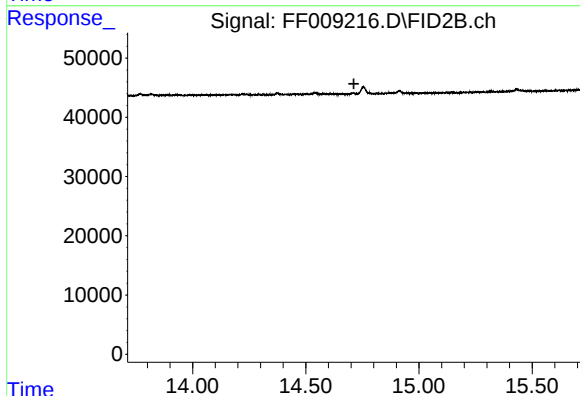


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.712 min
Response: 0
Conc: N.D.

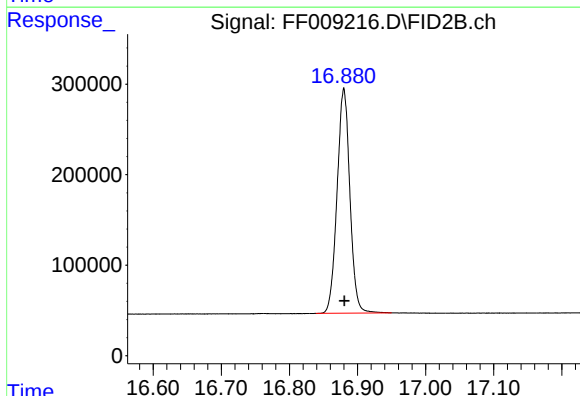


#12 N-OCTACOSANE

R.T.: 16.880 min
Delta R.T.: 0.000 min
Response: 3243637
Conc: 27.71 ug/ml

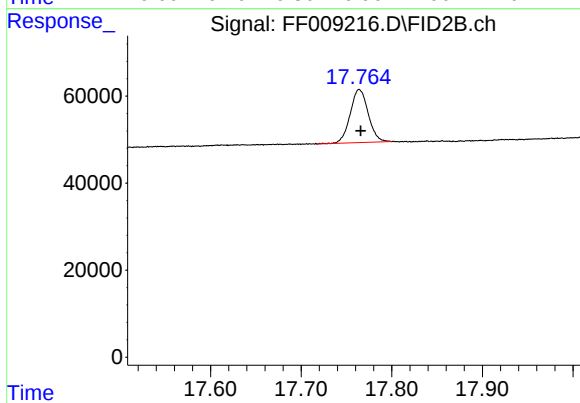

#13 N-TRIACONTANE


R.T.: 17.764 min
Delta R.T.: -0.002 min
Response: 168662
Conc: 1.49 ug/ml

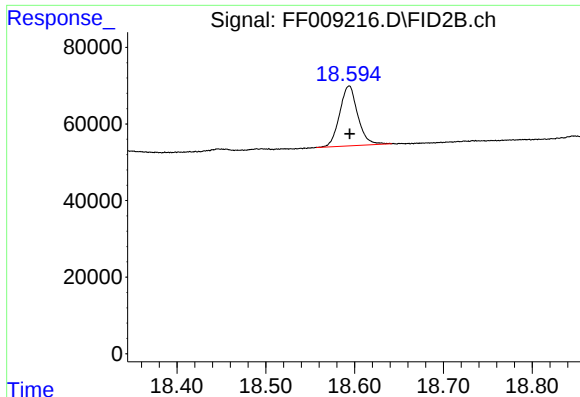

#14 N-DOTRIACONTANE


R.T.: 18.594 min
Delta R.T.: 0.000 min
Response: 220985
Conc: 2.09 ug/ml

Instrument :
FID_F
ClientSampleId :

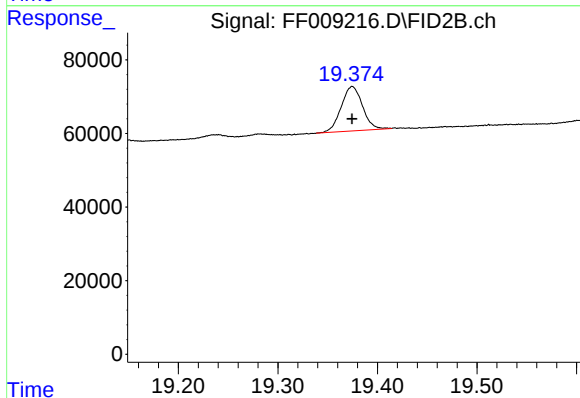

#15 N-TETRATRIACONTANE

R.T.: 19.375 min
Delta R.T.: 0.000 min
Response: 179458
Conc: 1.84 ug/ml

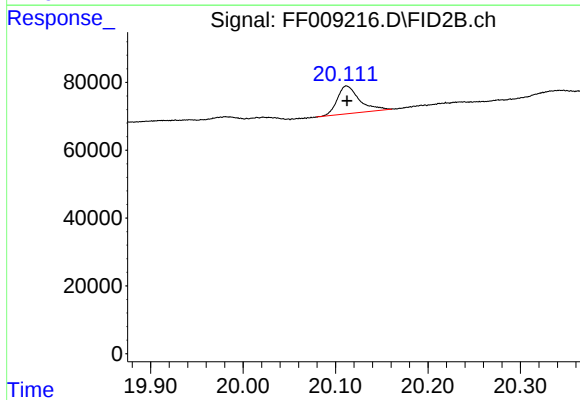

#16 N-HEXATRIACONTANE

R.T.: 20.112 min
Delta R.T.: 0.000 min
Response: 134974
Conc: 1.52 ug/ml