

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102921\
Data File : FF009223.D
Signal(s) : FID2B.ch
Acq On : 29 Oct 2021 18:38
Operator : AJ\MA
Sample : M4407-01 5X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 29 23:03:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.711	377356	3.441 ug/ml
Target Compounds			
15) N-TETRATRIACONTANE	19.380	47817	0.489 ug/ml
16) N-HEXATRIACONTANE	20.130	51360	0.578 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102921\
Data File : FF009223.D
Signal(s) : FID2B.ch
Acq On : 29 Oct 2021 18:38
Operator : AJ\MA
Sample : M4407-01 5X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Oct 29 23:03:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

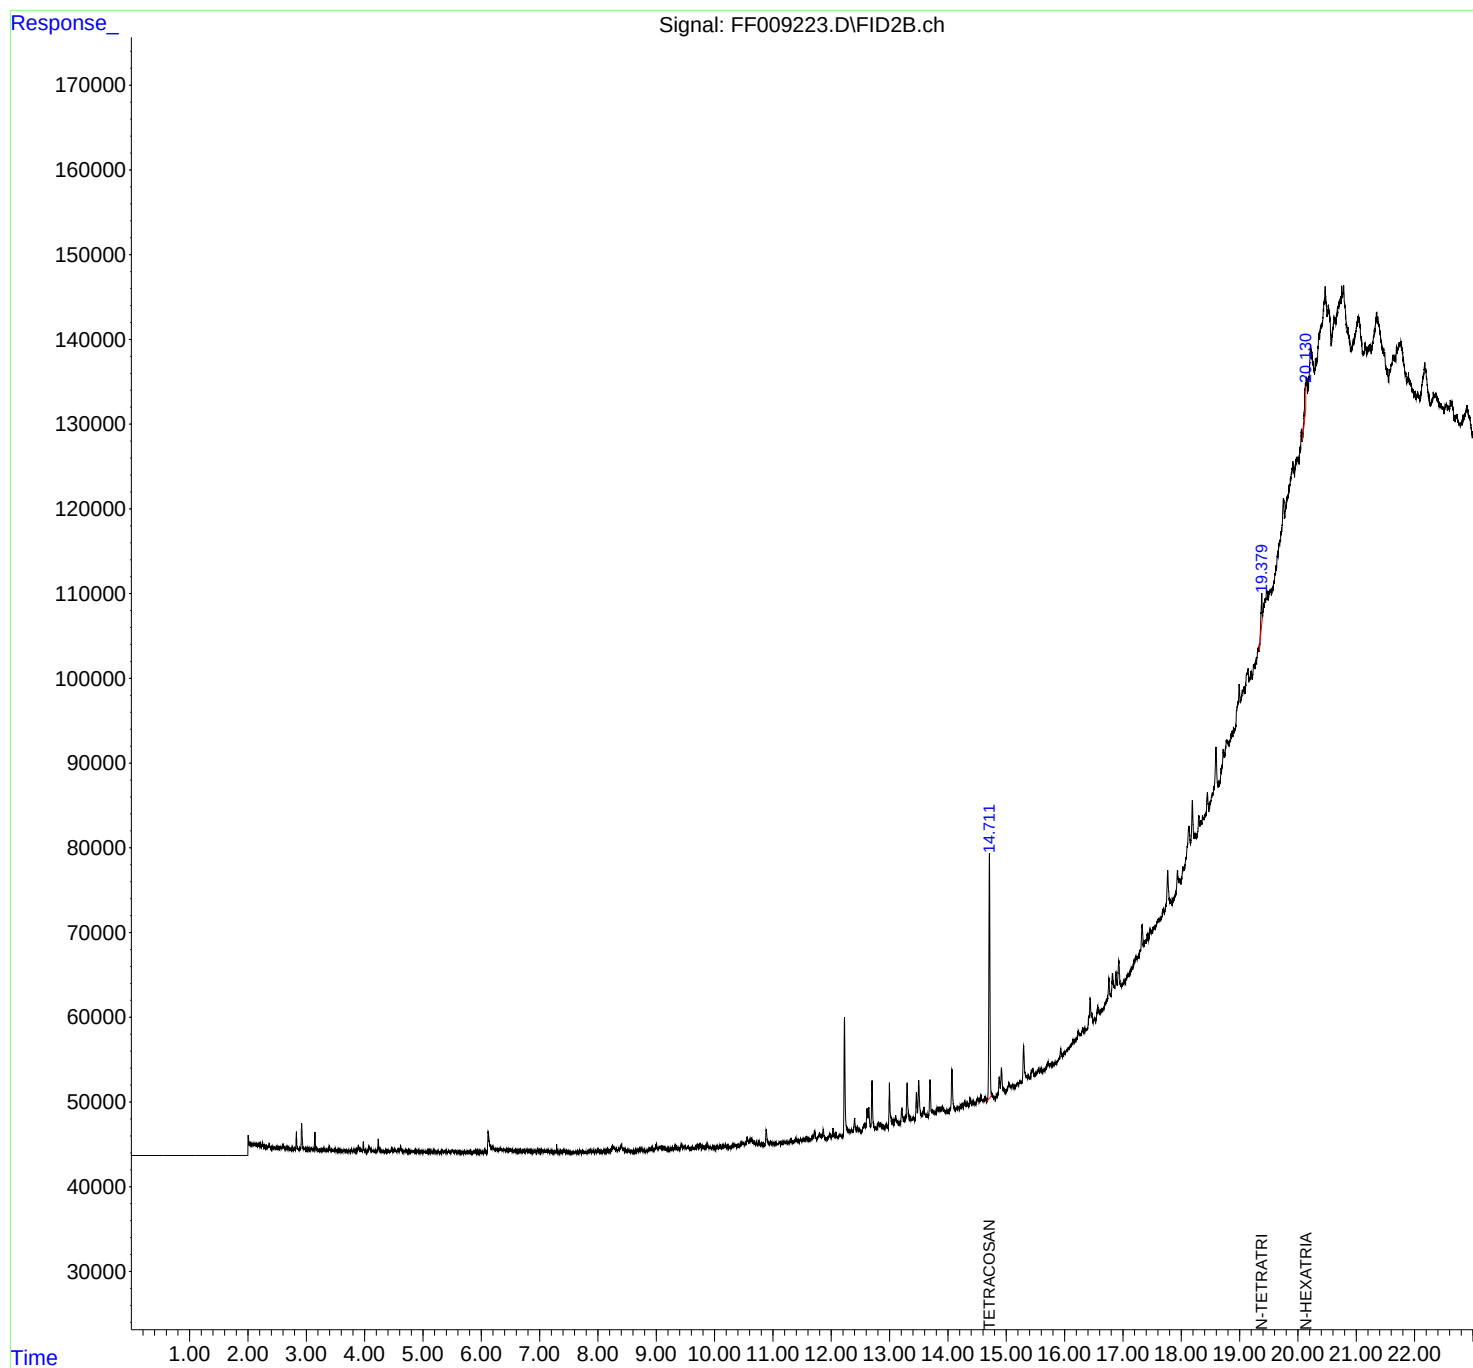


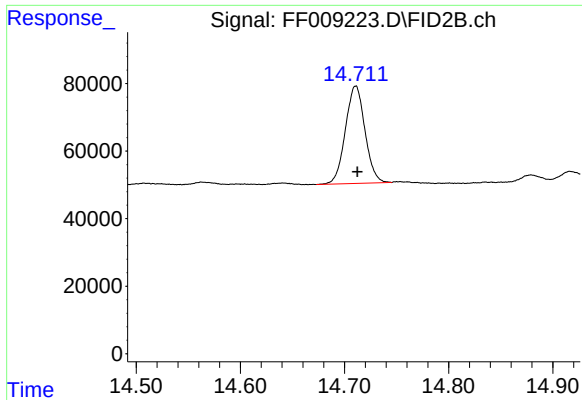

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.711 min
Delta R.T.: -0.001 min
Response: 377356
Conc: 3.44 ug/ml

Instrument :
FID_F
ClientSampleId :

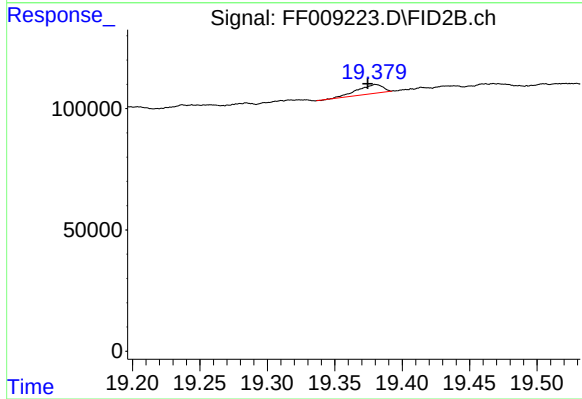

#15 N-TETRATRIACONTANE

R.T.: 19.380 min
Delta R.T.: 0.005 min
Response: 47817
Conc: 0.49 ug/ml

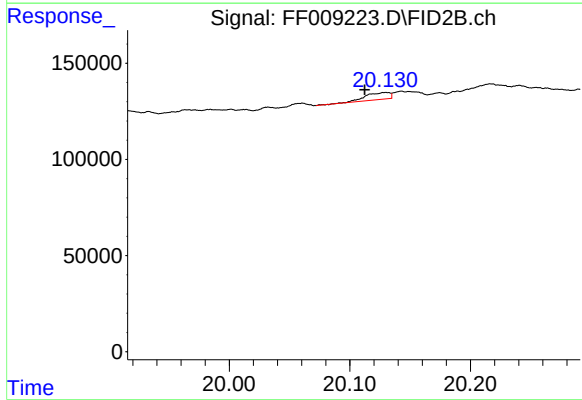

#16 N-HEXATRIACONTANE

R.T.: 20.130 min
Delta R.T.: 0.018 min
Response: 51360
Conc: 0.58 ug/ml