

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102921\
Data File : FF009220.D
Signal(s) : FID2B.ch
Acq On : 29 Oct 2021 17:06
Operator : AJ\MA
Sample : M4407-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
FDR-BH-1-20211028-5.5-6

Integration File: autoint1.e
Quant Time: Nov 01 09:57:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.711	2163719	19.732 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102921\
Data File : FF009220.D
Signal(s) : FID2B.ch
Acq On : 29 Oct 2021 17:06
Operator : AJ\MA
Sample : M4407-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
FDR-BH-1-20211028-5.5-6

Integration File: autoint1.e
Quant Time: Nov 01 09:57:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

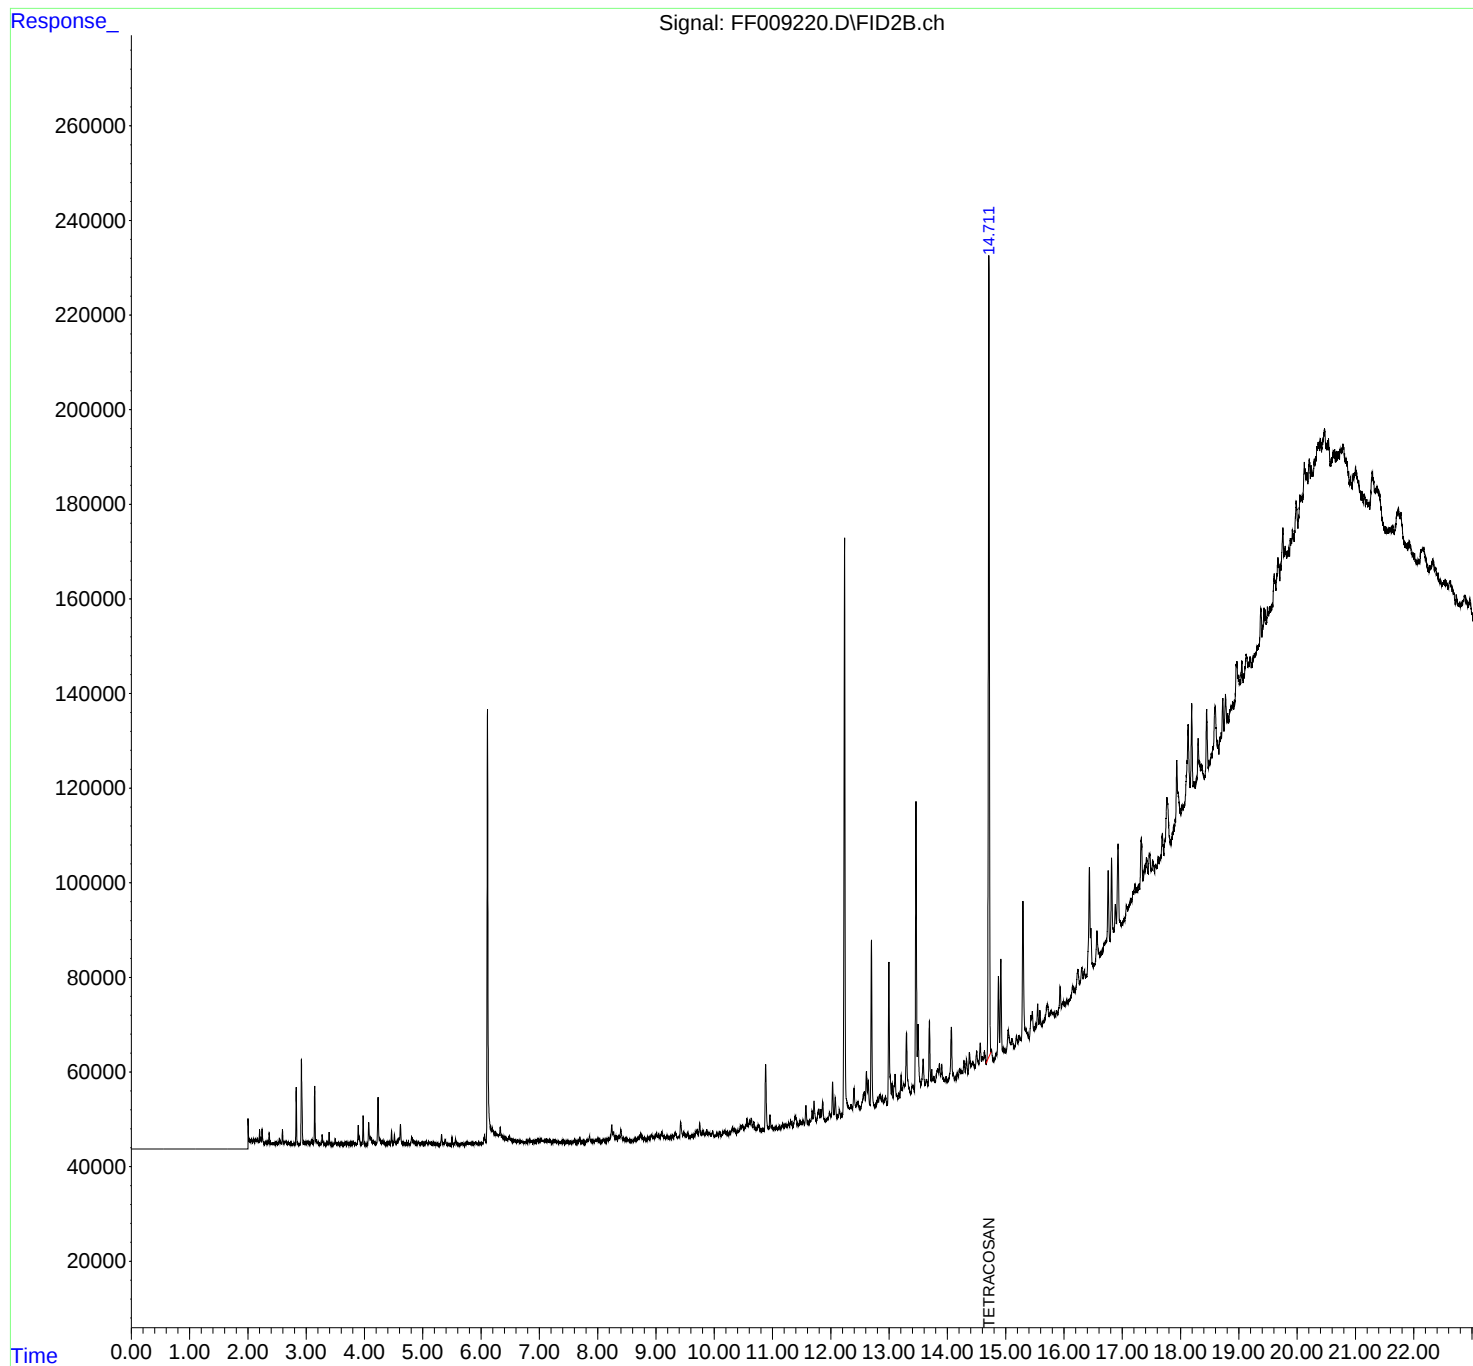

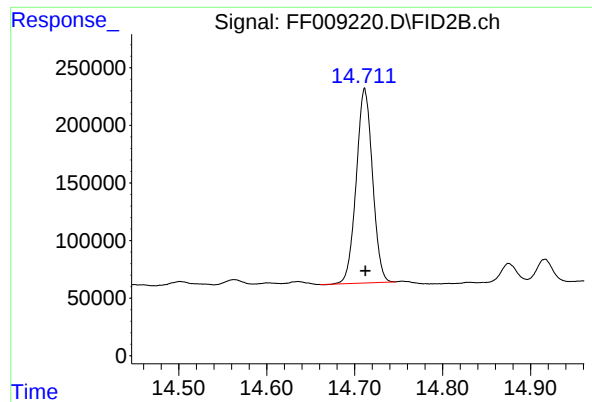

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.711 min
Delta R.T.: -0.001 min
Response: 2163719
Conc: 19.73 ug/ml

Instrument :
FID_F
ClientSampleId :
FDR-BH-1-20211028-5.5-6