

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102924\
Data File : FF014822.D
Signal(s) : FID2B.ch
Acq On : 29 Oct 2024 15:30
Operator : YP\AJ
Sample : P4595-04
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PITKIN-TPH3

Integration File: Sample.e
Quant Time: Oct 30 03:50:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102124.M
Quant Title :
QLast Update : Tue Oct 22 08:35:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.013	1146706	8.713 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF102924\
Data File : FF014822.D
Signal(s) : FID2B.ch
Acq On : 29 Oct 2024 15:30
Operator : YP\AJ
Sample : P4595-04
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
PITKIN-TPH3

Integration File: Sample.e
Quant Time: Oct 30 03:50:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102124.M
Quant Title :
QLast Update : Tue Oct 22 08:35:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

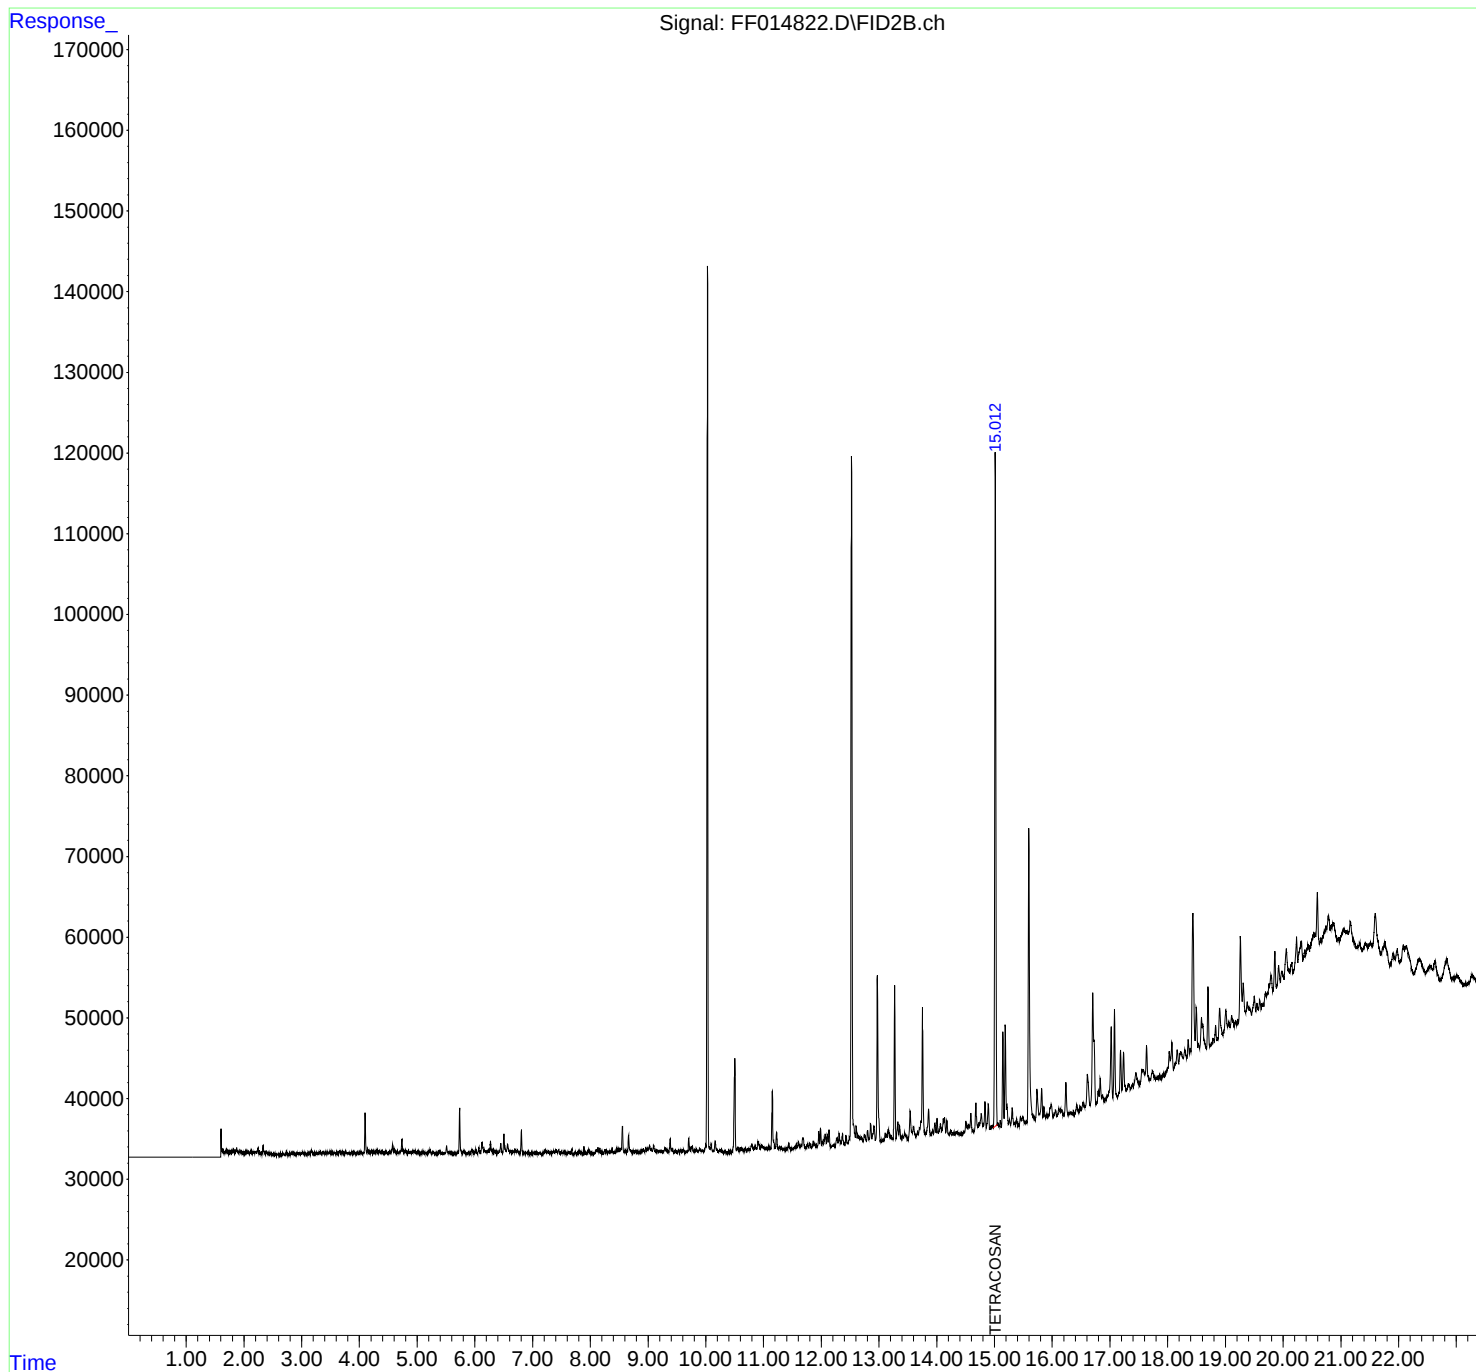

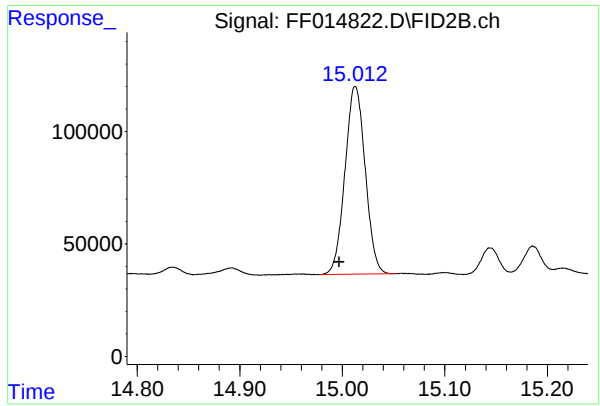

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.013 min
Delta R.T.: 0.016 min
Response: 1146706
Conc: 8.71 ug/ml

Instrument :
FID_F
ClientSampleId :
PITKIN-TPH3