

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF103025\  
Data File : FF016637.D  
Signal(s) : FID2B.ch  
Acq On : 30 Oct 2025 13:51  
Operator : YP\AJ  
Sample : Q3474-01  
Misc :  
ALS Vial : 34 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
WASTE

Manual Integrations  
APPROVED

Reviewed By :Rahul Chavli 10/31/2025  
Supervised By :Yogesh Patel 10/31/2025

Integration File: autoint1.e  
Quant Time: Oct 31 02:21:28 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF102925.M  
Quant Title :  
QLast Update : Wed Oct 29 12:48:52 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 15.057 | 1664743  | 15.934 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF103025\  
Data File : FF016637.D  
Signal(s) : FID2B.ch  
Acq On : 30 Oct 2025 13:51  
Operator : YP\AJ  
Sample : Q3474-01  
Misc :  
ALS Vial : 34 Sample Multiplier: 1


Instrument :  
FID\_F  
ClientSampleId :  
WASTE


Manual Integrations  
APPROVED

Reviewed By :Rahul Chavli 10/31/2025  
Supervised By :Yogesh Patel 10/31/2025

Integration File: autoint1.e  
Quant Time: Oct 31 02:21:28 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF102925.M  
Quant Title :  
QLast Update : Wed Oct 29 12:48:52 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

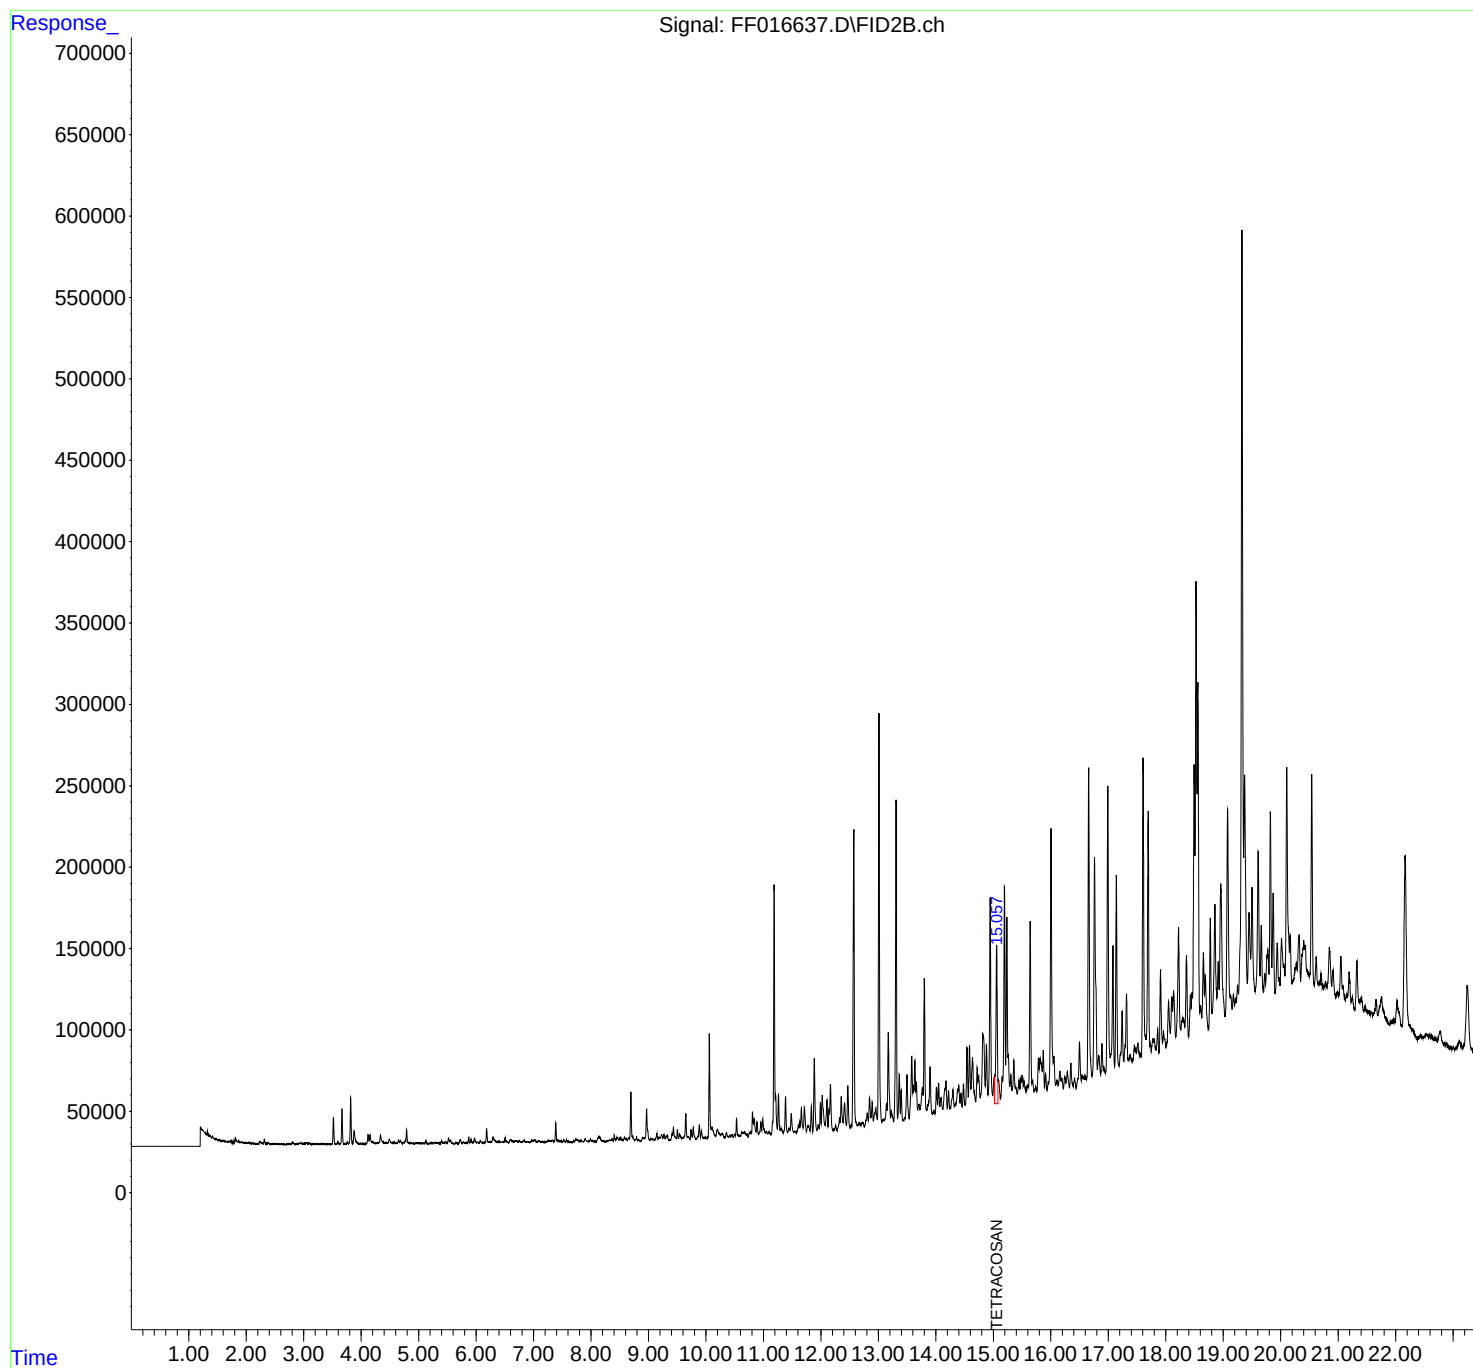

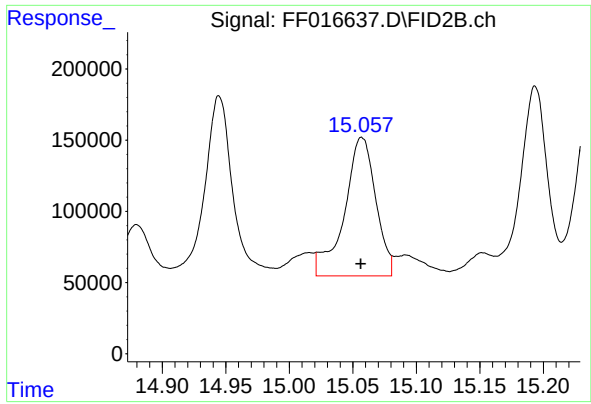

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.057 min  
Delta R.T.: 0.000 min  
Response: 1664743  
Conc: 15.93 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
WASTE

Manual Integrations  
APPROVED

Reviewed By :Rahul Chavli 10/31/2025  
Supervised By :Yogesh Patel 10/31/2025