

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF103118\
Data File : FF002535.D
Signal(s) : FID2B.ch
Acq On : 31 Oct 2018 19:56
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 01 04:41:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.652	2427052	17.462 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.720	98660	0.636 ug/ml
14) N-DOTRIACONTANE	18.556	164257	1.059 ug/ml
15) N-TETRATRIACONTANE	19.340	135449	0.920 ug/ml
16) N-HEXATRIACONTANE	20.083	54401	0.397 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF103118\
Data File : FF002535.D
Signal(s) : FID2B.ch
Acq On : 31 Oct 2018 19:56
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 01 04:41:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

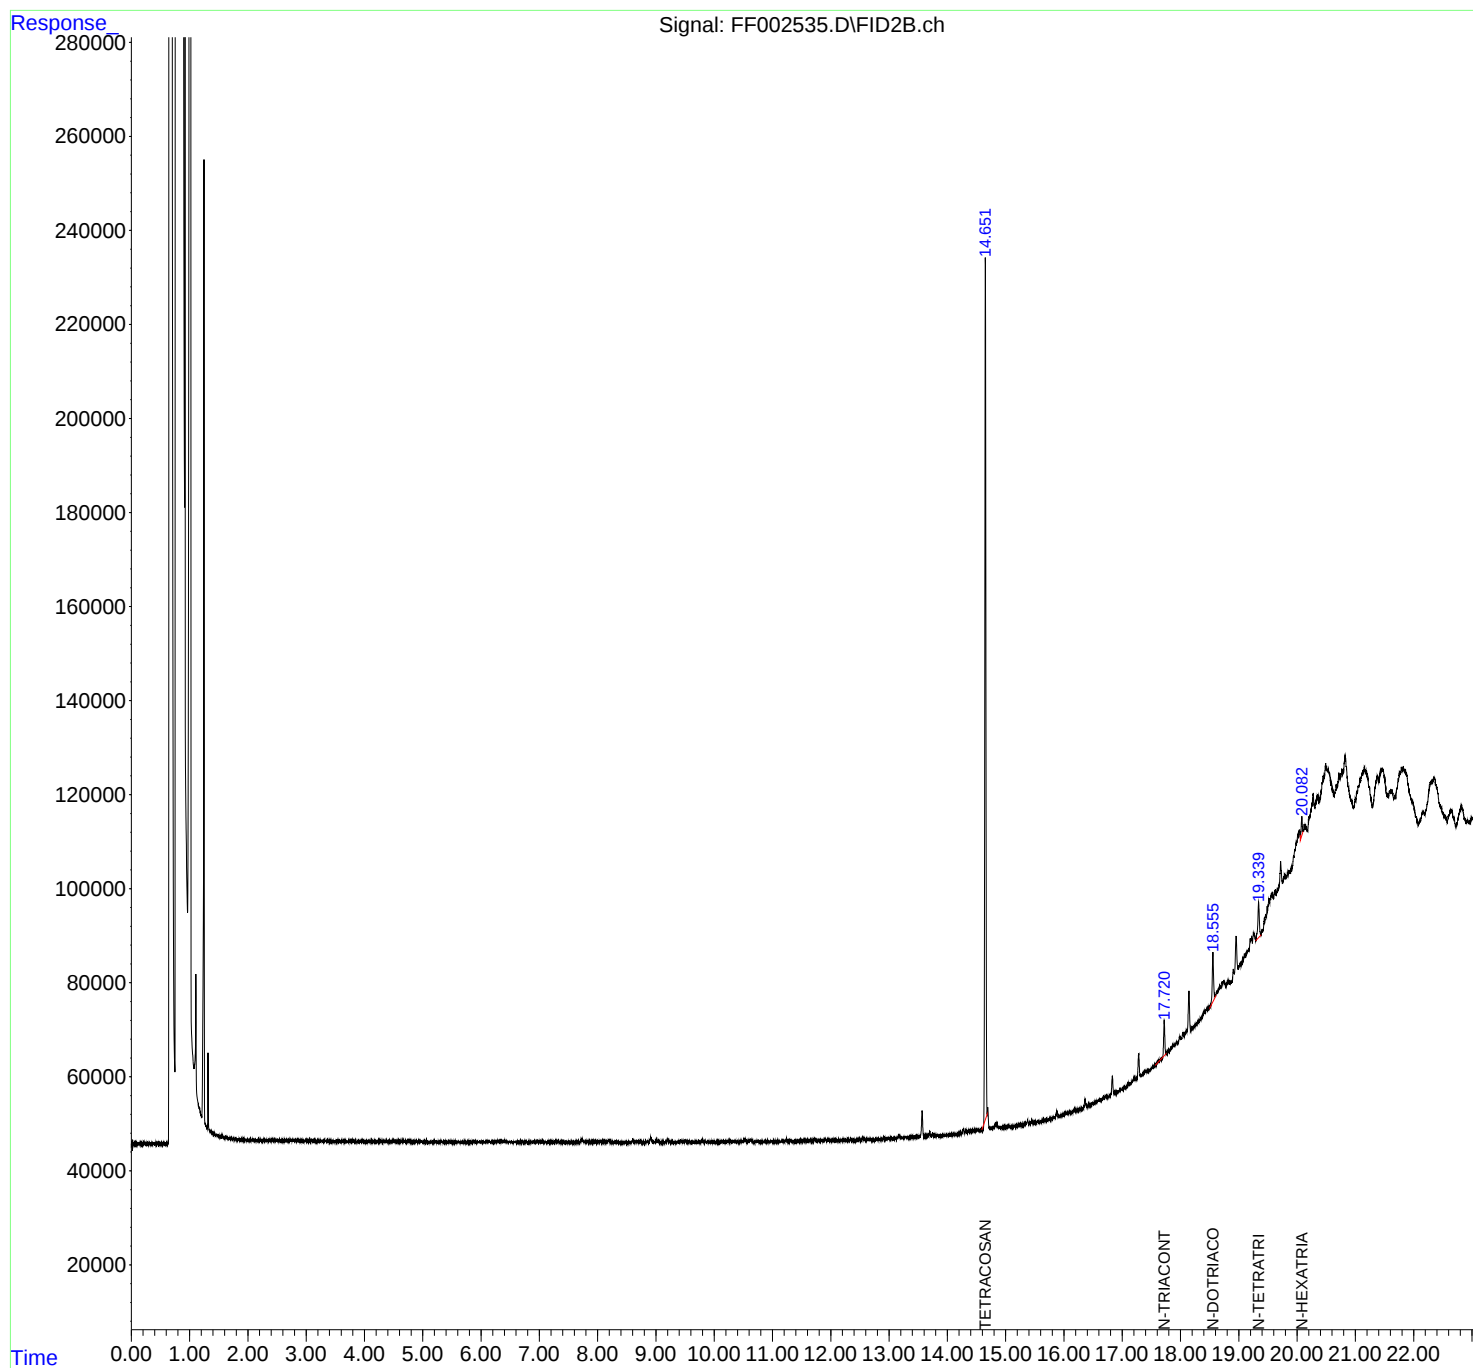

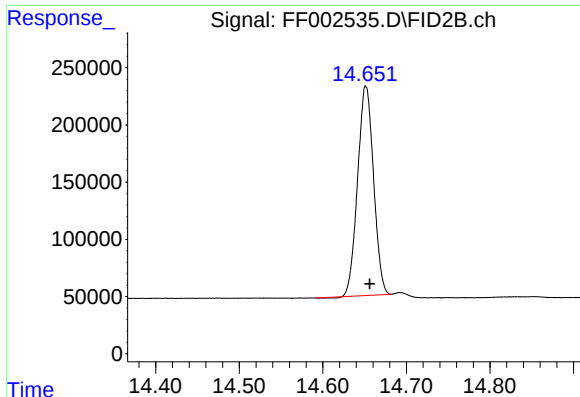


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.652 min
Delta R.T.: -0.005 min
Response: 2427052
Conc: 17.46 ug/ml

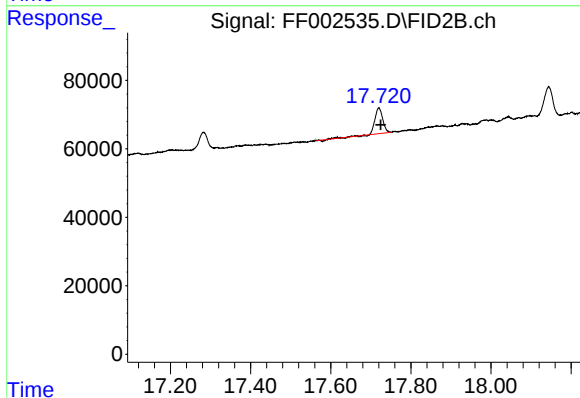


#13 N-TRIACONTANE

R.T.: 17.720 min
Delta R.T.: -0.005 min
Response: 98660
Conc: 0.64 ug/ml

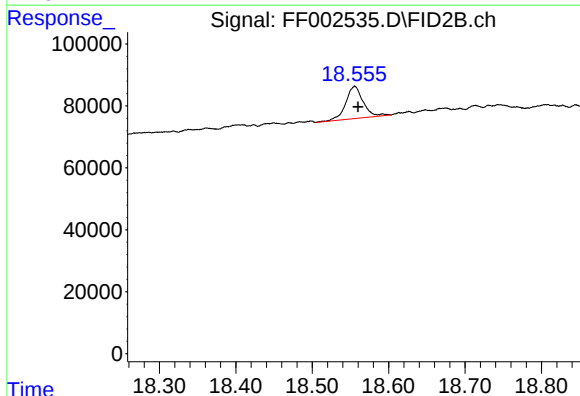


#14 N-DOTRIACONTANE

R.T.: 18.556 min
Delta R.T.: -0.004 min
Response: 164257
Conc: 1.06 ug/ml

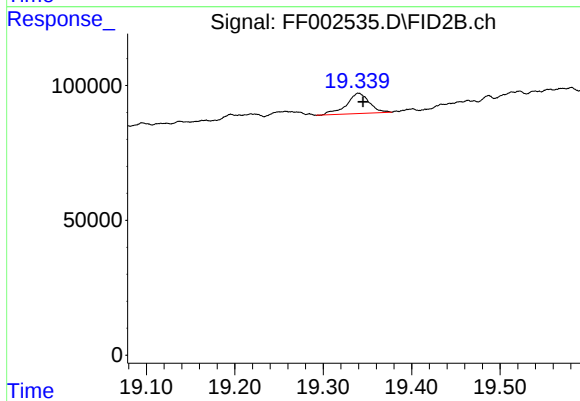

#15 N-TETRATRIACONTANE

R.T.: 19.340 min
Delta R.T.: -0.005 min
Response: 135449
Conc: 0.92 ug/ml

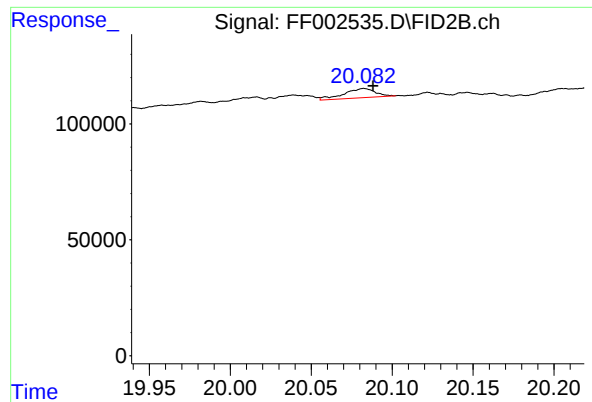

#16 N-HEXATRIACONTANE

R.T.: 20.083 min
Delta R.T.: -0.006 min
Response: 54401
Conc: 0.40 ug/ml