

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF103124\
Data File : FF014860.D
Signal(s) : FID2B.ch
Acq On : 31 Oct 2024 06:21
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Nov 01 06:30:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102124.M
Quant Title :
QLast Update : Tue Oct 22 08:35:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.013	2236953	16.998 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF103124\
Data File : FF014860.D
Signal(s) : FID2B.ch
Acq On : 31 Oct 2024 06:21
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Nov 01 06:30:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102124.M
Quant Title :
QLast Update : Tue Oct 22 08:35:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

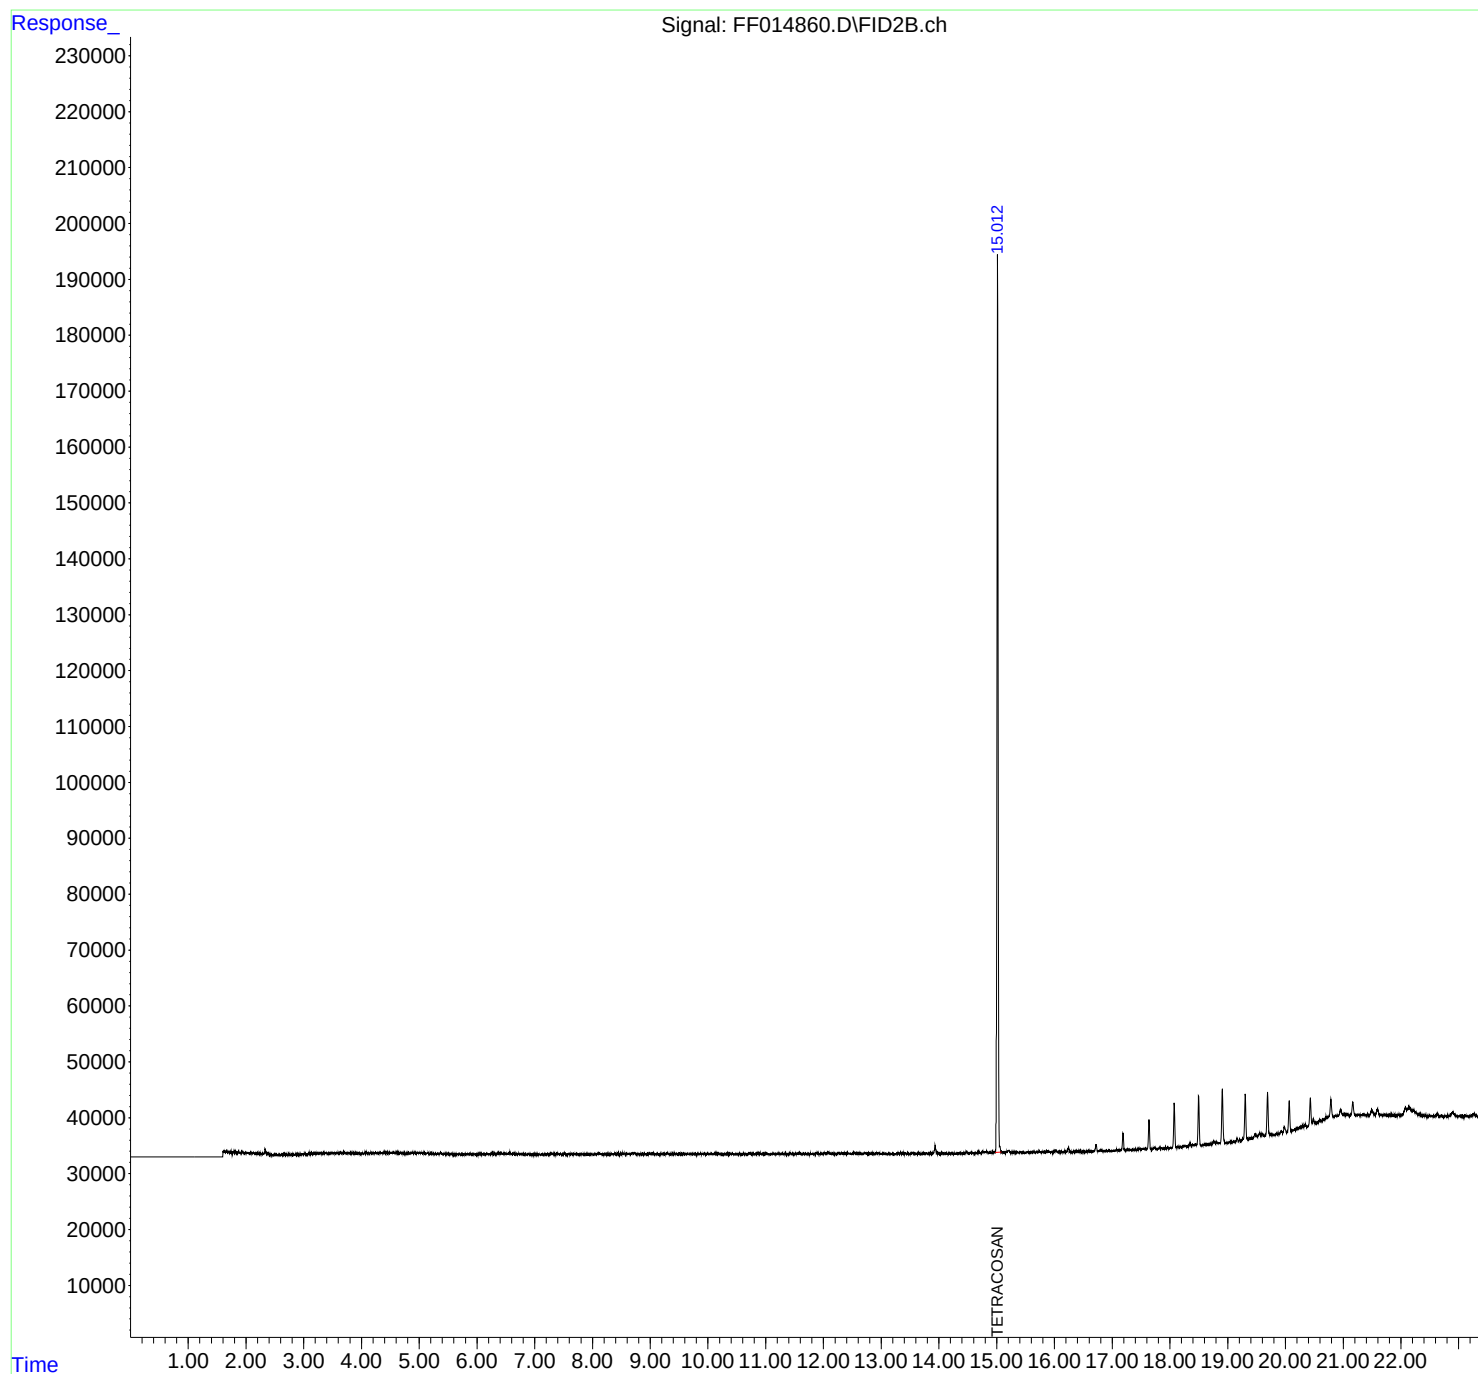

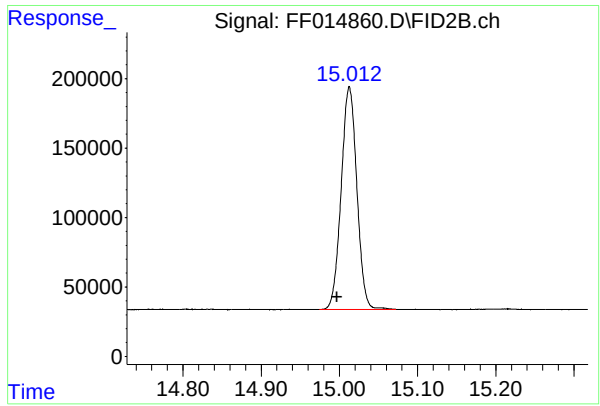

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.013 min

Delta R.T.: 0.016 min

Response: 2236953

Conc: 17.00 ug/ml

Instrument :

FID_F

ClientSampleId :

I.BLK