

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110118\
 Data File : FF002543.D
 Signal(s) : FID2B.ch
 Acq On : 01 Nov 2018 15:08
 Operator : AJ\SJ
 Sample : J5755-06
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 02 00:55:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
 Quant Title :
 QLast Update : Fri Oct 12 13:21:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.648	1099737	7.912 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.246f	341449	2.182 ug/ml
12)	N-OCTACOSANE	16.828	120252	0.775 ug/ml
13)	N-TRIACONTANE	17.717	121392	0.782 ug/ml
16)	N-HEXATRIACONTANE	20.123	91879	0.670 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110118\
Data File : FF002543.D
Signal(s) : FID2B.ch
Acq On : 01 Nov 2018 15:08
Operator : AJ\SJ
Sample : J5755-06
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 02 00:55:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

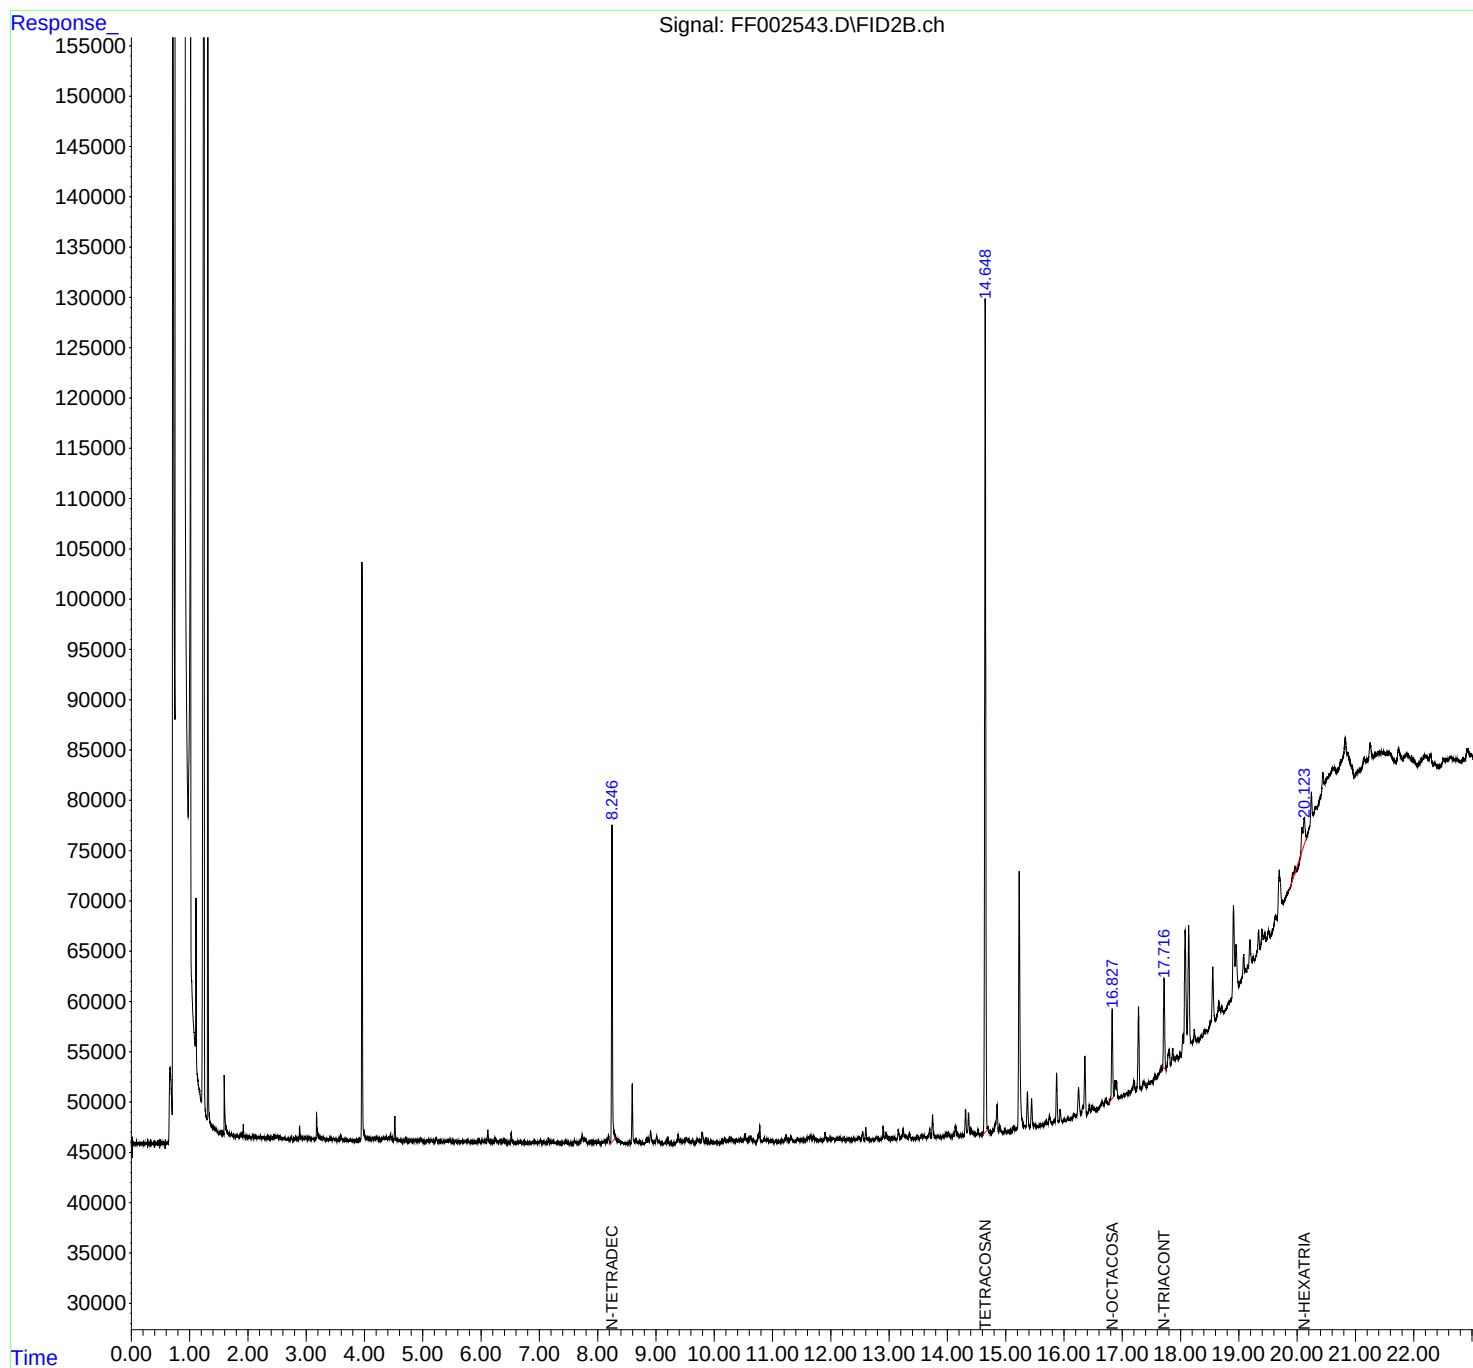

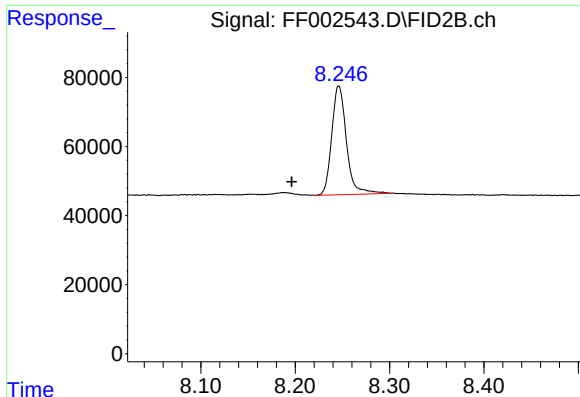


#4 N-TETRADECANE

R.T.: 8.246 min
Delta R.T.: 0.050 min
Response: 341449
Conc: 2.18 ug/ml

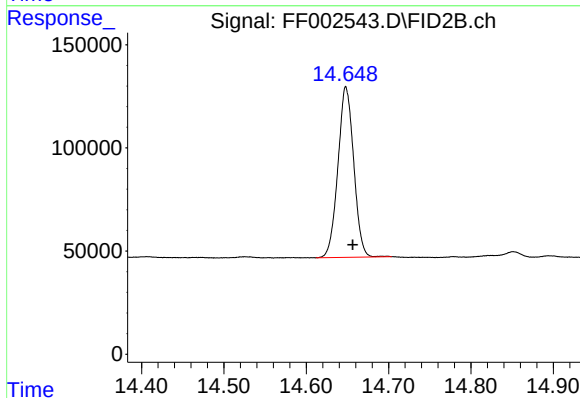


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.648 min
Delta R.T.: -0.008 min
Response: 1099737
Conc: 7.91 ug/ml

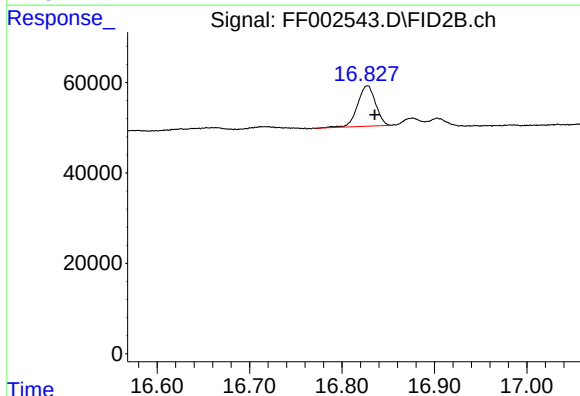


#12 N-OCTACOSANE

R.T.: 16.828 min
Delta R.T.: -0.008 min
Response: 120252
Conc: 0.78 ug/ml

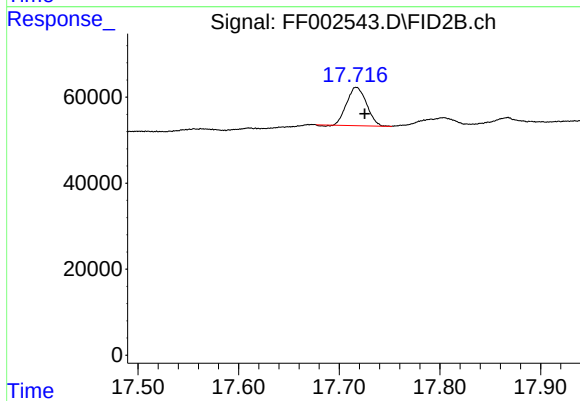

#13 N-TRIACONTANE

R.T.: 17.717 min
Delta R.T.: -0.008 min
Response: 121392
Conc: 0.78 ug/ml

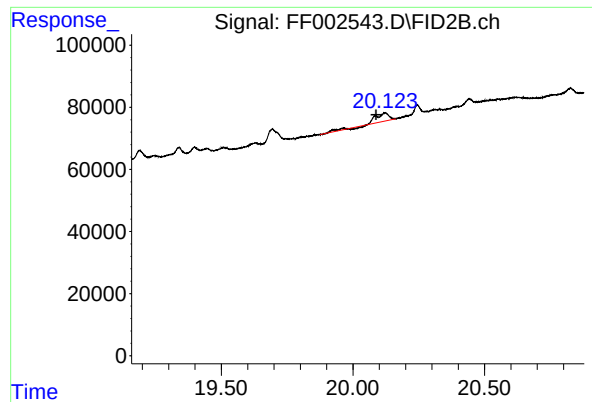

#16 N-HEXATRIACONTANE

R.T.: 20.123 min
Delta R.T.: 0.035 min
Response: 91879
Conc: 0.67 ug/ml