

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF110118\
 Data File : FF002546.D
 Signal(s) : FID2B.ch
 Acq On : 01 Nov 2018 16:39
 Operator : AJ\SJ
 Sample : J5755-01MS 5X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 02 00:55:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
 Quant Title :
 QLast Update : Fri Oct 12 13:21:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.650	685427	4.931 ug/ml
Target Compounds			
2) N-DECANE	4.377	484902	3.174 ug/ml
3) N-DODECANE	6.398	529691	3.421 ug/ml
4) N-TETRADECANE	8.191	549715	3.513 ug/ml
5) N-HEXADECANE	9.792	575352	3.661 ug/ml
6) N-OCTADECANE	11.235	518386	3.262 ug/mlm
7) N-EICOSANE	12.547	703527	4.442 ug/ml
8) N-DOCOSANE	13.748	940319	5.960 ug/ml
10) N-TETRACOSANE	14.853	600210	3.836 ug/ml
11) N-HEXACOSANE	15.877	631533	4.056 ug/ml
12) N-OCTACOSANE	16.827	915732	5.904 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF110118\
Data File : FF002546.D
Signal(s) : FID2B.ch
Acq On : 01 Nov 2018 16:39
Operator : AJ\SJ
Sample : J5755-01MS 5X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 02 00:55:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

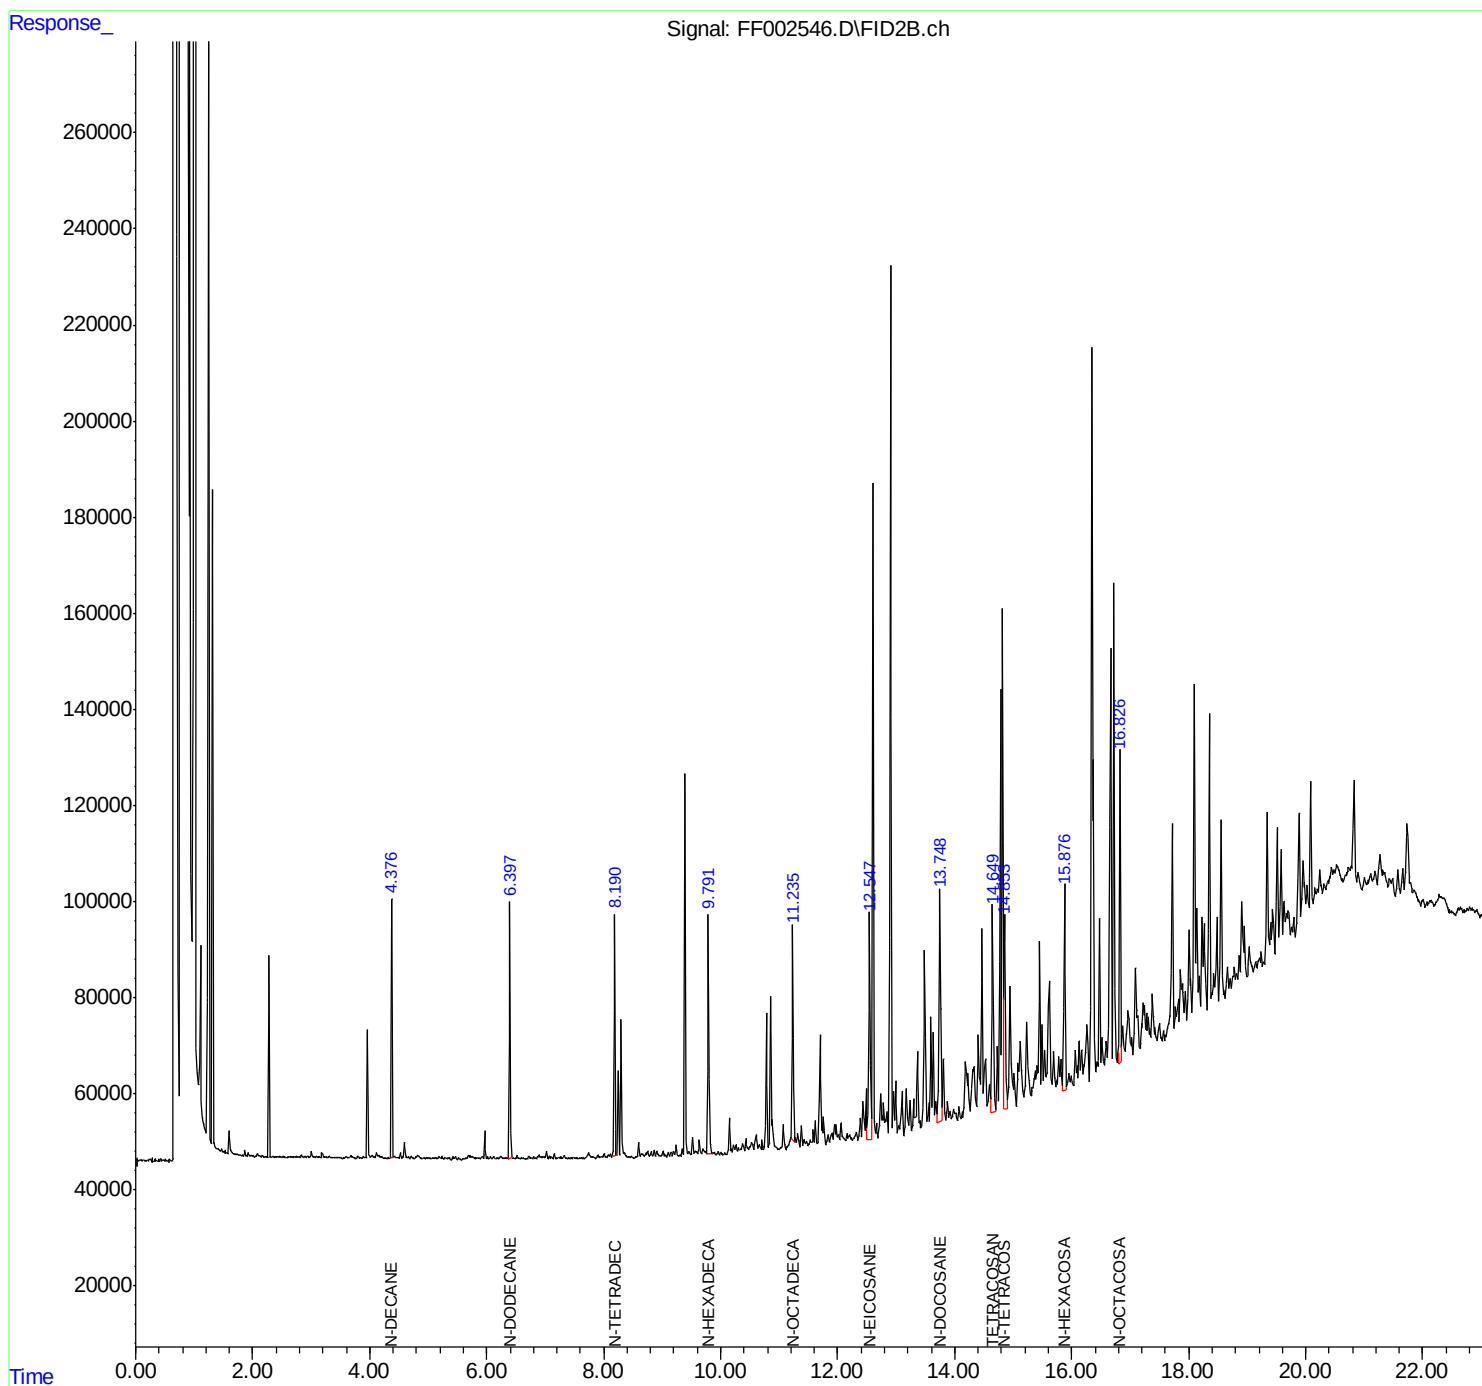

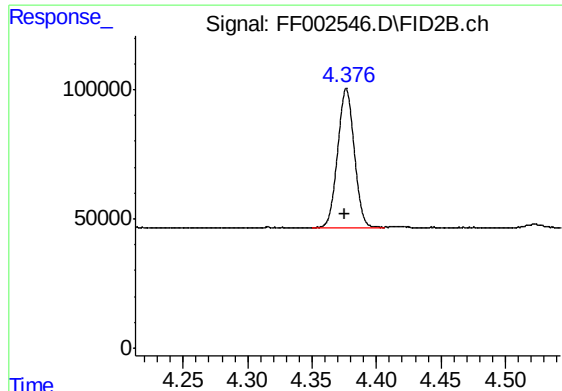


#2 N-DECANE

R.T.: 4.377 min
Delta R.T.: 0.001 min
Response: 484902
Conc: 3.17 ug/ml

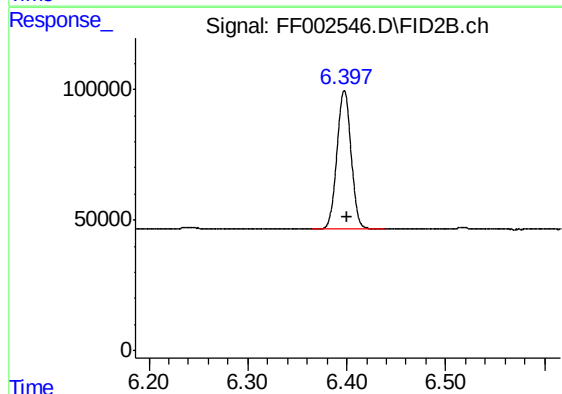


#3 N-DODECANE

R.T.: 6.398 min
Delta R.T.: -0.003 min
Response: 529691
Conc: 3.42 ug/ml

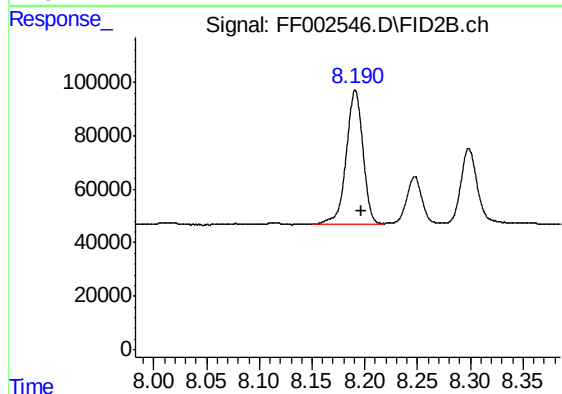


#4 N-TETRADECANE

R.T.: 8.191 min
Delta R.T.: -0.005 min
Response: 549715
Conc: 3.51 ug/ml

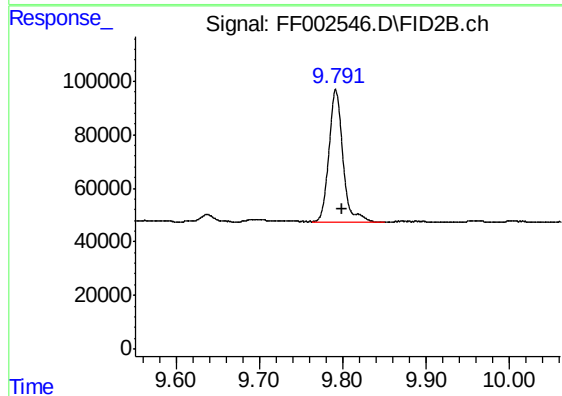


#5 N-HEXADECANE

R.T.: 9.792 min
Delta R.T.: -0.007 min
Response: 575352
Conc: 3.66 ug/ml

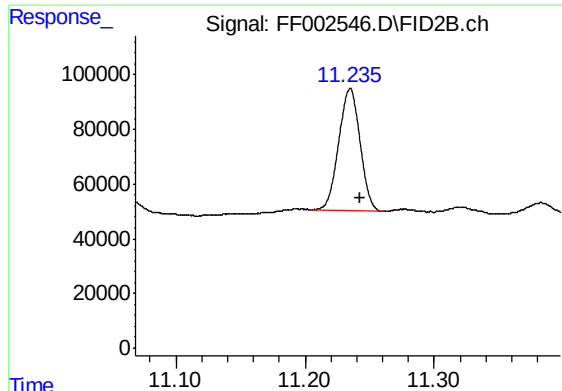


#6 N-OCTADECANE

R.T.: 11.235 min
Delta R.T.: -0.007 min
Response: 518386
Conc: 3.26 ug/ml m

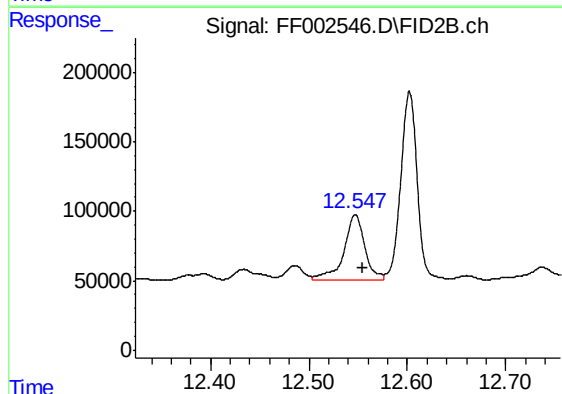


#7 N-EICOSANE

R.T.: 12.547 min
Delta R.T.: -0.007 min
Response: 703527
Conc: 4.44 ug/ml

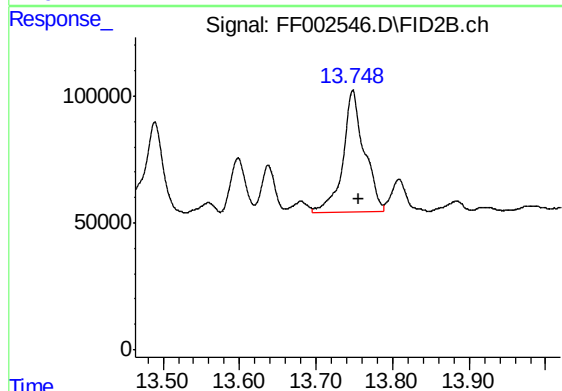


#8 N-DOCOSANE

R.T.: 13.748 min
Delta R.T.: -0.008 min
Response: 940319
Conc: 5.96 ug/ml

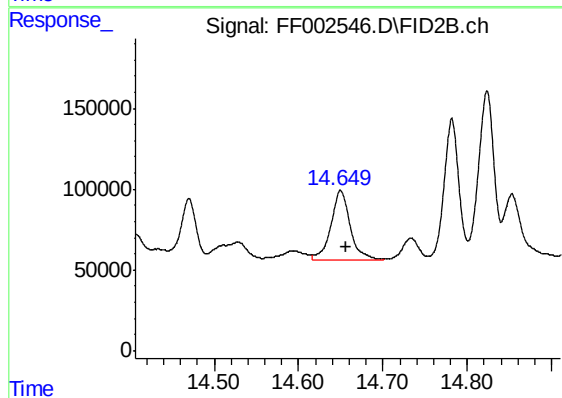


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.650 min
Delta R.T.: -0.006 min
Response: 685427
Conc: 4.93 ug/ml

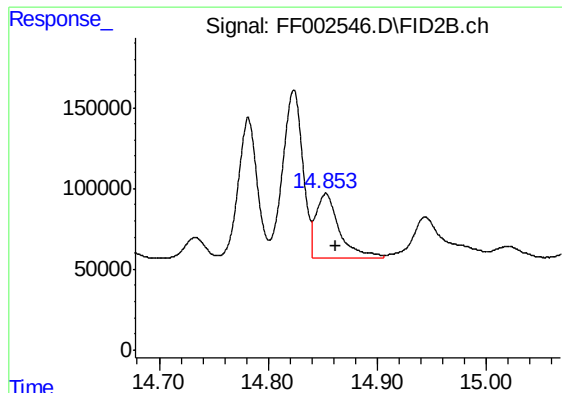


#10 N-TETRACOSANE

R.T.: 14.853 min
Delta R.T.: -0.009 min
Response: 600210
Conc: 3.84 ug/ml

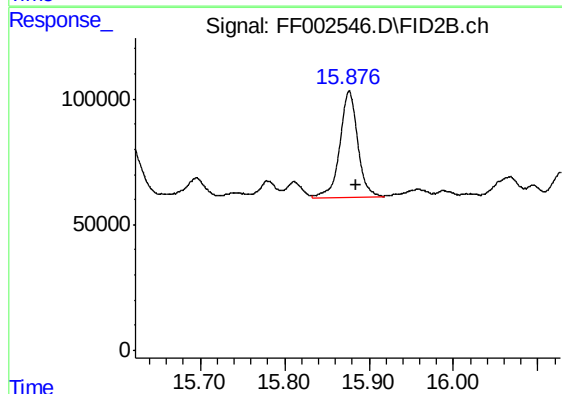

#11 N-HEXACOSANE

R.T.: 15.877 min
Delta R.T.: -0.008 min
Response: 631533
Conc: 4.06 ug/ml

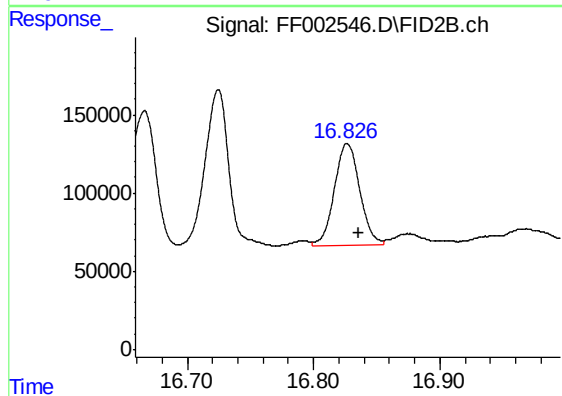

#12 N-OCTACOSANE

R.T.: 16.827 min
Delta R.T.: -0.009 min
Response: 915732
Conc: 5.90 ug/ml