

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF110118\
 Data File : FF002547.D
 Signal(s) : FID2B.ch
 Acq On : 01 Nov 2018 17:09
 Operator : AJ\SJ
 Sample : J5755-01MSD 5X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 02 00:55:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
 Quant Title :
 QLast Update : Fri Oct 12 13:21:40 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.650	737466	5.306 ug/ml
Target Compounds			
2) N-DECANE	4.376	526992	3.450 ug/ml
3) N-DODECANE	6.397	574334	3.709 ug/ml
4) N-TETRADECANE	8.190	598641	3.826 ug/ml
5) N-HEXADECANE	9.791	623614	3.968 ug/ml
6) N-OCTADECANE	11.235	560590	3.527 ug/mlm
7) N-EICOSANE	12.547	754490	4.764 ug/ml
8) N-DOCOSANE	13.748	1014747	6.432 ug/ml
10) N-TETRACOSANE	14.854	638323	4.080 ug/ml
11) N-HEXACOSANE	15.879	659601	4.236 ug/ml
12) N-OCTACOSANE	16.829	878717	5.665 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF110118\
Data File : FF002547.D
Signal(s) : FID2B.ch
Acq On : 01 Nov 2018 17:09
Operator : AJ\SJ
Sample : J5755-01MSD 5X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 02 00:55:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF101218.M
Quant Title :
QLast Update : Fri Oct 12 13:21:40 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

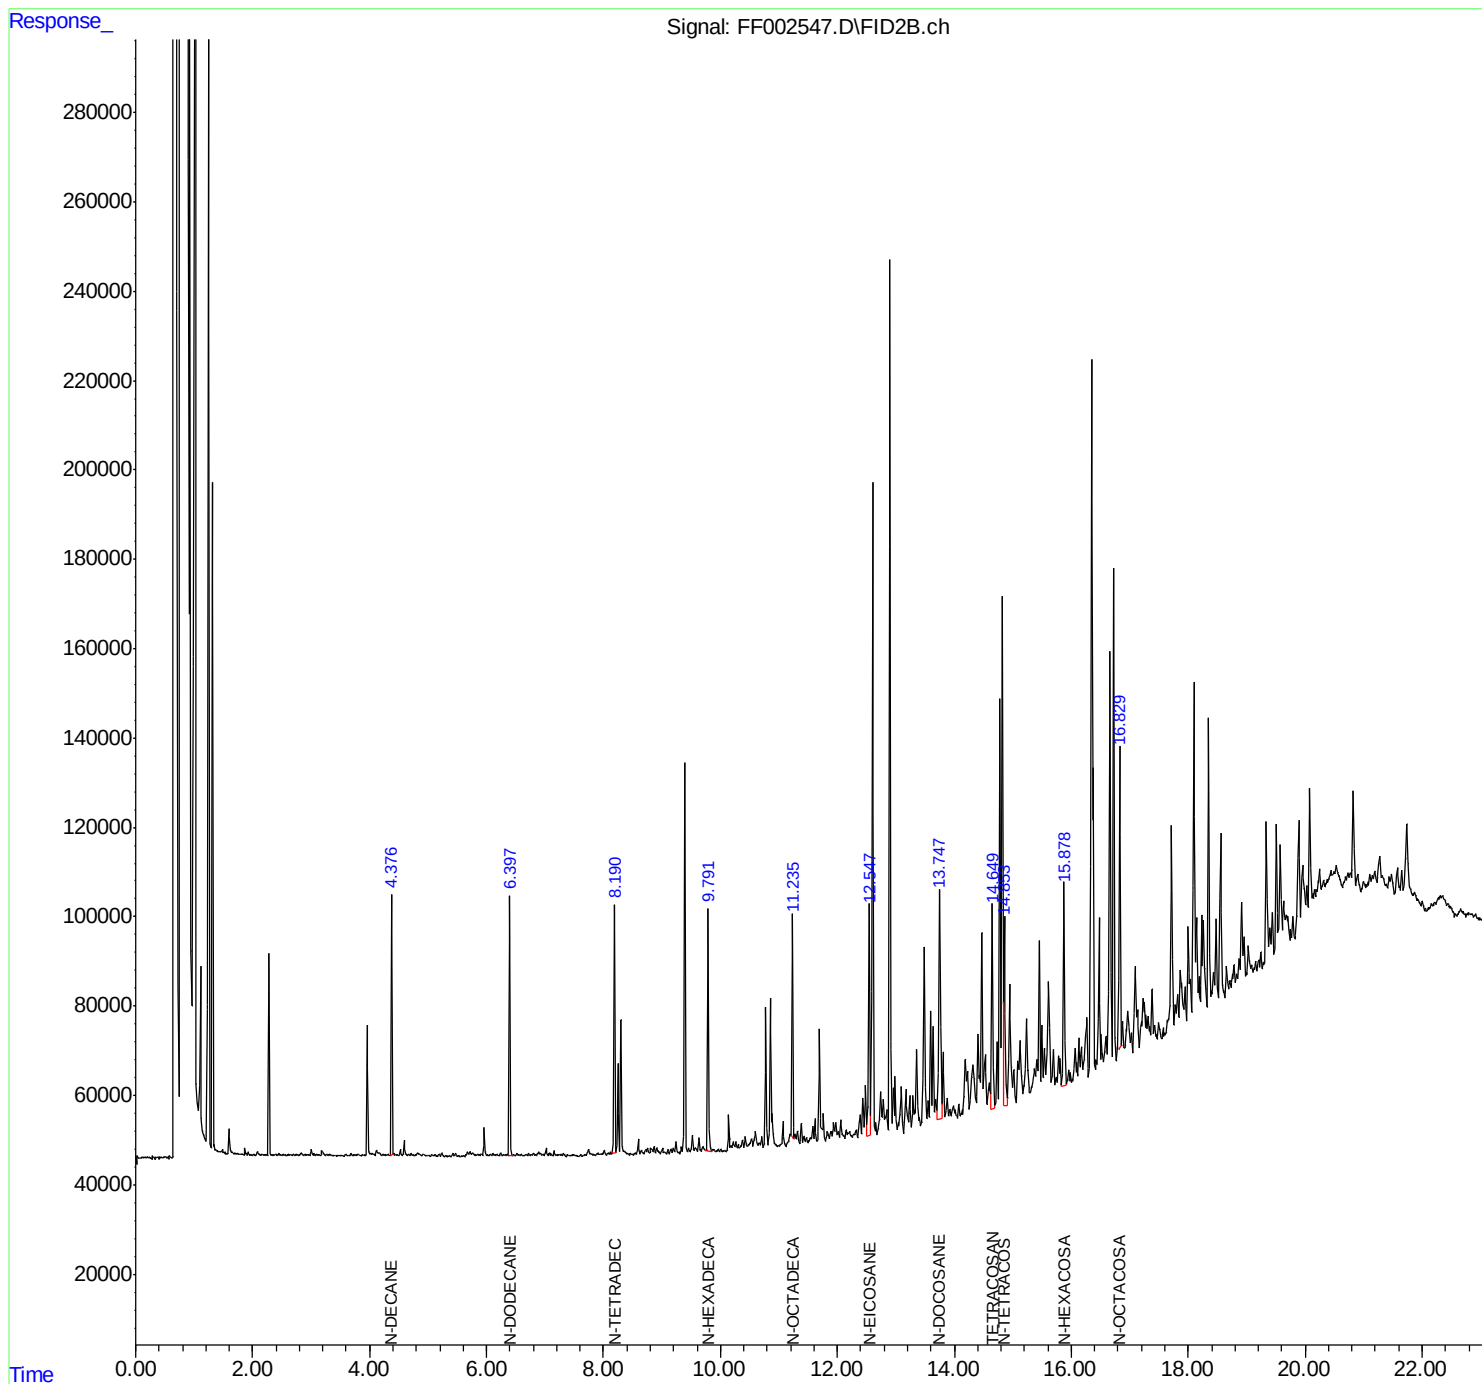

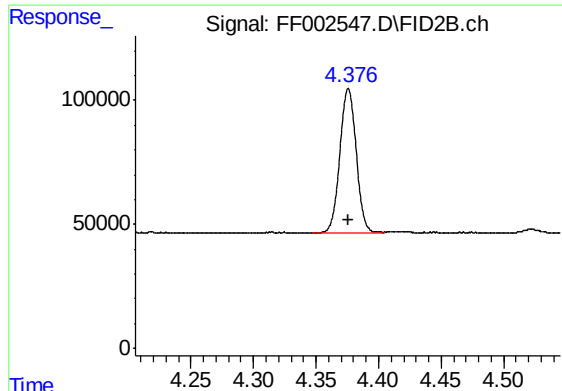


#2 N-DECANE

R.T.: 4.376 min
Delta R.T.: 0.000 min
Response: 526992
Conc: 3.45 ug/ml

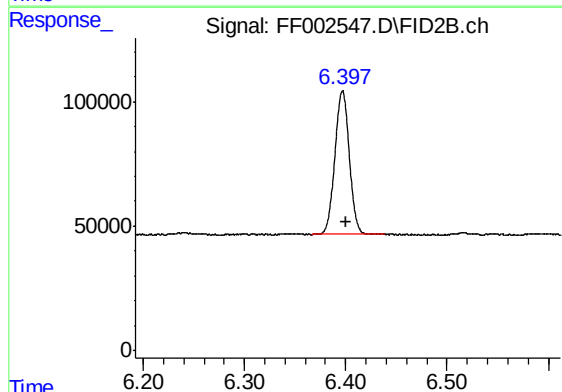


#3 N-DODECANE

R.T.: 6.397 min
Delta R.T.: -0.003 min
Response: 574334
Conc: 3.71 ug/ml

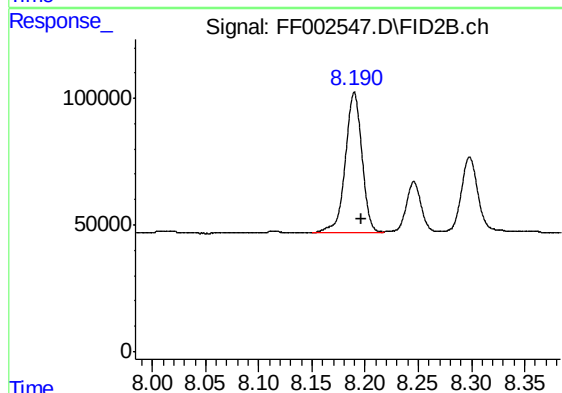


#4 N-TETRADECANE

R.T.: 8.190 min
Delta R.T.: -0.006 min
Response: 598641
Conc: 3.83 ug/ml

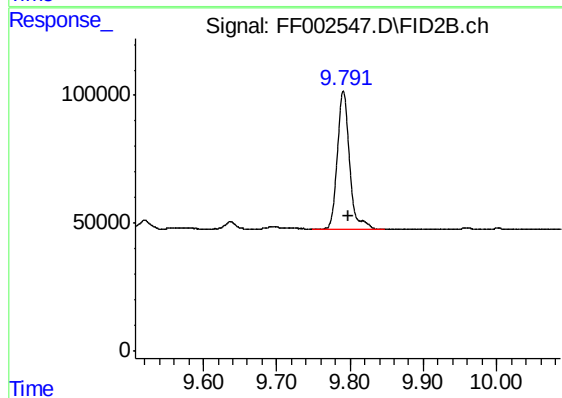


#5 N-HEXADECANE

R.T.: 9.791 min
Delta R.T.: -0.008 min
Response: 623614
Conc: 3.97 ug/ml

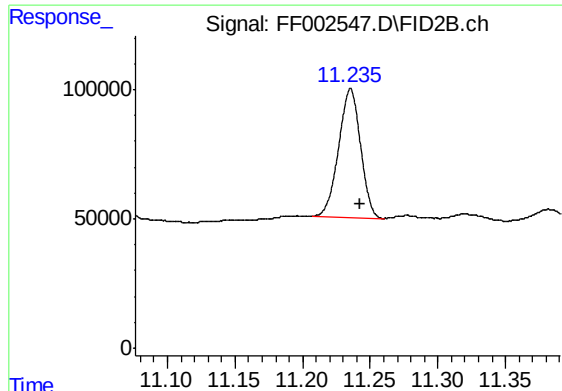


#6 N-OCTADECANE

R.T.: 11.235 min
Delta R.T.: -0.007 min
Response: 560590
Conc: 3.53 ug/ml m

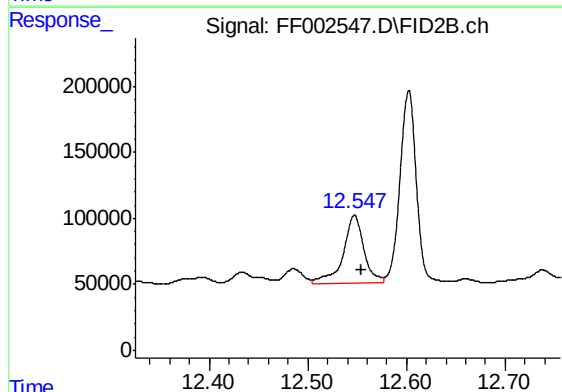


#7 N-EICOSANE

R.T.: 12.547 min
Delta R.T.: -0.007 min
Response: 754490
Conc: 4.76 ug/ml

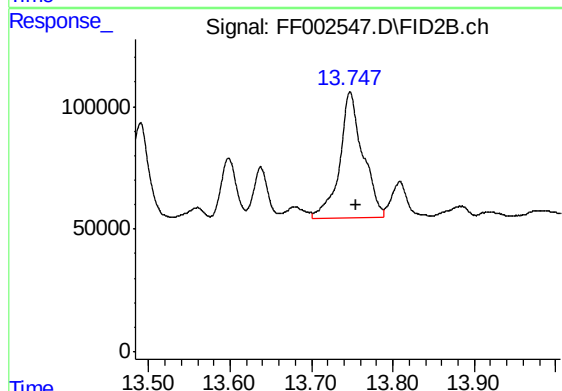


#8 N-DOCOSANE

R.T.: 13.748 min
Delta R.T.: -0.008 min
Response: 1014747
Conc: 6.43 ug/ml

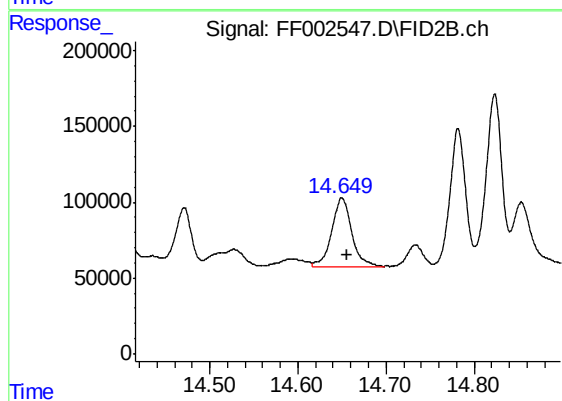


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.650 min
Delta R.T.: -0.006 min
Response: 737466
Conc: 5.31 ug/ml

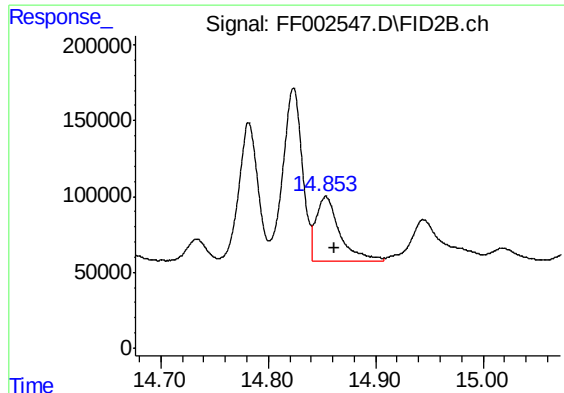


#10 N-TETRACOSANE

R.T.: 14.854 min
Delta R.T.: -0.008 min
Response: 638323
Conc: 4.08 ug/ml

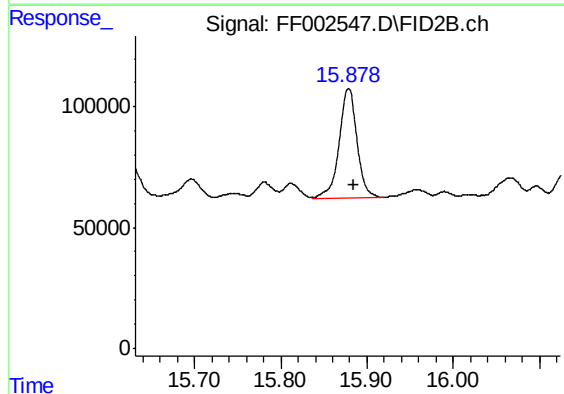

#11 N-HEXACOSANE

R.T.: 15.879 min
Delta R.T.: -0.006 min
Response: 659601
Conc: 4.24 ug/ml

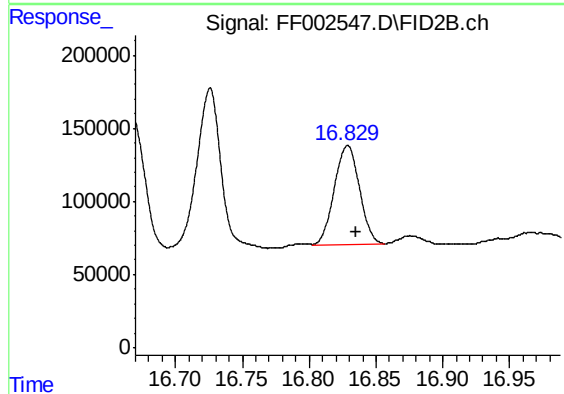

#12 N-OCTACOSANE

R.T.: 16.829 min
Delta R.T.: -0.007 min
Response: 878717
Conc: 5.66 ug/ml m