

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110121\
 Data File : FF009244.D
 Signal(s) : FID2B.ch
 Acq On : 01 Nov 2021 22:08
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 02 01:14:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
 Quant Title :
 QLast Update : Fri Oct 08 02:25:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.712	1713441	15.626 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.596	26273	0.249 ug/ml
18) N-TETRACONTANE	21.745	256037	3.152 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF110121\
Data File : FF009244.D
Signal(s) : FID2B.ch
Acq On : 01 Nov 2021 22:08
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 02 01:14:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF100721.M
Quant Title :
QLast Update : Fri Oct 08 02:25:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

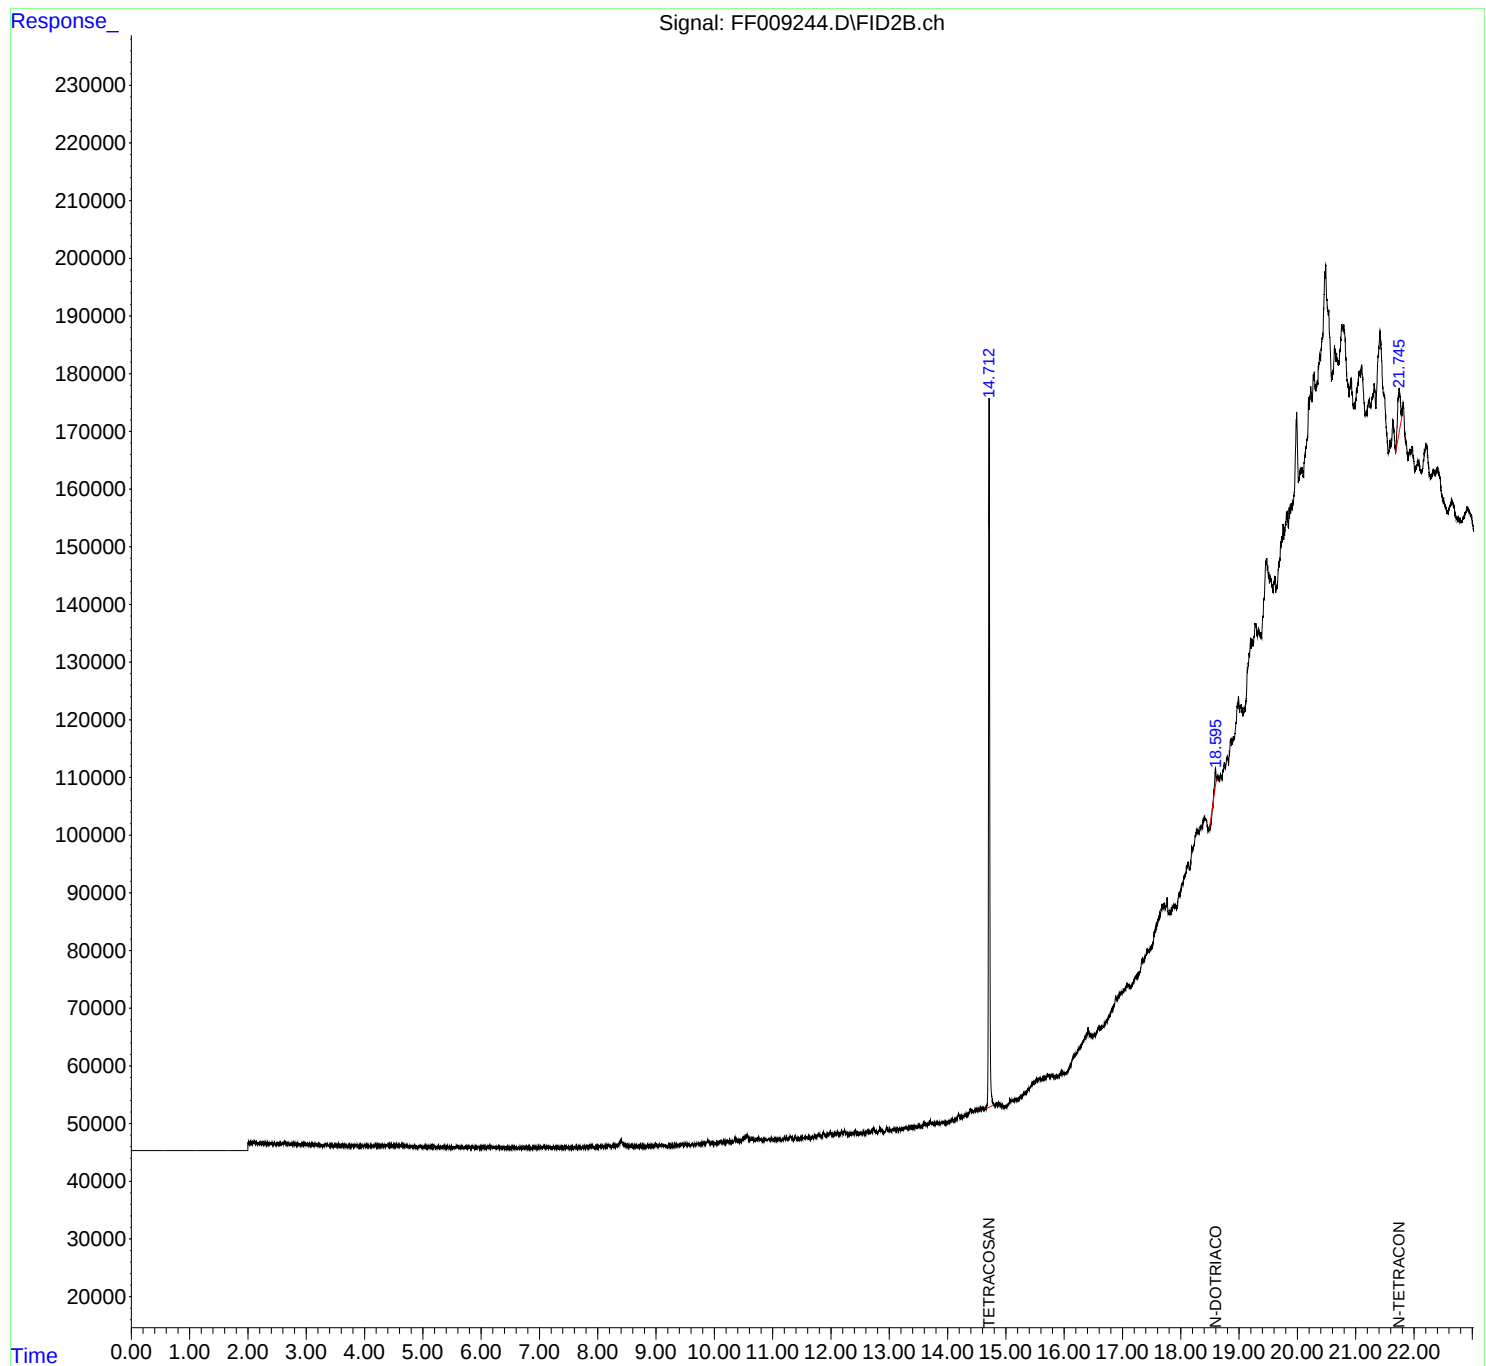


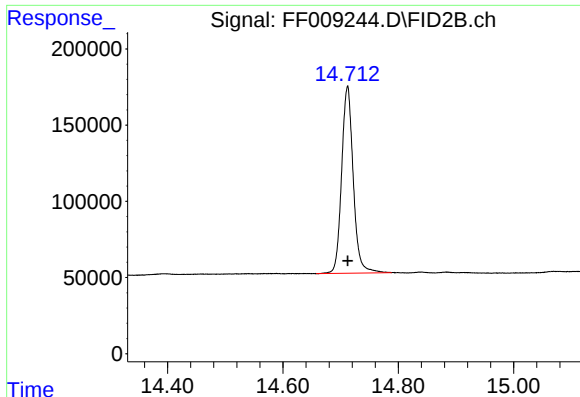

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.712 min
Delta R.T.: 0.000 min
Response: 1713441
Conc: 15.63 ug/ml

Instrument :
FID_F
ClientSampleId :

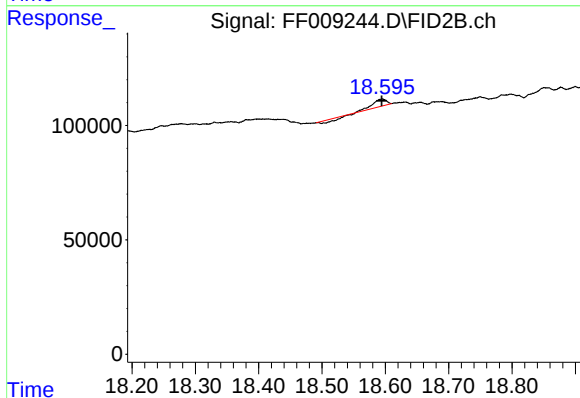

#14 N-DOTRIACONTANE

R.T.: 18.596 min
Delta R.T.: 0.001 min
Response: 26273
Conc: 0.25 ug/ml

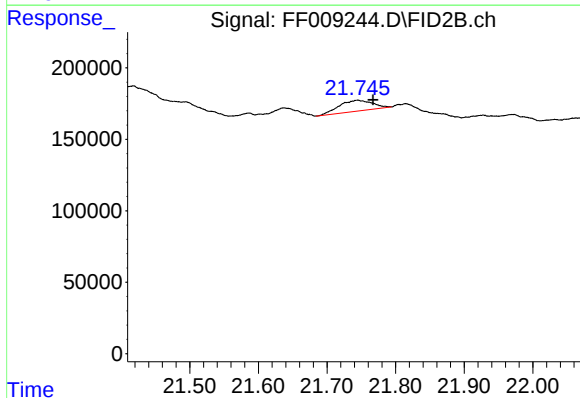

#18 N-TETRACONTANE

R.T.: 21.745 min
Delta R.T.: -0.022 min
Response: 256037
Conc: 3.15 ug/ml